

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
 Data File : FB027555.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2022 1:20
 Operator : AJ/MA
 Sample : N3494-09 50X
 Misc : 5.09G/5.00 ML MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 28 04:28:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	275980	24.604 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	20297	1.205 ng/ml
3) t n-Heptane	7.748	16584	0.947 ng/ml
4) t Benzene	7.918	12477	0.612 ng/ml
6) t Toluene	10.619	5823	0.301 ng/ml
8) t m-Xylene	13.187	19811	1.111 ng/ml
9) t O-Xylene	13.928	6274	0.361 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	5078	0.296 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
Data File : FB027555.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2022 1:20
Operator : AJ/MA
Sample : N3494-09 50X
Misc : 5.09G/5.00 ML MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 28 04:28:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

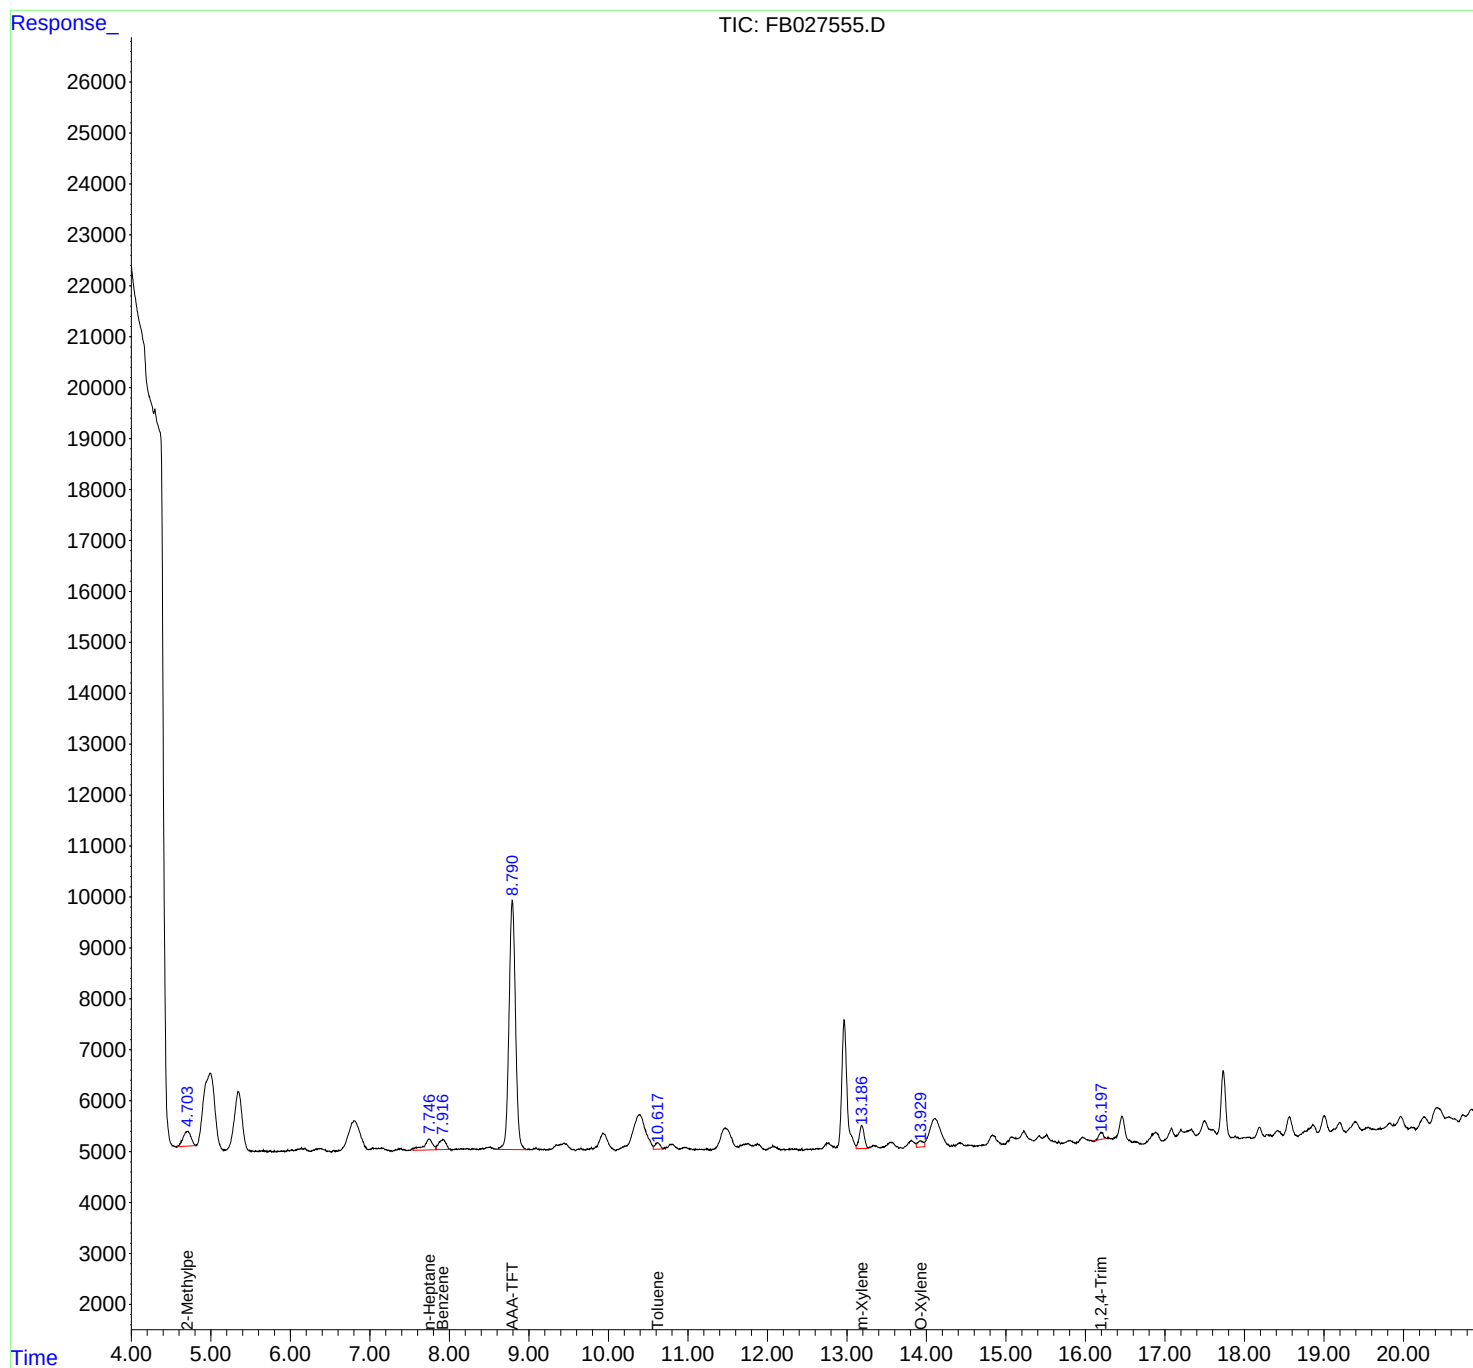


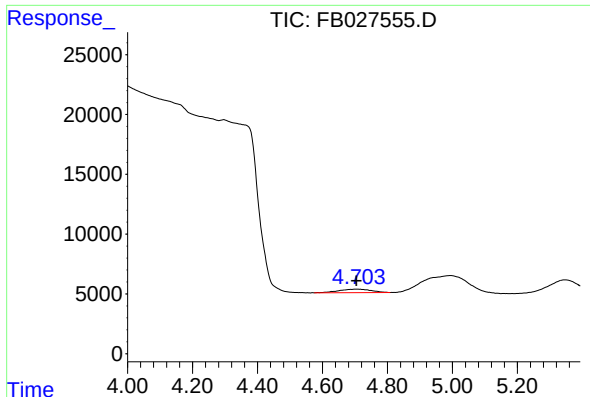

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: 0.004 min
Response: 20297
Conc: 1.20 ng/ml

Instrument :
FID_B
ClientSampleId :

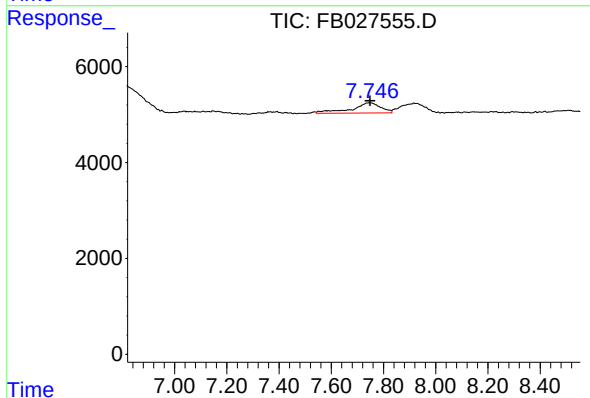


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.002 min
Response: 16584
Conc: 0.95 ng/ml

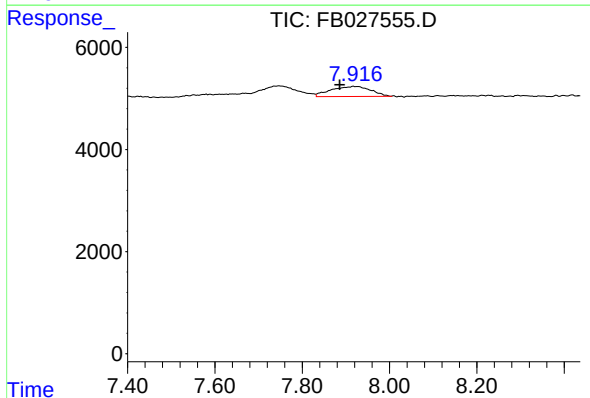


#4 Benzene

R.T.: 7.918 min
Delta R.T.: 0.032 min
Response: 12477
Conc: 0.61 ng/ml

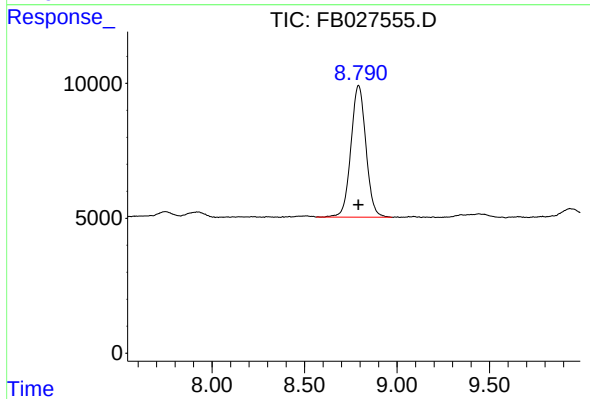

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.001 min
Response: 275980
Conc: 24.60 ng/ml

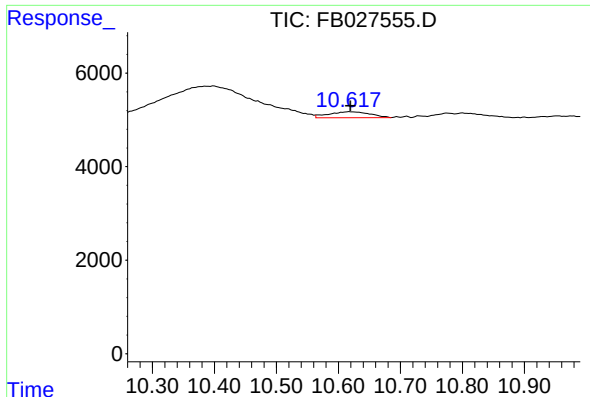

#6 Toluene


R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 5823
Conc: 0.30 ng/ml

Instrument :
FID_B
ClientSampleId :

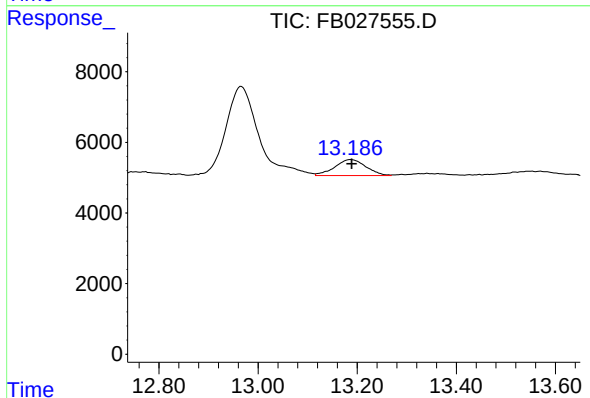


#8 m-Xylene

R.T.: 13.187 min
Delta R.T.: -0.002 min
Response: 19811
Conc: 1.11 ng/ml

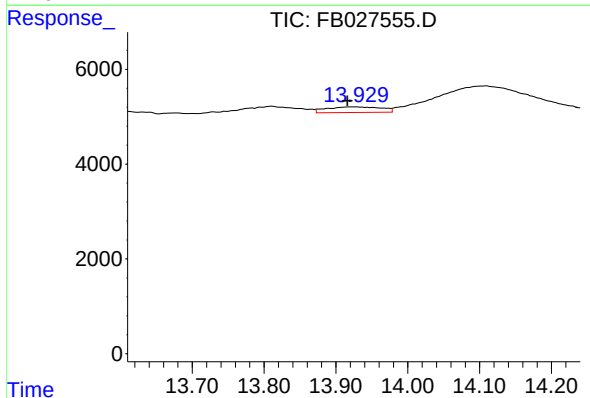

#9 o-Xylene

R.T.: 13.928 min
Delta R.T.: 0.012 min
Response: 6274
Conc: 0.36 ng/ml

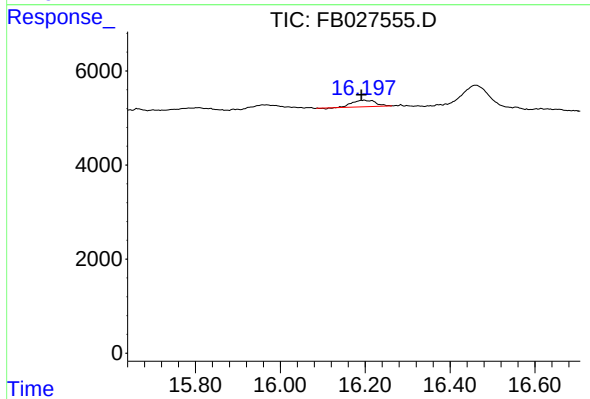

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.007 min
Response: 5078
Conc: 0.30 ng/ml