

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
 Data File : FB027556.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2022 1:56
 Operator : AJ/MA
 Sample : N3494-14 50X
 Misc : 5.07G/5.00 ML MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 28 04:28:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	320703	28.592 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	43374	2.575 ng/ml
2) t 2,2,4-Trimethylpentane	7.483	132902	7.569 ng/ml
3) t n-Heptane	7.743	143601	8.197 ng/ml
4) t Benzene	7.873	43178	2.117 ng/ml
7) t Ethylbenzene	13.015	2735110	151.033 ng/ml
9) t O-Xylene	13.937	531113	30.566 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	166096	9.669 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
Data File : FB027556.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2022 1:56
Operator : AJ/MA
Sample : N3494-14 50X
Misc : 5.07G/5.00 ML MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 28 04:28:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

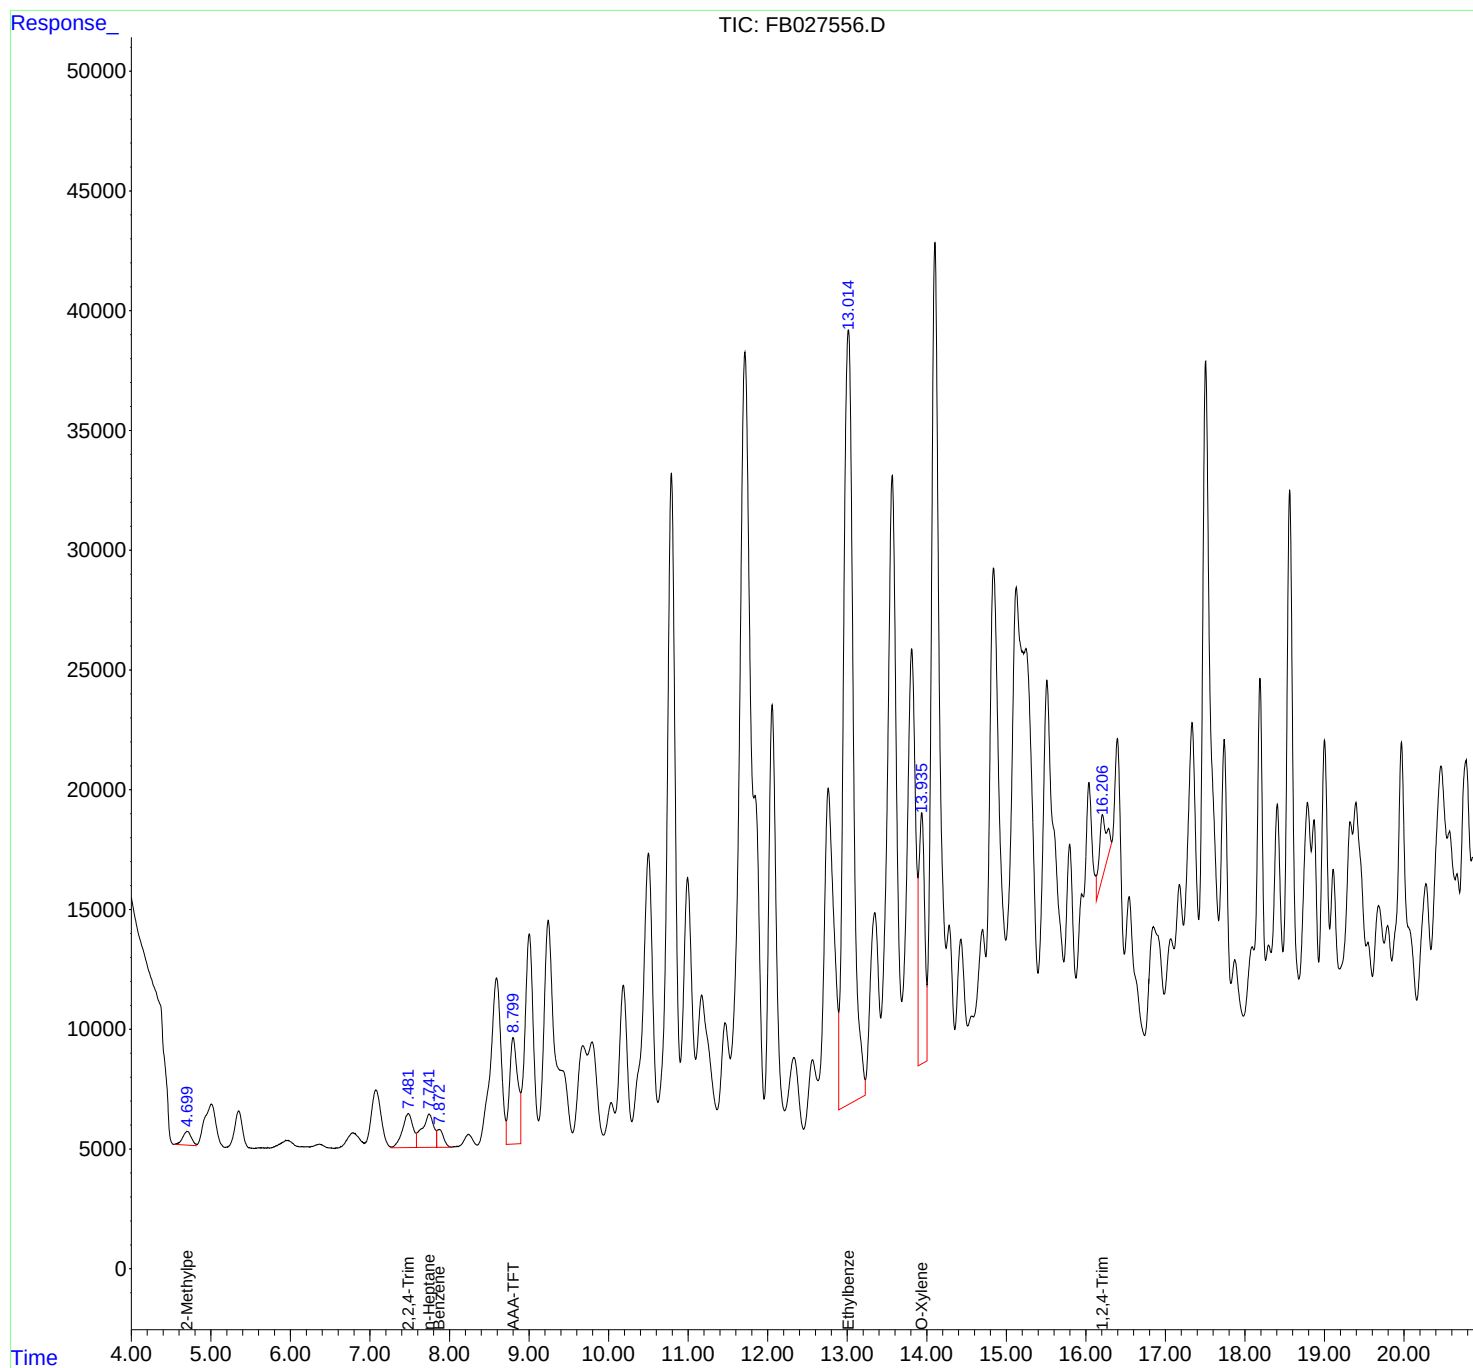


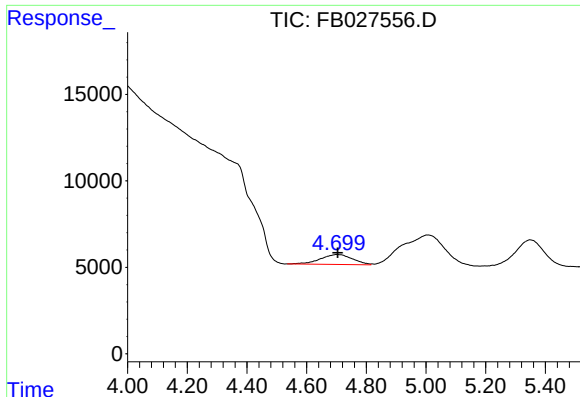

#1 2-Methylpentane


R.T.: 4.701 min
Delta R.T.: -0.003 min
Response: 43374
Conc: 2.57 ng/ml

Instrument :
FID_B
ClientSampleId :

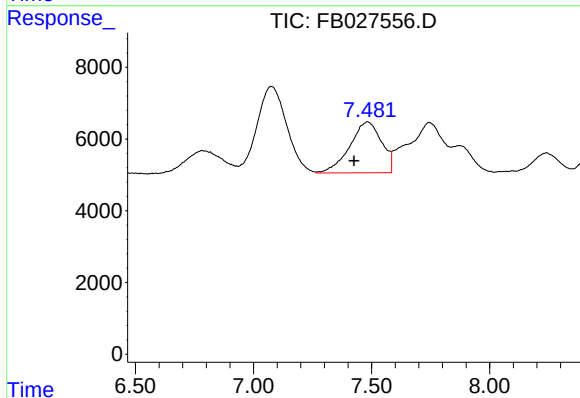


#2 2,2,4-Trimethylpentane

R.T.: 7.483 min
Delta R.T.: 0.056 min
Response: 132902
Conc: 7.57 ng/ml

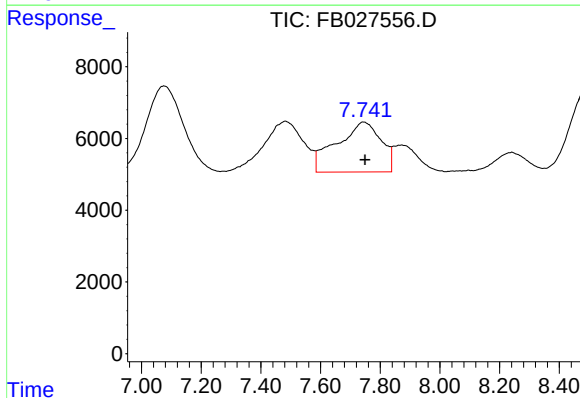


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.007 min
Response: 143601
Conc: 8.20 ng/ml

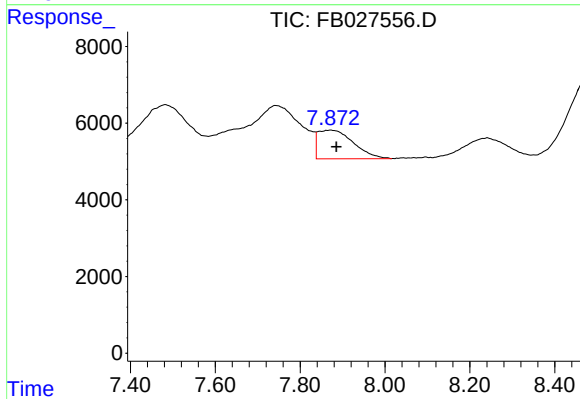

#4 Benzene


R.T.: 7.873 min
Delta R.T.: -0.013 min
Response: 43178
Conc: 2.12 ng/ml

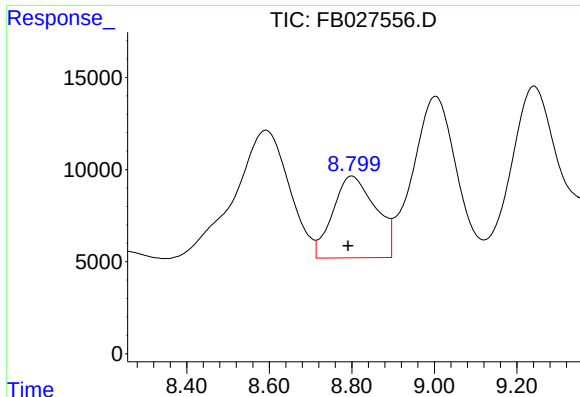

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.009 min
Response: 320703
Conc: 28.59 ng/ml

Instrument :
FID_B
ClientSampleId :

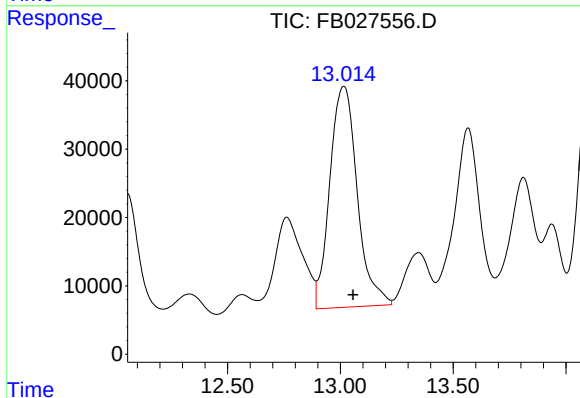


#7 Ethylbenzene

R.T.: 13.015 min
Delta R.T.: -0.042 min
Response: 2735110
Conc: 151.03 ng/ml

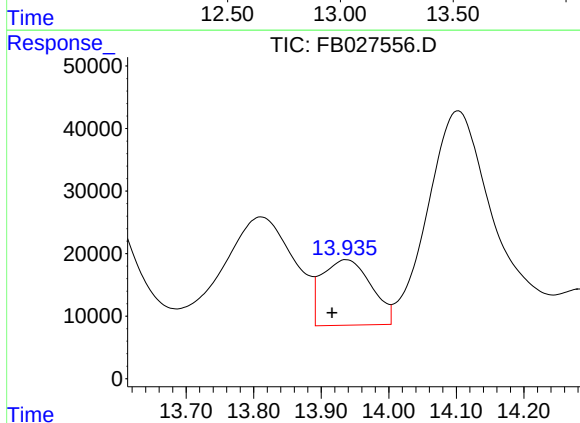

#9 O-Xylene

R.T.: 13.937 min
Delta R.T.: 0.021 min
Response: 531113
Conc: 30.57 ng/ml

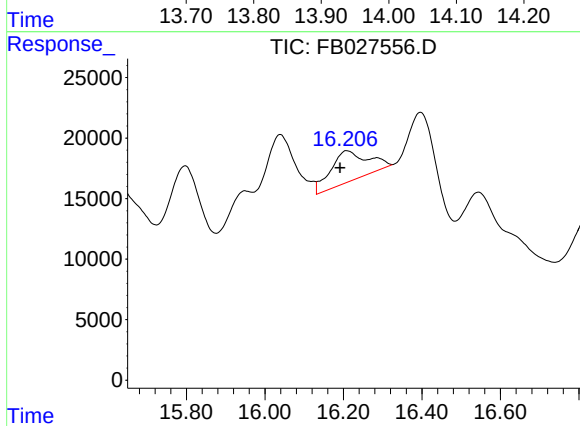

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.019 min
Response: 166096
Conc: 9.67 ng/ml