

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
 Data File : FB027557.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2022 2:33
 Operator : AJ/MA
 Sample : N3494-19 50X
 Misc : 5.09G/5.00 ML MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 28 04:28:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	290982	25.942 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	22277	1.322 ng/ml
3) t n-Heptane	7.752	12704	0.725 ng/ml
4) t Benzene	7.902	11008	0.540 ng/ml
6) t Toluene	10.624	13618	0.703 ng/ml
7) t Ethylbenzene	13.120	2572	0.142 ng/ml
8) t m-Xylene	13.191	41791	2.344 ng/ml
9) t O-Xylene	13.929	6571	0.378 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	27861	1.622 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
Data File : FB027557.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2022 2:33
Operator : AJ/MA
Sample : N3494-19 50X
Misc : 5.09G/5.00 ML MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 28 04:28:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

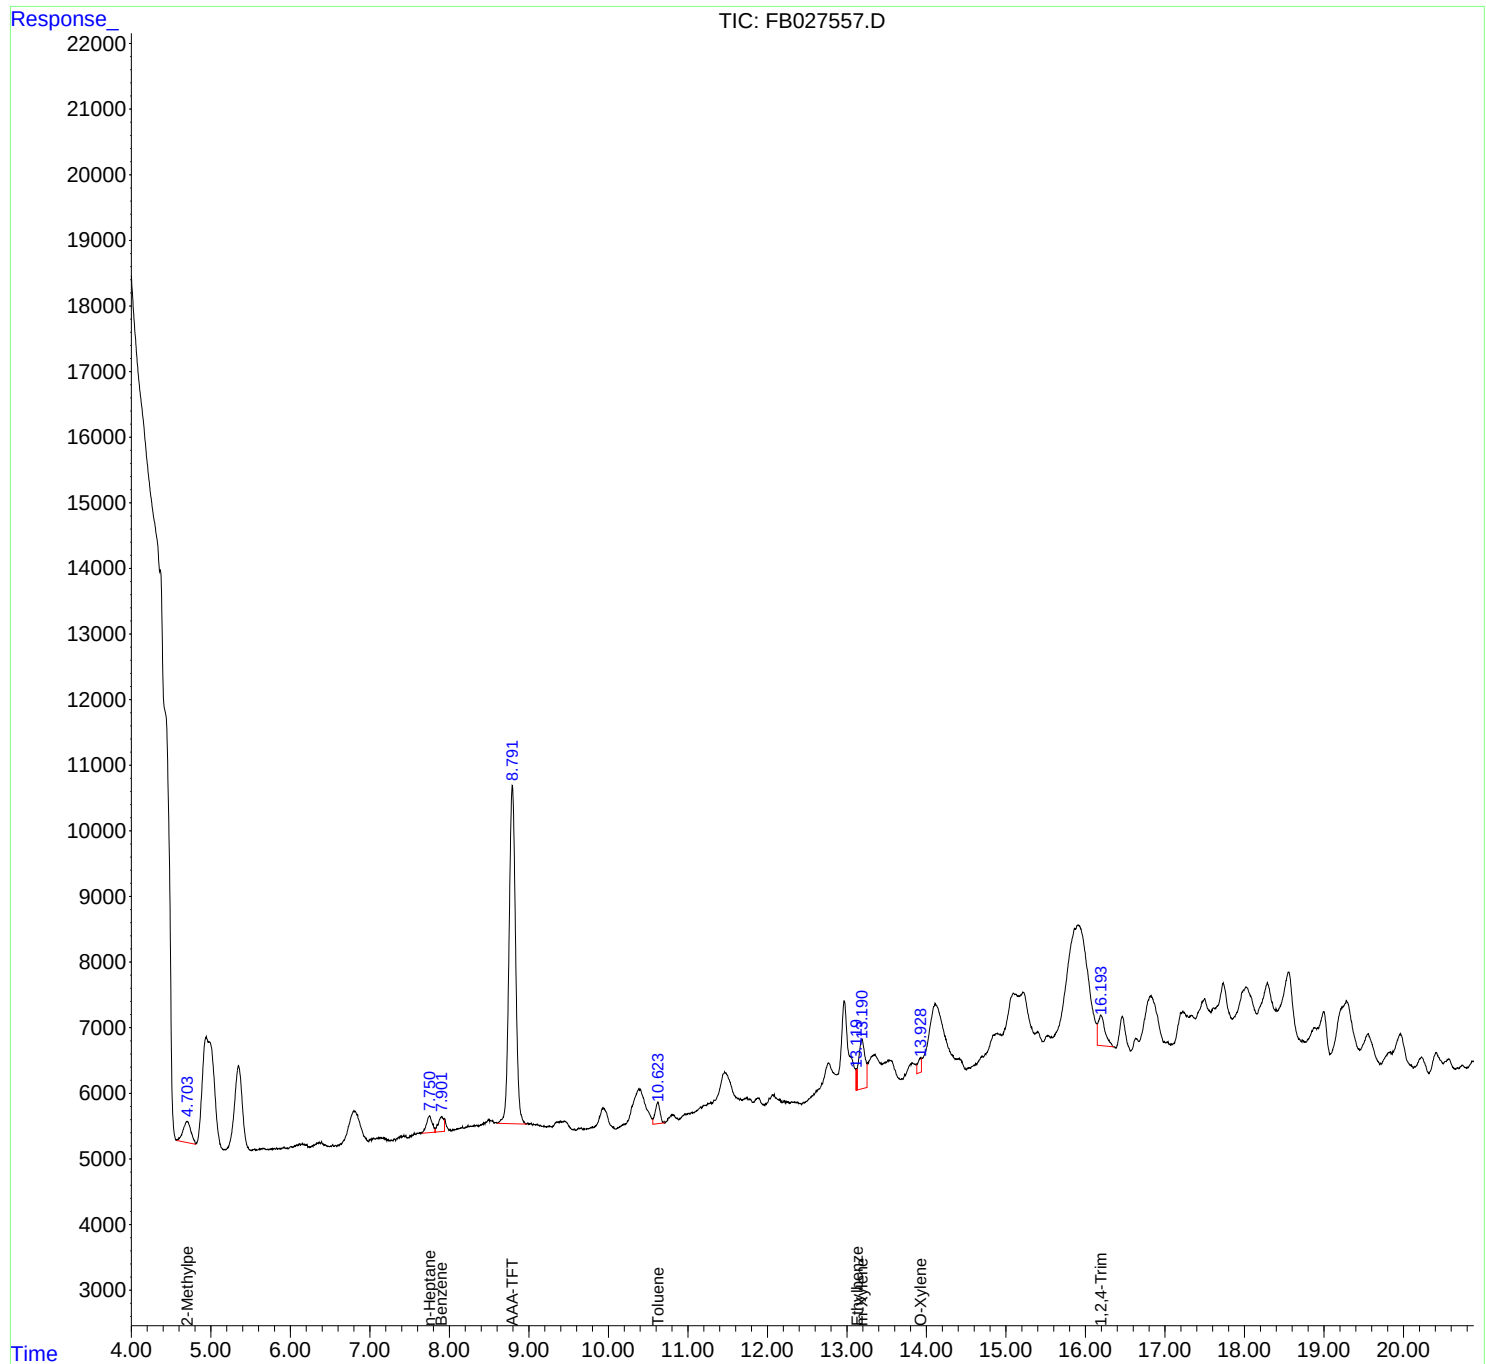


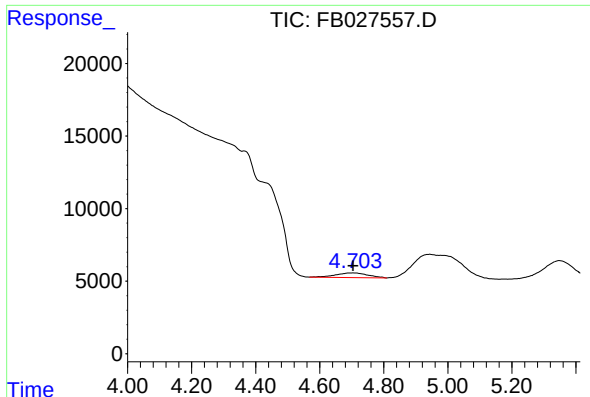

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: 0.000 min
Response: 22277
Conc: 1.32 ng/ml

Instrument :
FID_B
ClientSampleId :

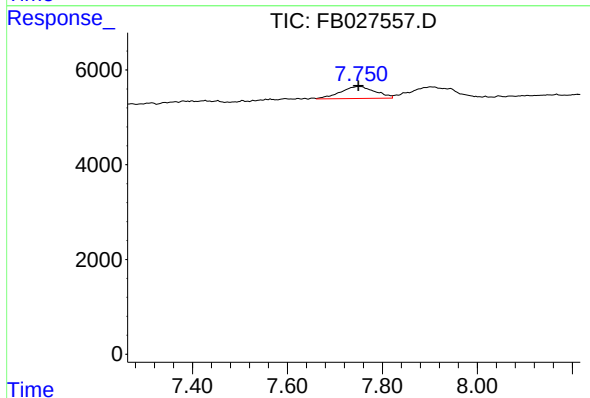


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.002 min
Response: 12704
Conc: 0.73 ng/ml

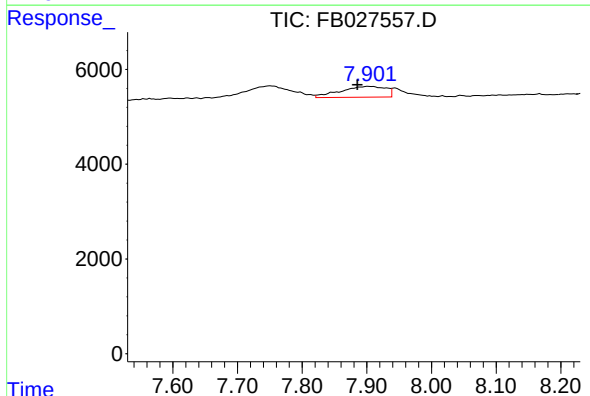


#4 Benzene

R.T.: 7.902 min
Delta R.T.: 0.017 min
Response: 11008
Conc: 0.54 ng/ml

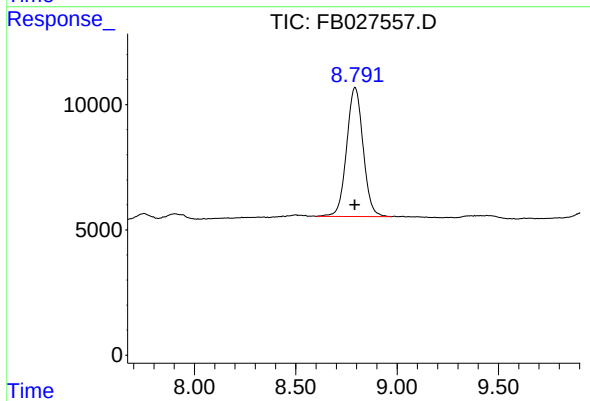

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 290982
Conc: 25.94 ng/ml

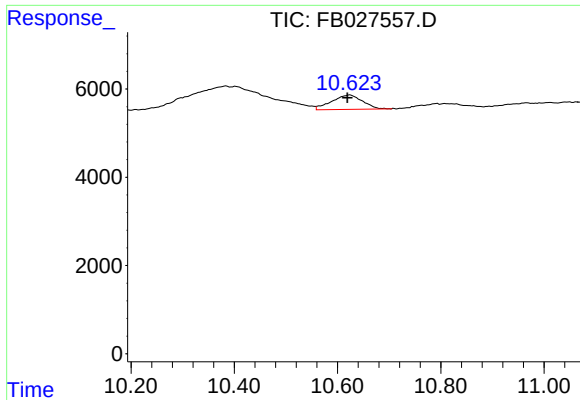

#6 Toluene


R.T.: 10.624 min
Delta R.T.: 0.005 min
Response: 13618
Conc: 0.70 ng/ml

Instrument :
FID_B
ClientSampleId :

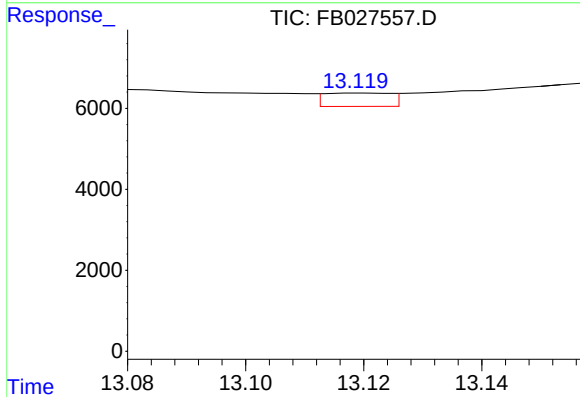


#7 Ethylbenzene

R.T.: 13.120 min
Delta R.T.: 0.064 min
Response: 2572
Conc: 0.14 ng/ml

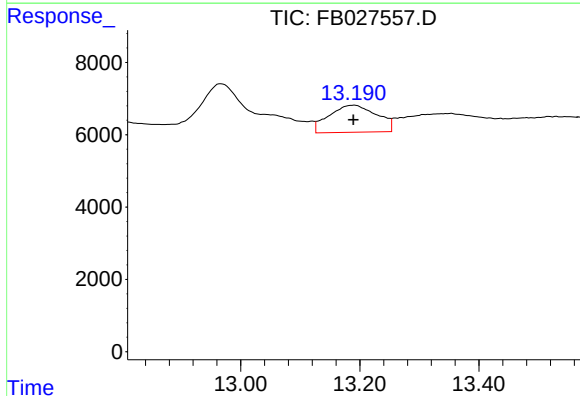


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 41791
Conc: 2.34 ng/ml

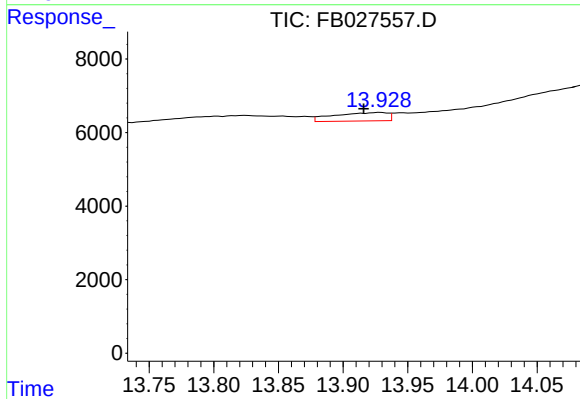

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.013 min
Response: 6571
Conc: 0.38 ng/ml

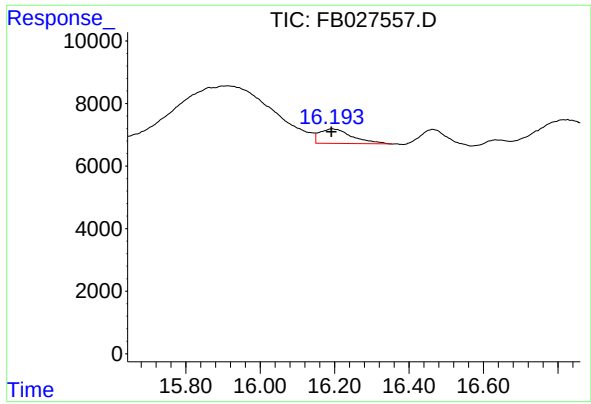

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.002 min
Response: 27861
Conc: 1.62 ng/ml

Instrument :
FID_B
ClientSampleId :