

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
 Data File : FB027536.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jun 2022 12:02
 Operator : AJ/MA
 Sample : BSF0627S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0627S1

Integration File: Calibration.e
 Quant Time: Jun 28 04:25:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	262979	23.445 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	524712	31.145 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	546634	31.132 ng/ml
3) t n-Heptane	7.753	189313	10.806 ng/ml
4) t Benzene	7.890	207285	10.165 ng/ml
6) t Toluene	10.623	599350	30.955 ng/ml
7) t Ethylbenzene	13.060	183946	10.157 ng/ml
8) t m-Xylene	13.193	366670	20.569 ng/ml
9) t O-Xylene	13.920	354401	20.396 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	350040	20.377 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
Data File : FB027536.D
Signal(s) : FID2B.CH
Acq On : 27 Jun 2022 12:02
Operator : AJ/MA
Sample : BSF0627S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0627S1

Integration File: Calibration.e
Quant Time: Jun 28 04:25:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

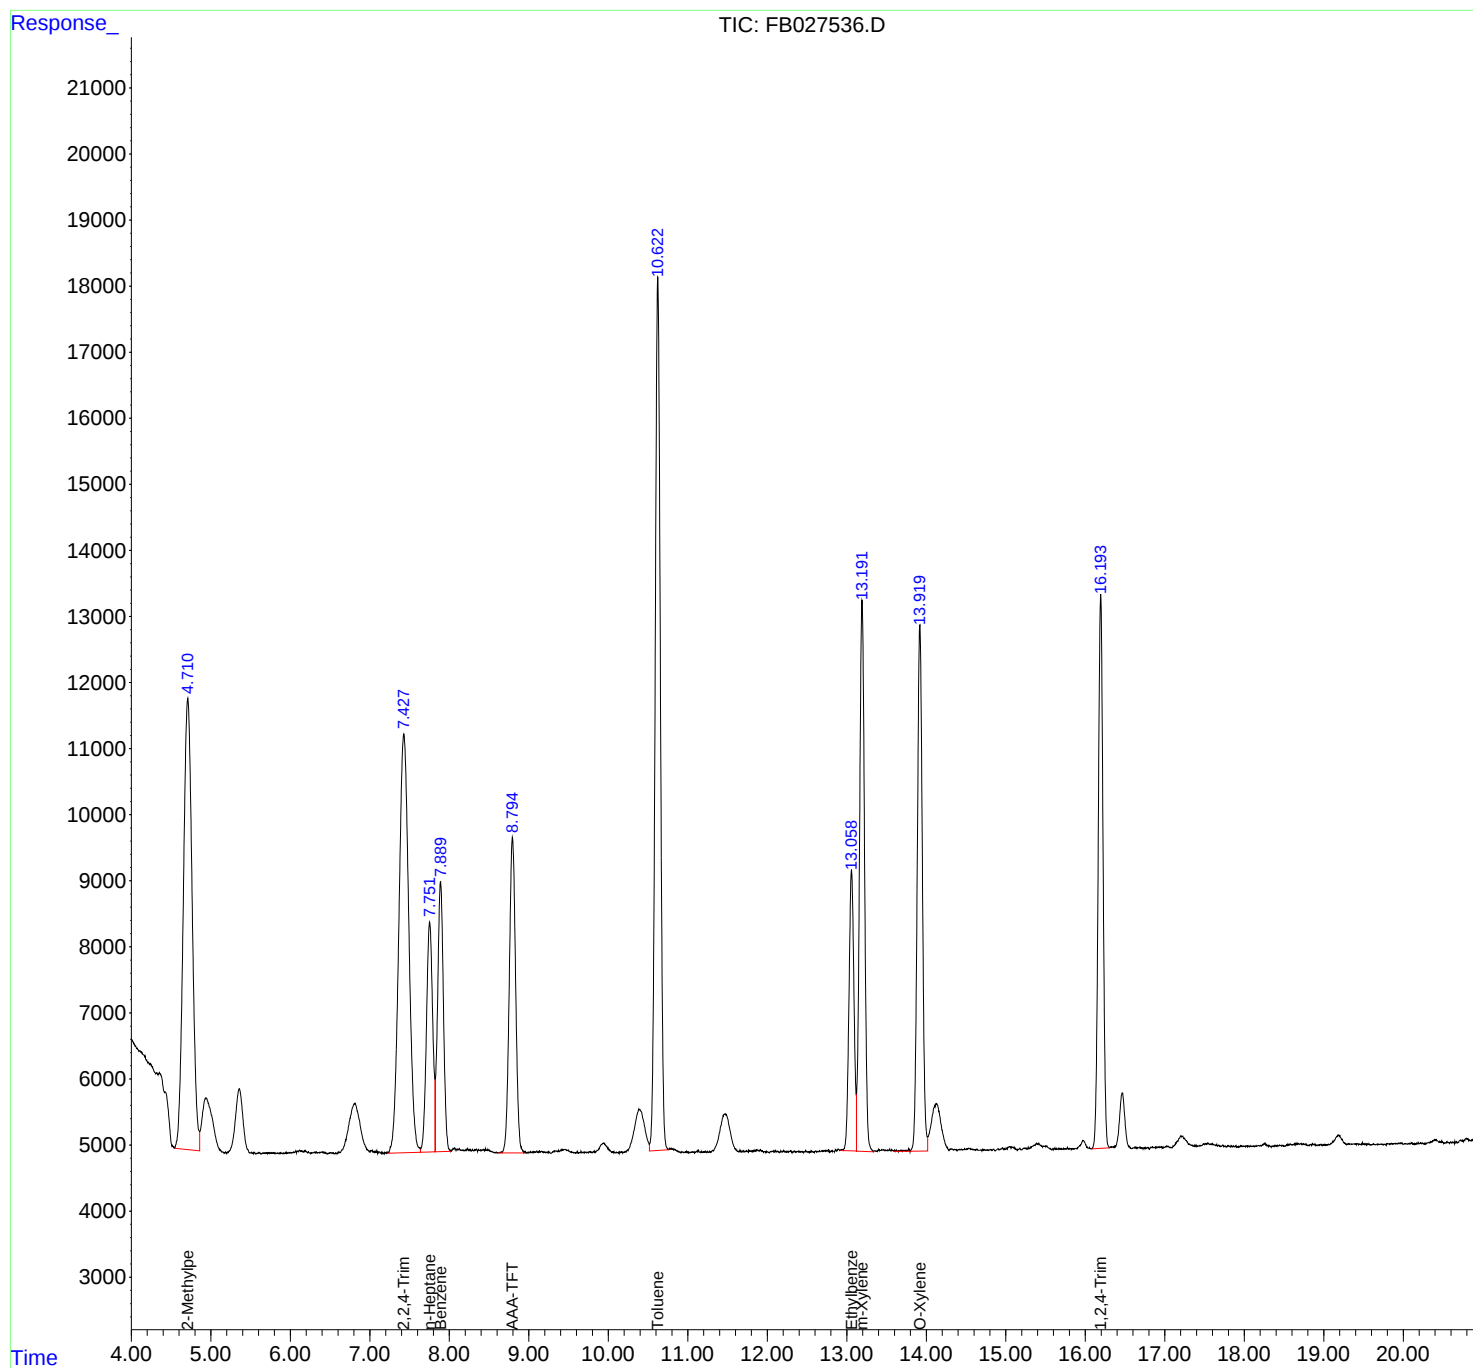


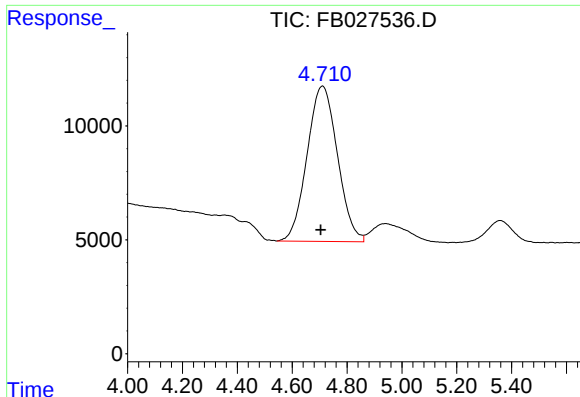

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.007 min
Response: 524712
Conc: 31.15 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0627S1

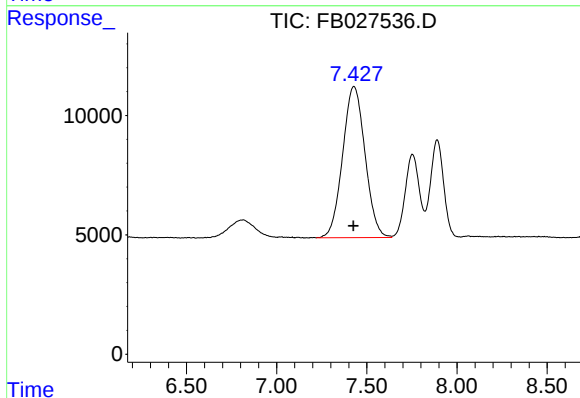


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: 0.003 min
Response: 546634
Conc: 31.13 ng/ml

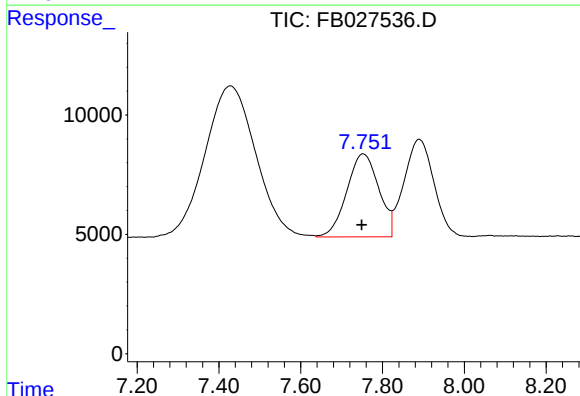


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.003 min
Response: 189313
Conc: 10.81 ng/ml

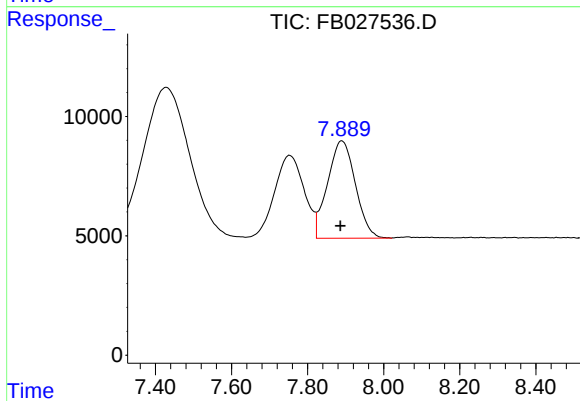

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.004 min
Response: 207285
Conc: 10.16 ng/ml

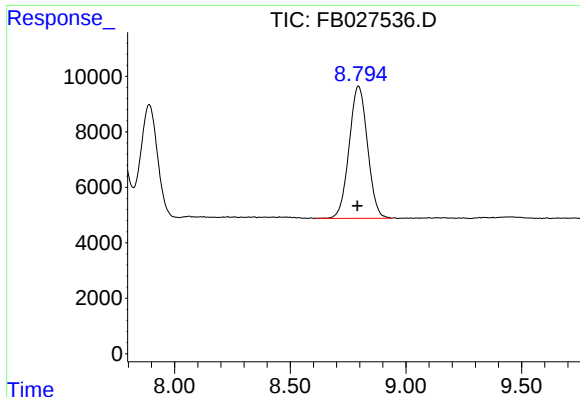

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.004 min
Response: 262979
Conc: 23.45 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0627S1

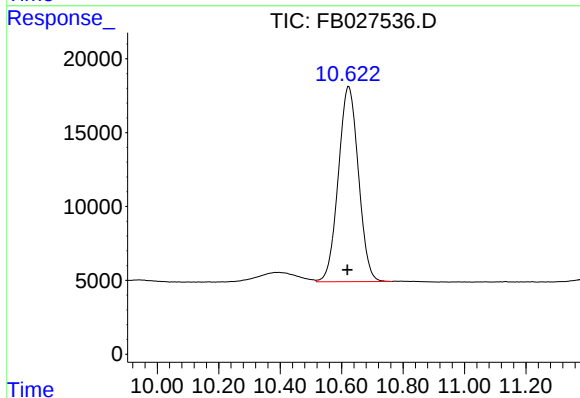


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.004 min
Response: 599350
Conc: 30.95 ng/ml

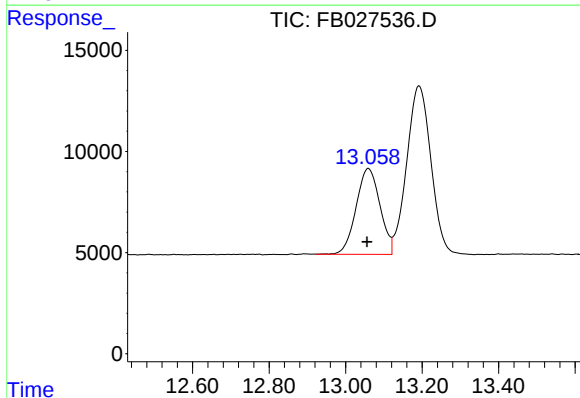


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.004 min
Response: 183946
Conc: 10.16 ng/ml

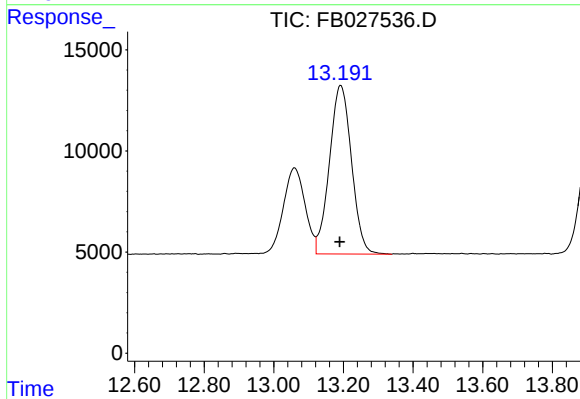

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: 0.003 min
Response: 366670
Conc: 20.57 ng/ml

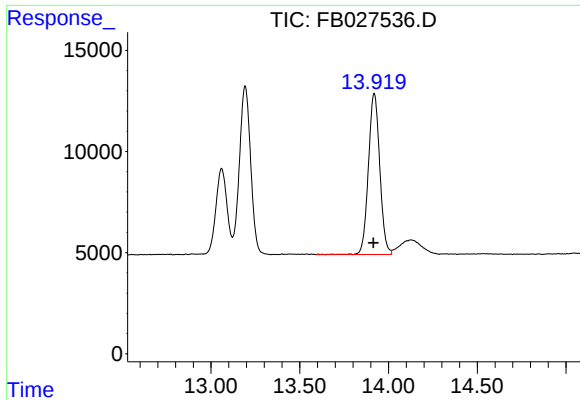

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.004 min
Response: 354401
Conc: 20.40 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0627S1

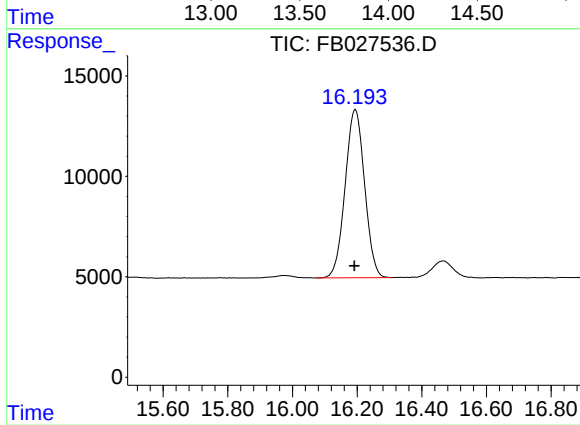

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.003 min
Response: 350040
Conc: 20.38 ng/ml