

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
 Data File : FB027542.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jun 2022 16:07
 Operator : AJ/MA
 Sample : BSF0627S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0627S2

Integration File: Calibration.e
 Quant Time: Jun 28 04:26:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	213938	19.073 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	535858	31.807 ng/ml
2) t 2,2,4-Trimethylpentane	7.431	553977	31.551 ng/ml
3) t n-Heptane	7.756	187812	10.721 ng/ml
4) t Benzene	7.892	207059	10.154 ng/ml
6) t Toluene	10.626	601197	31.050 ng/ml
7) t Ethylbenzene	13.063	186868	10.319 ng/ml
8) t m-Xylene	13.195	371119	20.819 ng/ml
9) t O-Xylene	13.922	360934	20.772 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	357400	20.805 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
Data File : FB027542.D
Signal(s) : FID2B.CH
Acq On : 27 Jun 2022 16:07
Operator : AJ/MA
Sample : BSF0627S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0627S2

Integration File: Calibration.e
Quant Time: Jun 28 04:26:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

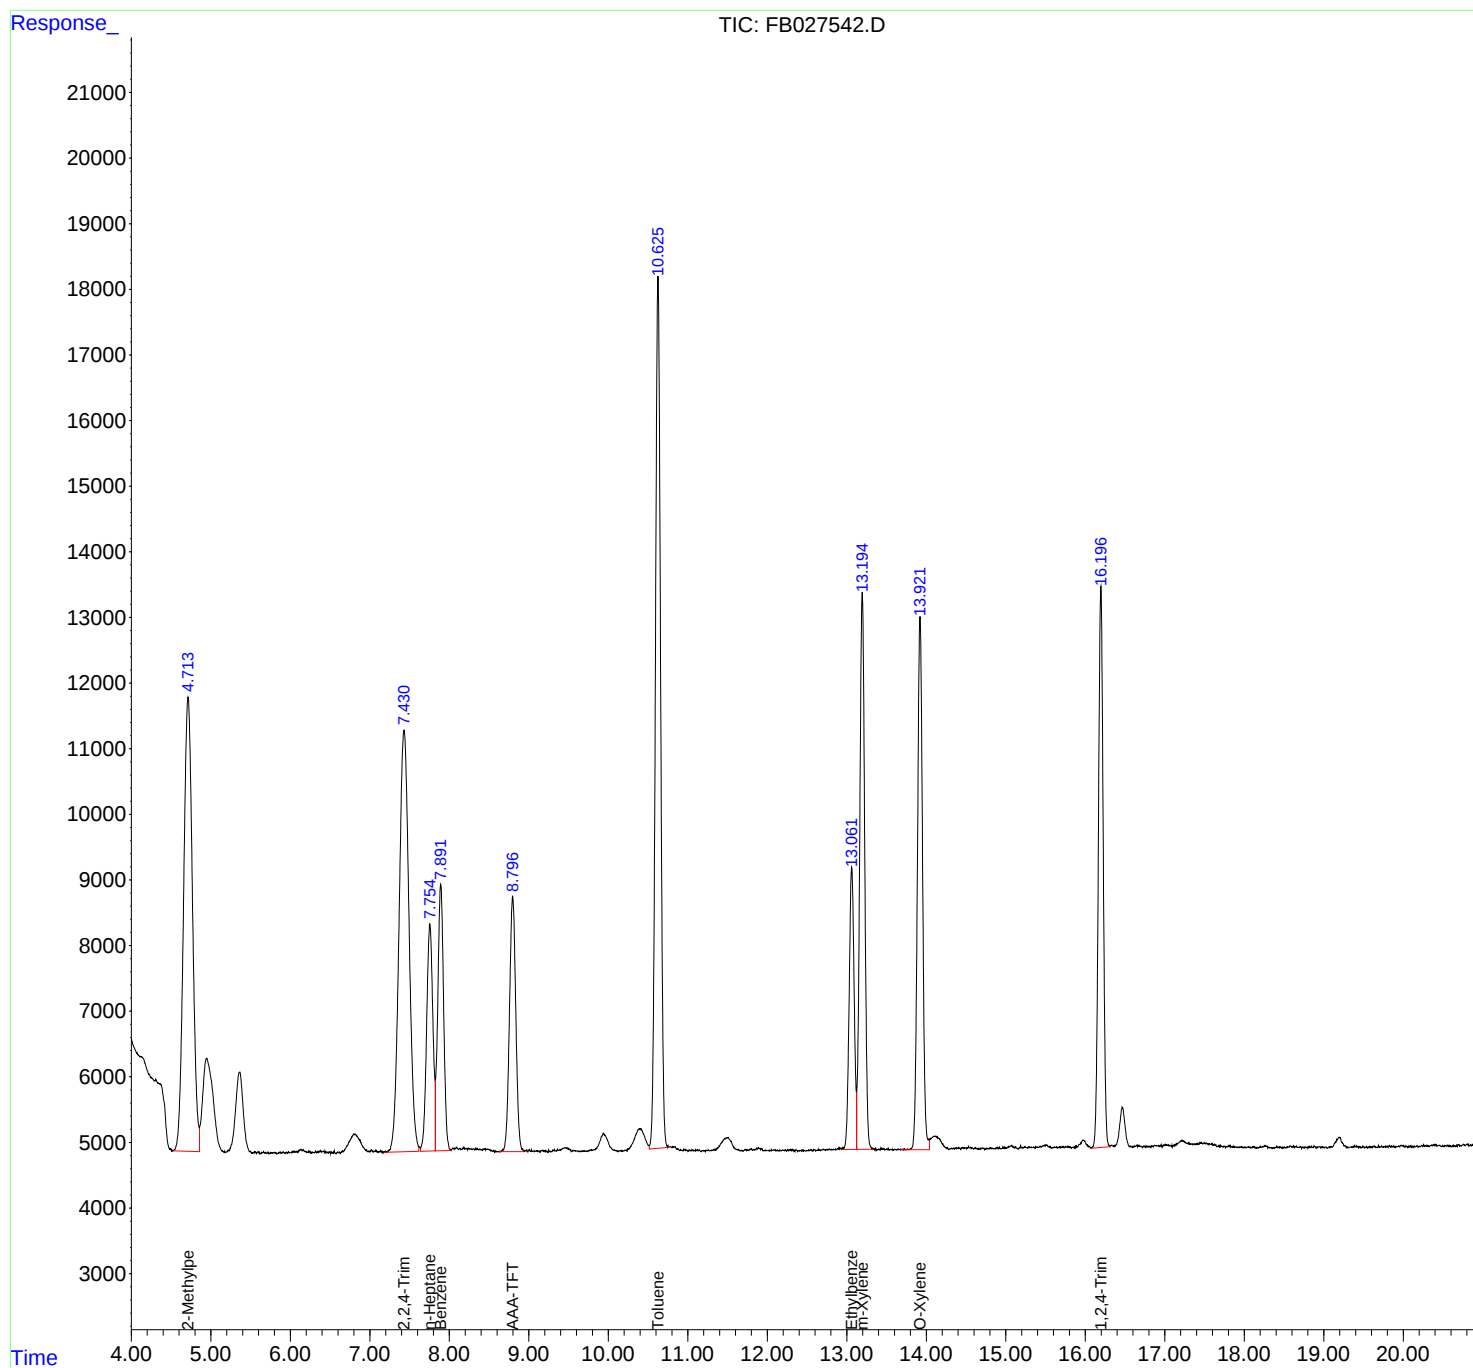


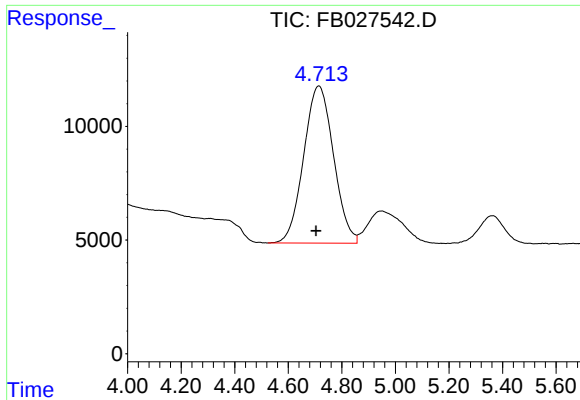

#1 2-Methylpentane


R.T.: 4.715 min
Delta R.T.: 0.011 min
Response: 535858
Conc: 31.81 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0627S2

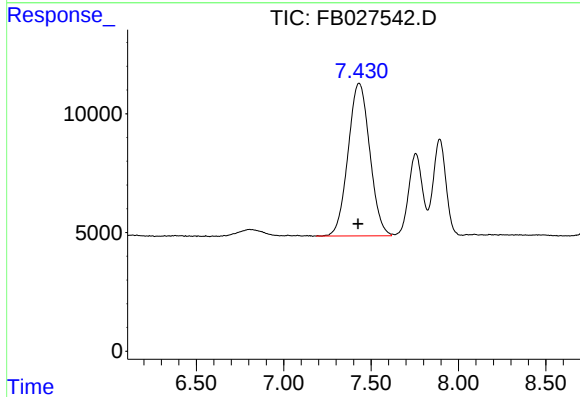


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: 0.005 min
Response: 553977
Conc: 31.55 ng/ml

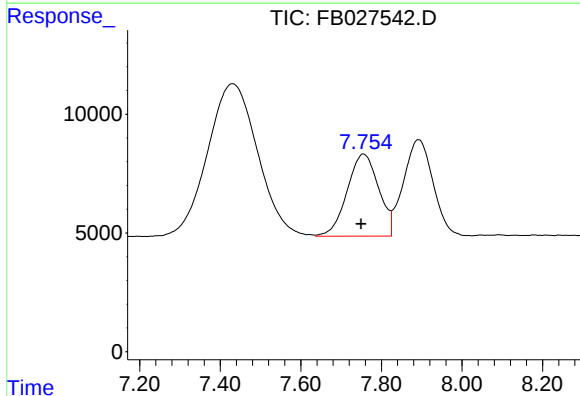


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.006 min
Response: 187812
Conc: 10.72 ng/ml

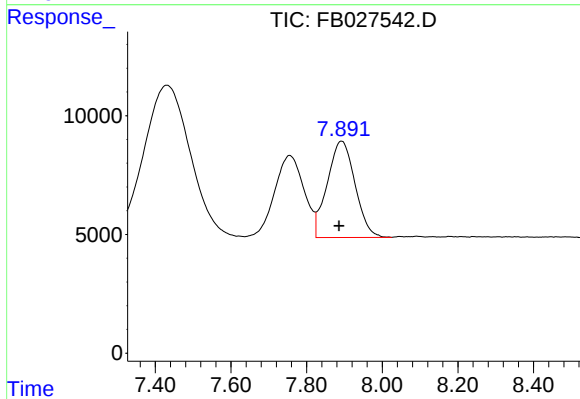

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.007 min
Response: 207059
Conc: 10.15 ng/ml

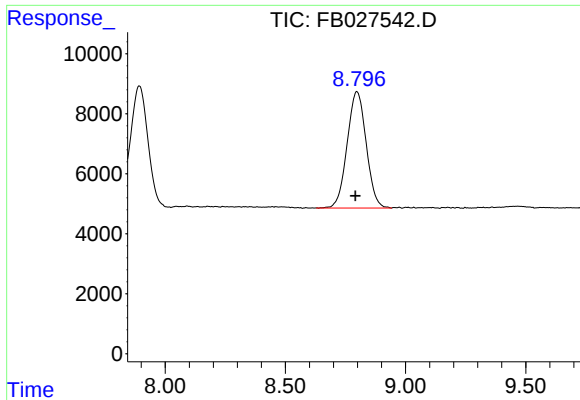

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.007 min
Response: 213938
Conc: 19.07 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0627S2

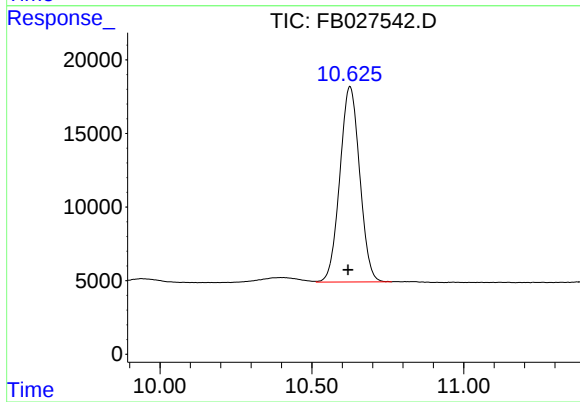


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.007 min
Response: 601197
Conc: 31.05 ng/ml

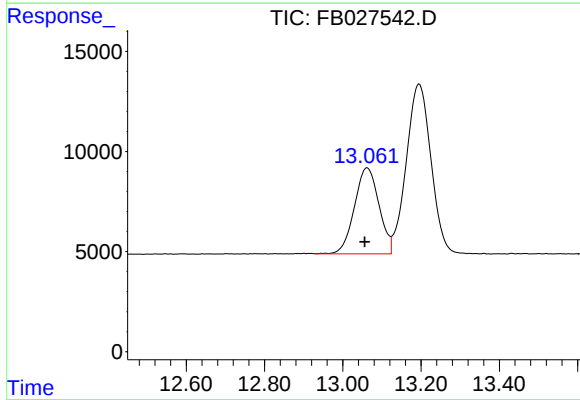


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.006 min
Response: 186868
Conc: 10.32 ng/ml

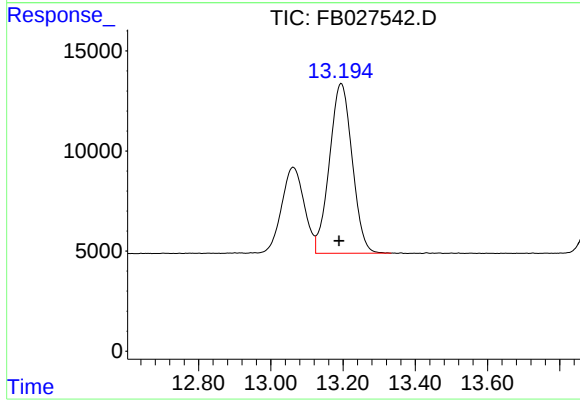

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: 0.006 min
Response: 371119
Conc: 20.82 ng/ml

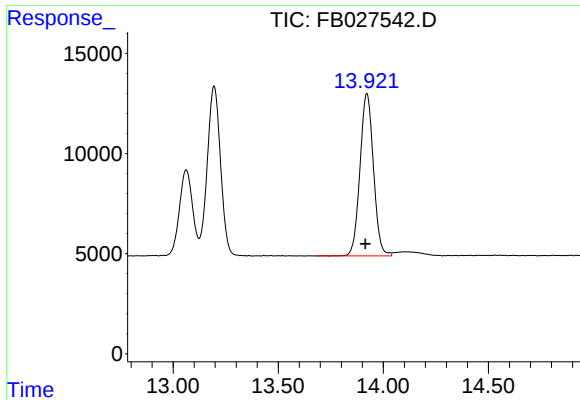

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.006 min
Response: 360934
Conc: 20.77 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0627S2

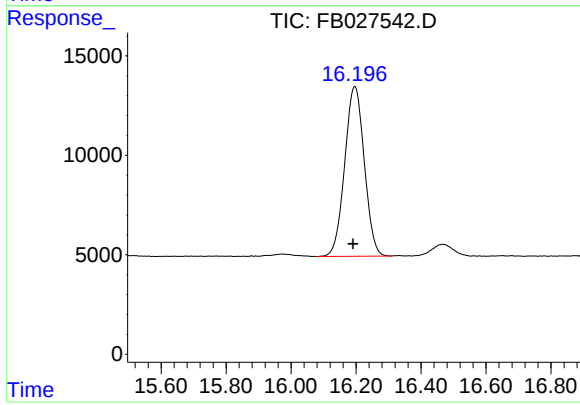

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.005 min
Response: 357400
Conc: 20.81 ng/ml