

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
 Data File : FB027560.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2022 4:22
 Operator : AJ/MA
 Sample : N3494-34MS 50X
 Misc : 5.07G/5.00 ML MEOH
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SP-EXC-1-1-GRMS

Integration File: Calibration.e
 Quant Time: Jun 28 06:27:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	183994	16.404 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	496875	29.493 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	520757	29.659 ng/ml
3) t n-Heptane	7.749	186716	10.658 ng/ml
4) t Benzene	7.885	222416	10.907 ng/ml
6) t Toluene	10.620	592256	30.589 ng/ml
7) t Ethylbenzene	13.057	198147	10.942 ng/ml
8) t m-Xylene	13.189	361636	20.287 ng/ml
9) t O-Xylene	13.916	345489	19.883 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	319145	18.578 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
Data File : FB027560.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2022 4:22
Operator : AJ/MA
Sample : N3494-34MS 50X
Misc : 5.07G/5.00 ML MEOH
ALS Vial : 30 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SP-EXC-1-1-GRMS

Integration File: Calibration.e
Quant Time: Jun 28 06:27:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

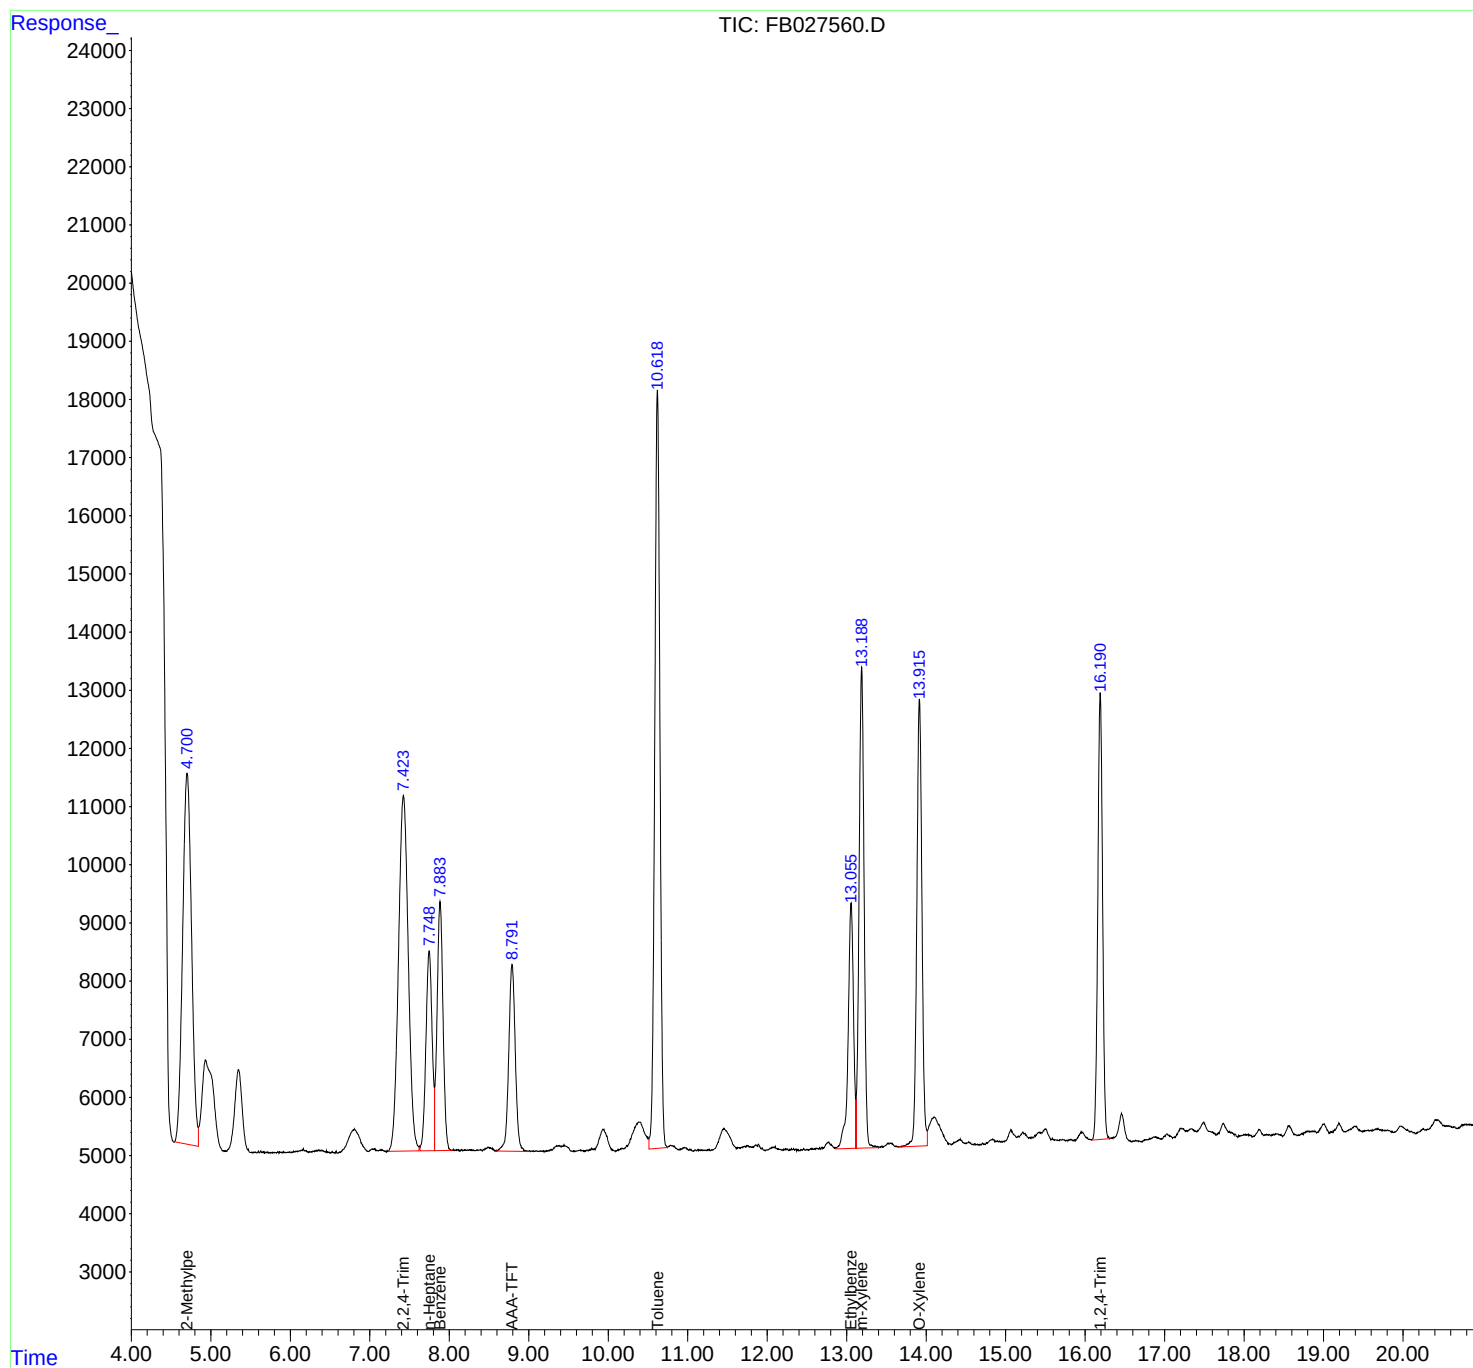


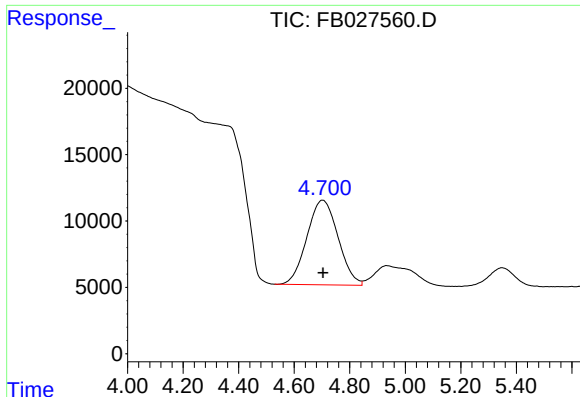

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: -0.002 min
Response: 496875
Conc: 29.49 ng/ml

Instrument :
FID_B
ClientSampleId :
SP-EXC-1-1-GRMS

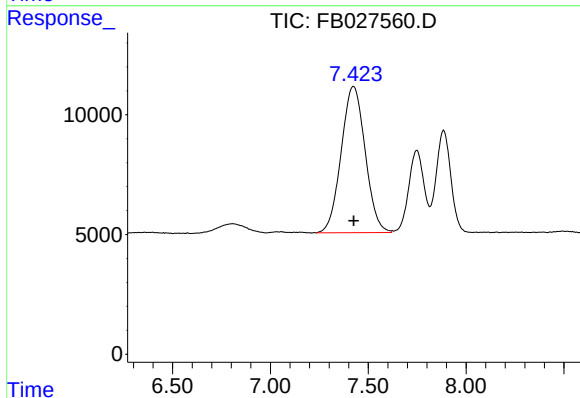


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: -0.002 min
Response: 520757
Conc: 29.66 ng/ml

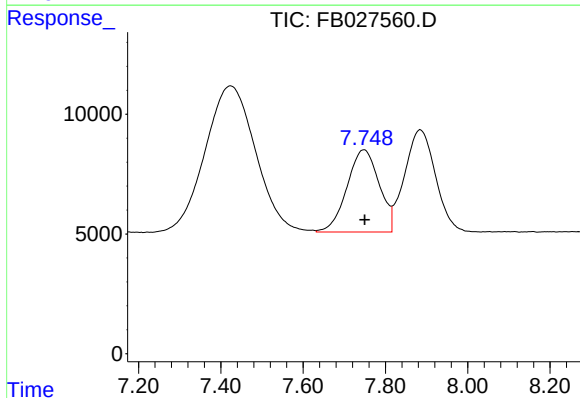


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 186716
Conc: 10.66 ng/ml

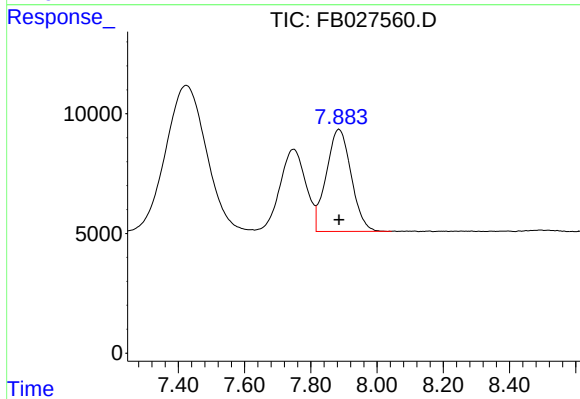

#4 Benzene


R.T.: 7.885 min
Delta R.T.: 0.000 min
Response: 222416
Conc: 10.91 ng/ml

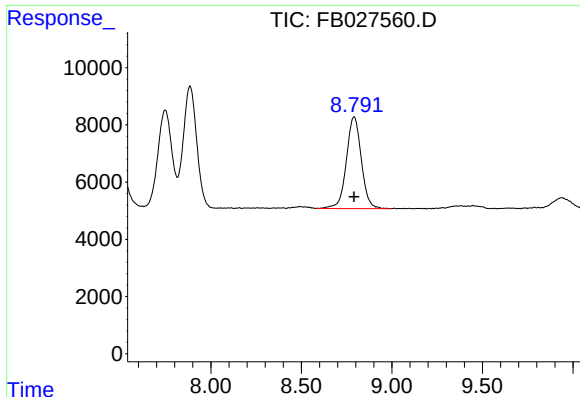

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 183994
Conc: 16.40 ng/ml

Instrument :
FID_B
ClientSampleId :
SP-EXC-1-1-GRMS

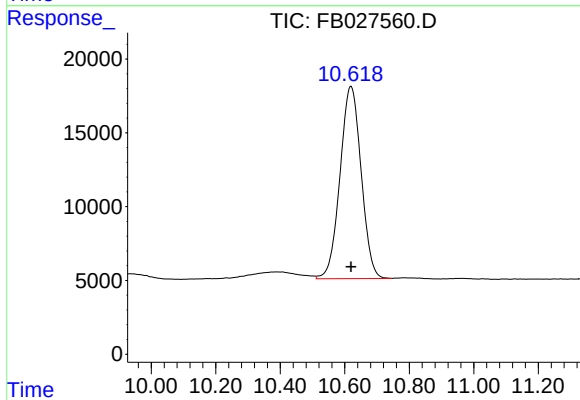


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 592256
Conc: 30.59 ng/ml

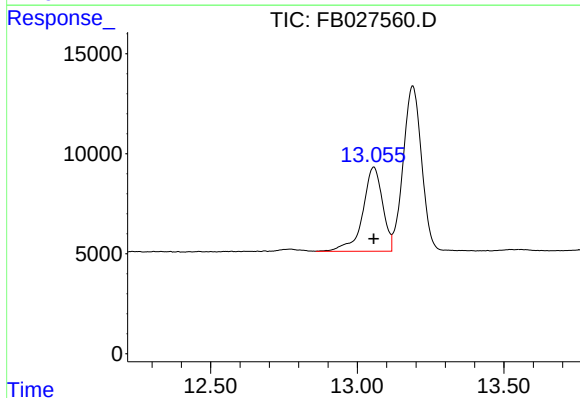


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 198147
Conc: 10.94 ng/ml

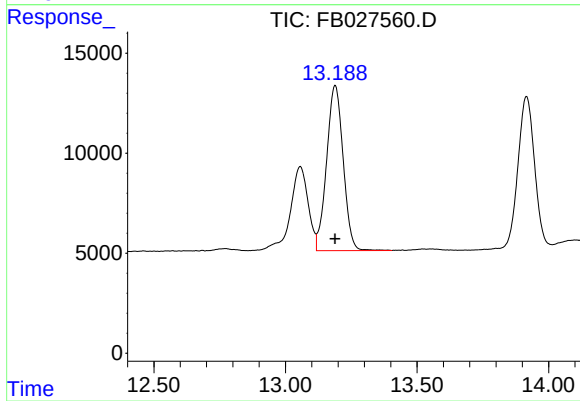

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 361636
Conc: 20.29 ng/ml

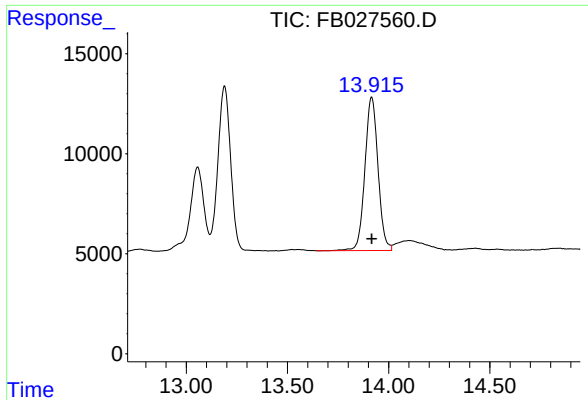

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 345489
Conc: 19.88 ng/ml

Instrument :
FID_B
ClientSampleId :
SP-EXC-1-1-GRMS

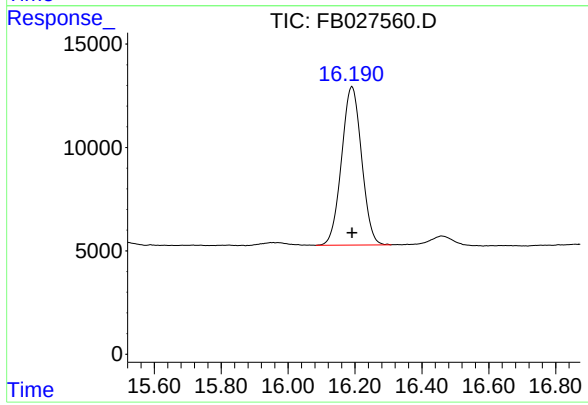

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 319145
Conc: 18.58 ng/ml