

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
 Data File : FB027561.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2022 4:59
 Operator : AJ/MA
 Sample : N3494-34MSD 50X
 Misc : 5.00G/5.00 ML MEOH
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SP-EXC-1-1-GRMSD

Integration File: Calibration.e
 Quant Time: Jun 28 06:28:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	223205	19.899 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	506573	30.069 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	526845	30.005 ng/ml
3) t n-Heptane	7.749	194832	11.121 ng/ml
4) t Benzene	7.886	231321	11.343 ng/ml
6) t Toluene	10.620	611313	31.573 ng/ml
7) t Ethylbenzene	13.056	201386	11.120 ng/ml
8) t m-Xylene	13.189	366889	20.582 ng/ml
9) t O-Xylene	13.916	349205	20.097 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	320418	18.652 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
Data File : FB027561.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2022 4:59
Operator : AJ/MA
Sample : N3494-34MSD 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SP-EXC-1-1-GRMSD

Integration File: Calibration.e
Quant Time: Jun 28 06:28:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

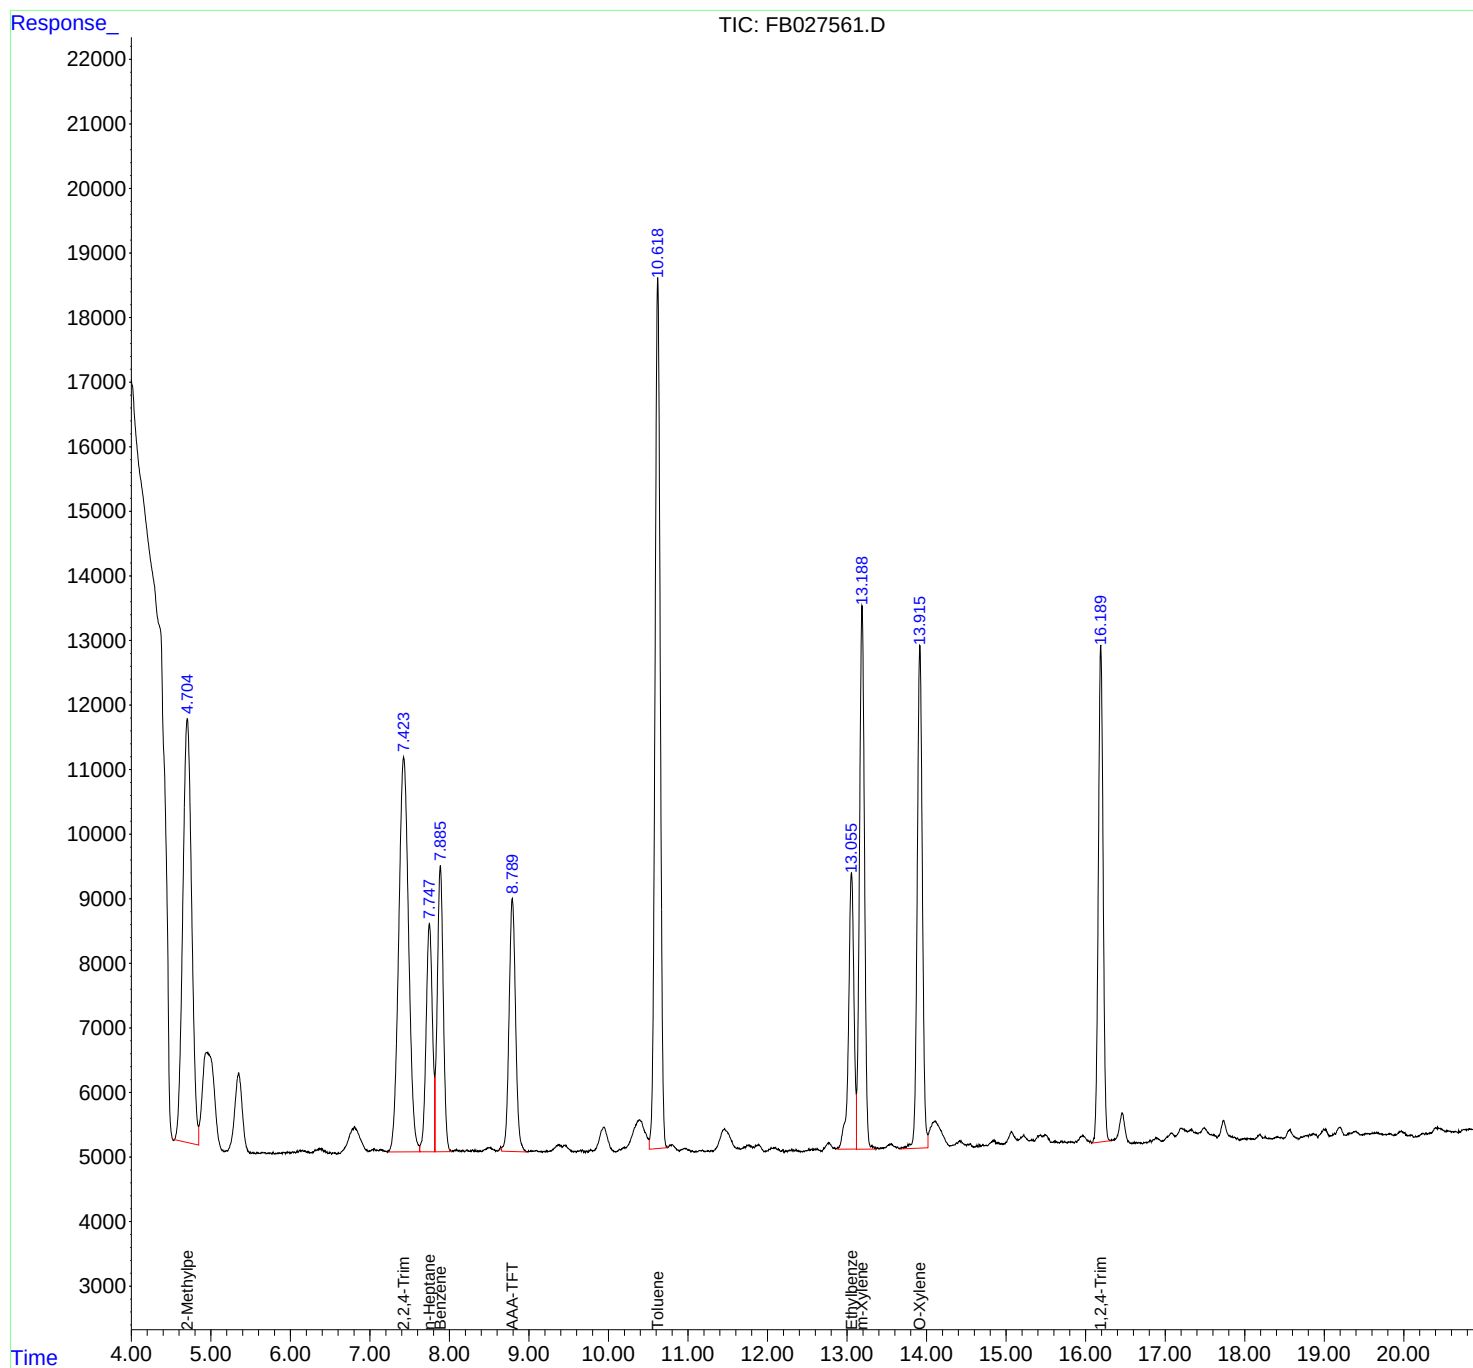


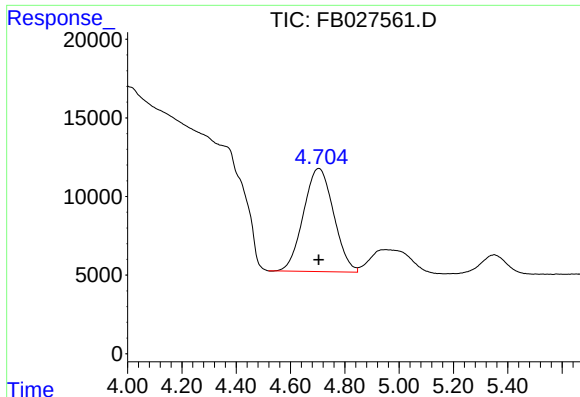

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: 0.001 min
Response: 506573
Conc: 30.07 ng/ml

Instrument :
FID_B
ClientSampleId :
SP-EXC-1-1-GRMSD

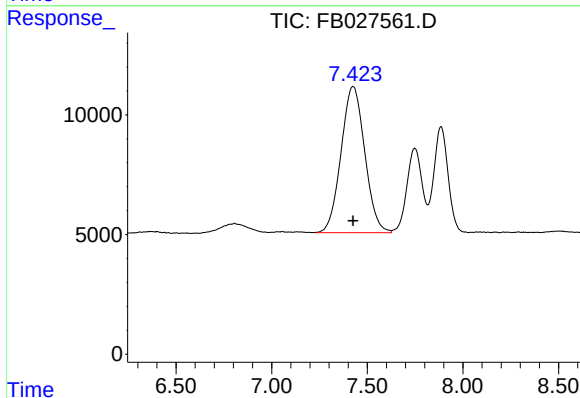


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: -0.002 min
Response: 526845
Conc: 30.01 ng/ml

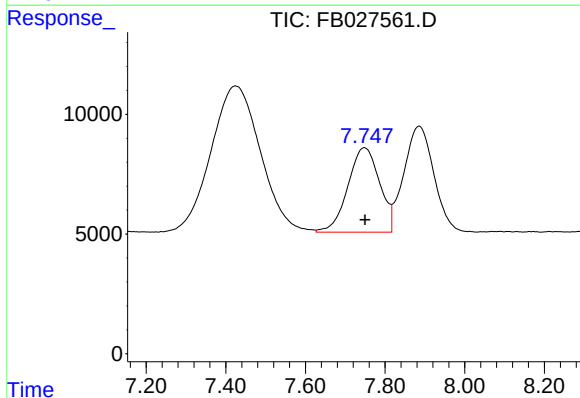


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 194832
Conc: 11.12 ng/ml

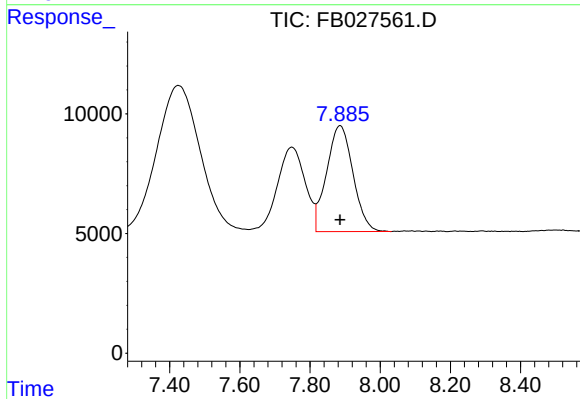

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 231321
Conc: 11.34 ng/ml

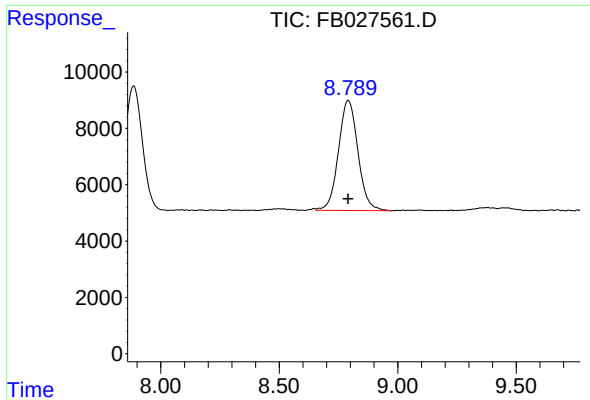

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 223205
Conc: 19.90 ng/ml

Instrument :
FID_B
ClientSampleId :
SP-EXC-1-1-GRMSD

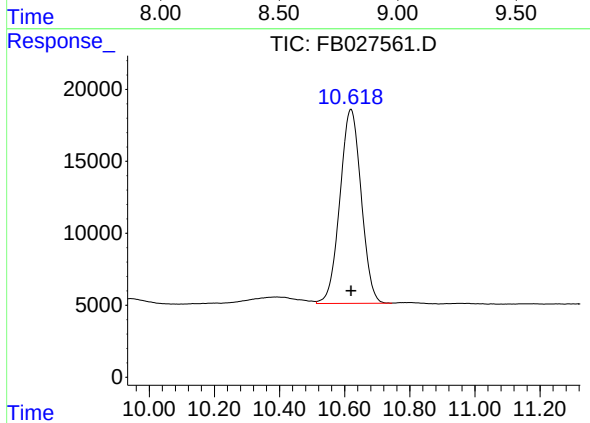


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 611313
Conc: 31.57 ng/ml

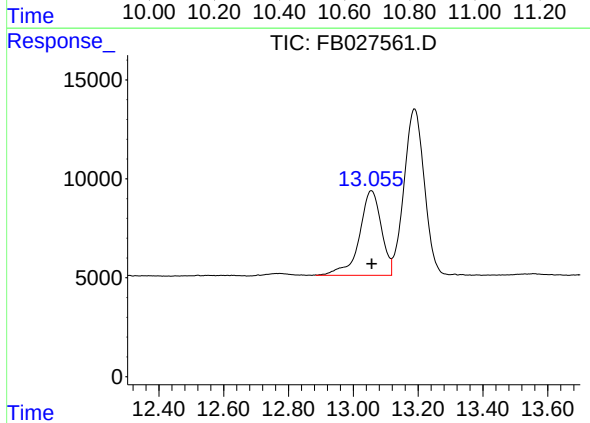


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 201386
Conc: 11.12 ng/ml

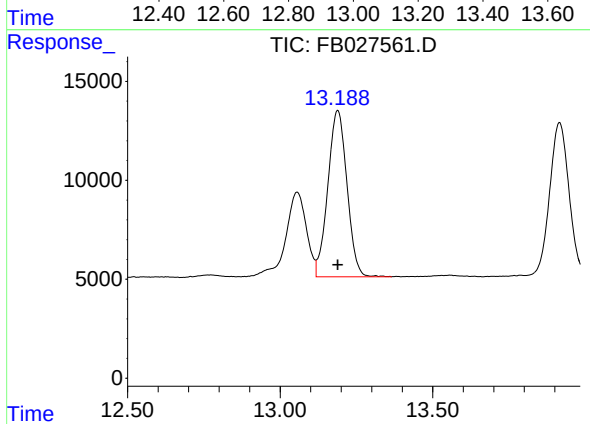

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 366889
Conc: 20.58 ng/ml

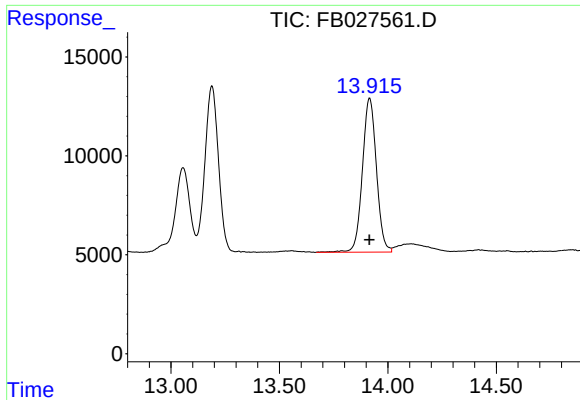

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 349205
Conc: 20.10 ng/ml

Instrument :
FID_B
ClientSampleId :
SP-EXC-1-1-GRMSD

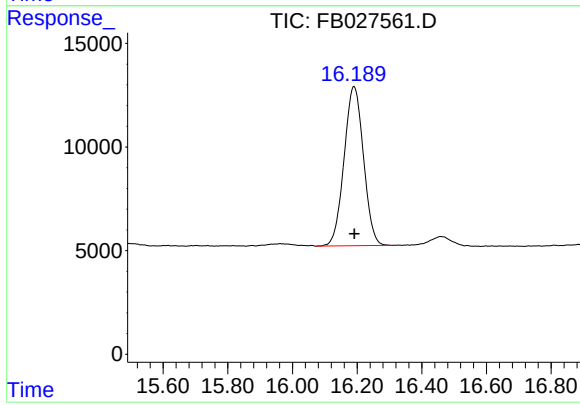

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 320418
Conc: 18.65 ng/ml