

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
 Data File : FB027562.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2022 5:35
 Operator : AJ/MA
 Sample : BSF0627S3
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0627S3

Integration File: Calibration.e
 Quant Time: Jun 28 06:28:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	206060	18.371 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	543770	32.276 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	552518	31.468 ng/ml
3) t n-Heptane	7.751	175314	10.007 ng/ml
4) t Benzene	7.887	218081	10.694 ng/ml
6) t Toluene	10.620	607903	31.397 ng/ml
7) t Ethylbenzene	13.057	186086	10.276 ng/ml
8) t m-Xylene	13.189	370358	20.776 ng/ml
9) t O-Xylene	13.916	365805	21.052 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	357404	20.805 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062722\
Data File : FB027562.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2022 5:35
Operator : AJ/MA
Sample : BSF0627S3
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0627S3

Integration File: Calibration.e
Quant Time: Jun 28 06:28:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

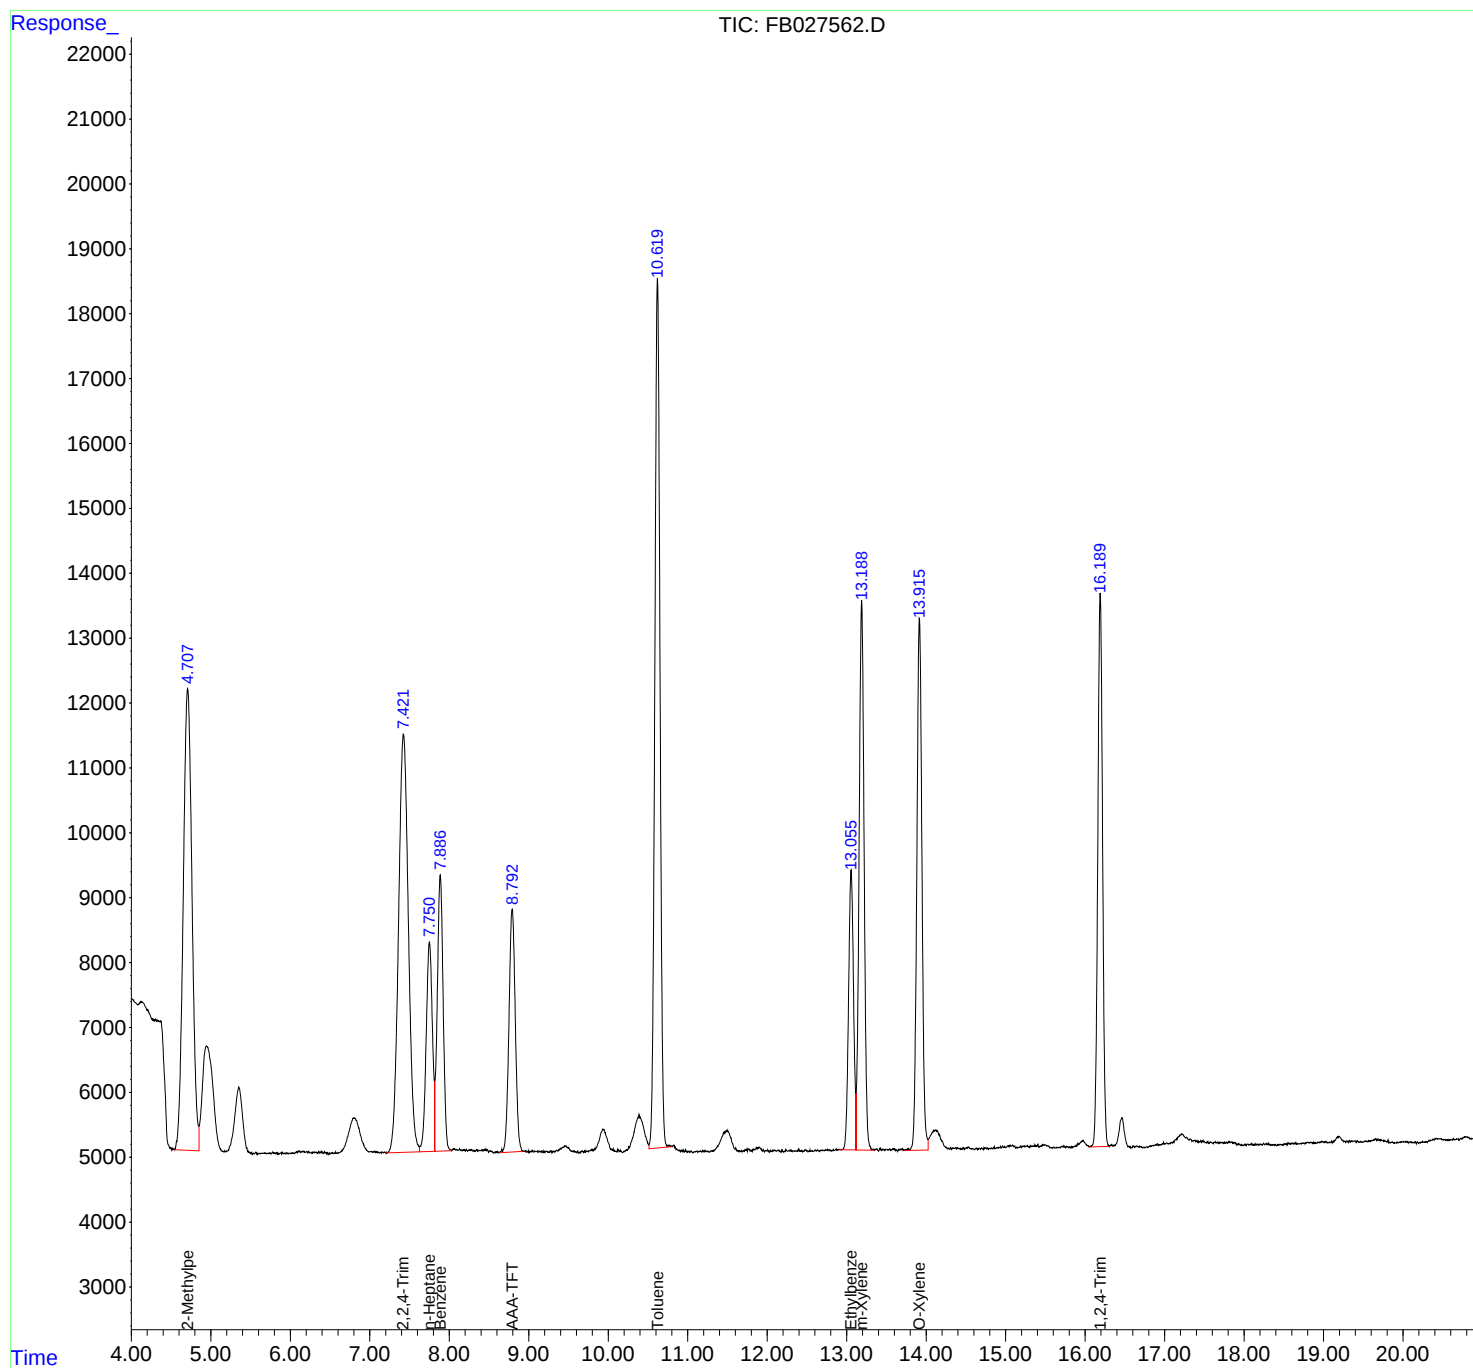


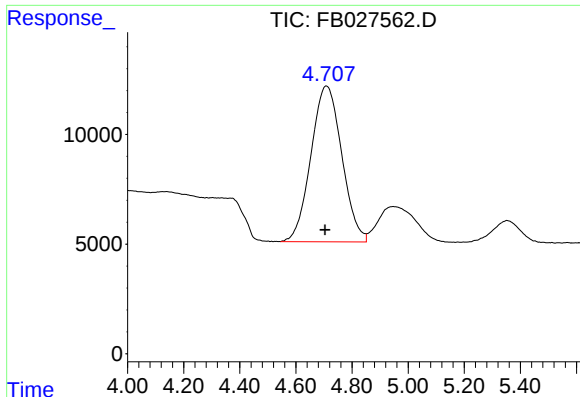

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.005 min
Response: 543770
Conc: 32.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0627S3

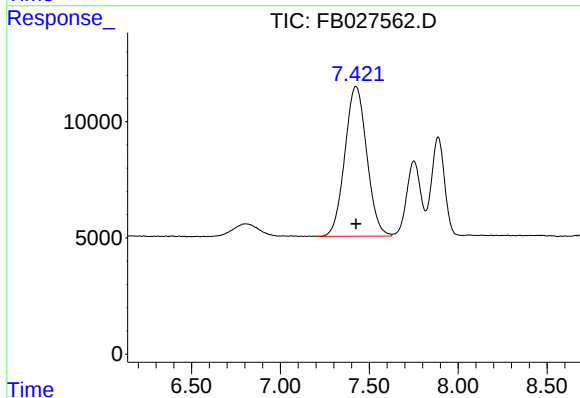


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: -0.002 min
Response: 552518
Conc: 31.47 ng/ml

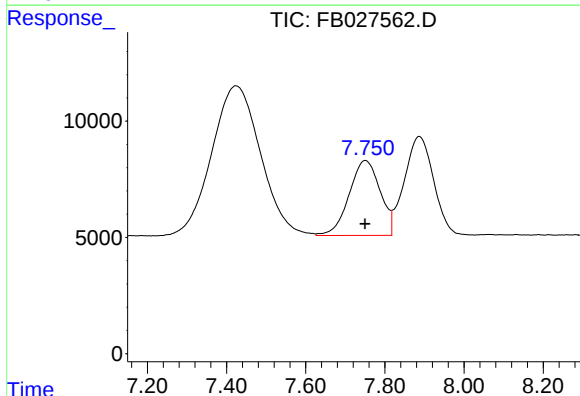


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.002 min
Response: 175314
Conc: 10.01 ng/ml

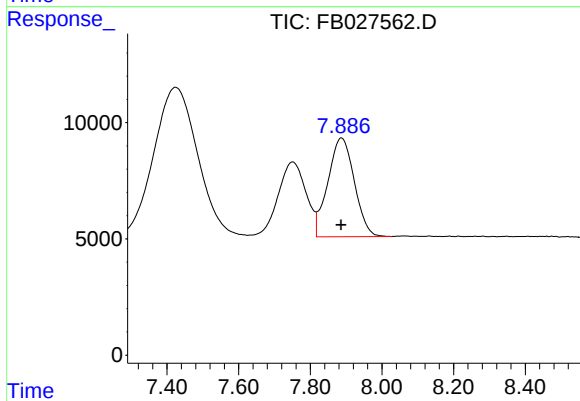

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.002 min
Response: 218081
Conc: 10.69 ng/ml

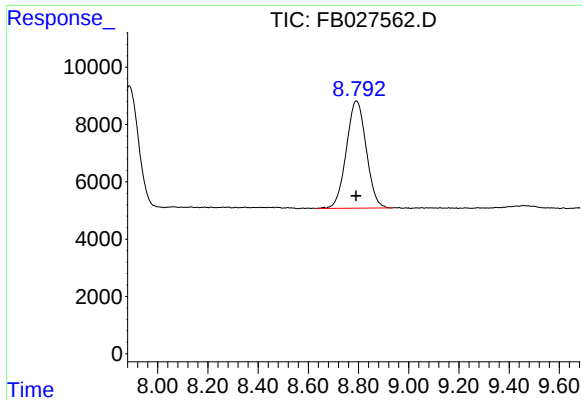

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.002 min
Response: 206060
Conc: 18.37 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0627S3

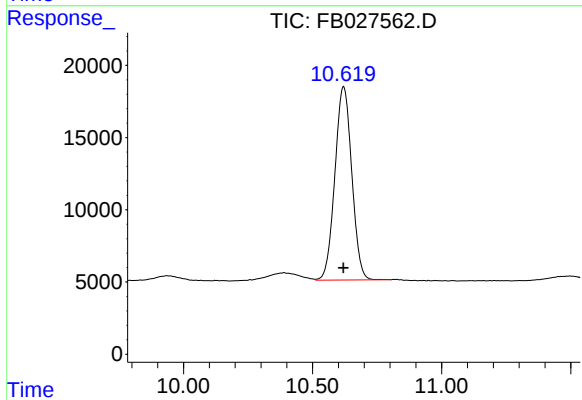


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.001 min
Response: 607903
Conc: 31.40 ng/ml

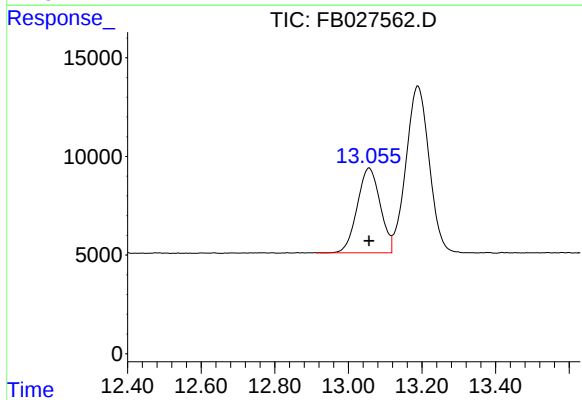


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 186086
Conc: 10.28 ng/ml

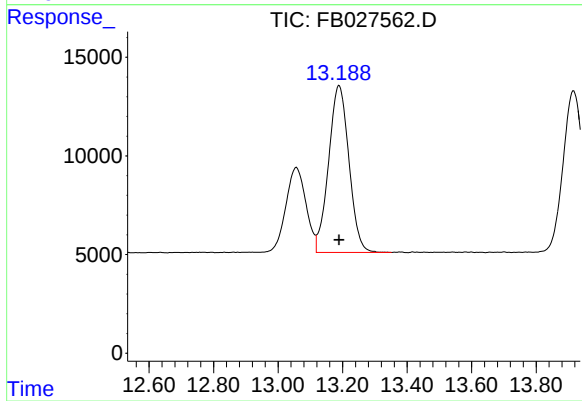

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 370358
Conc: 20.78 ng/ml

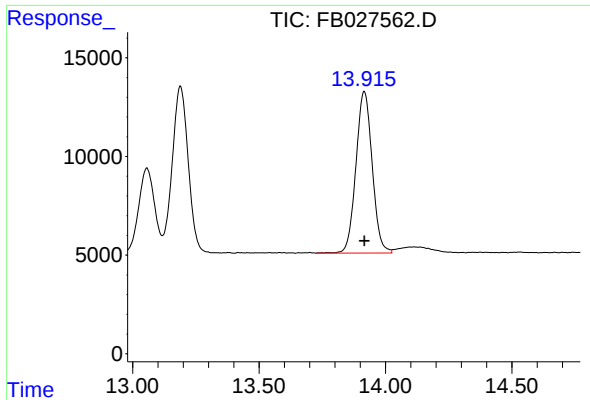

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: 0.000 min
Response: 365805
Conc: 21.05 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0627S3

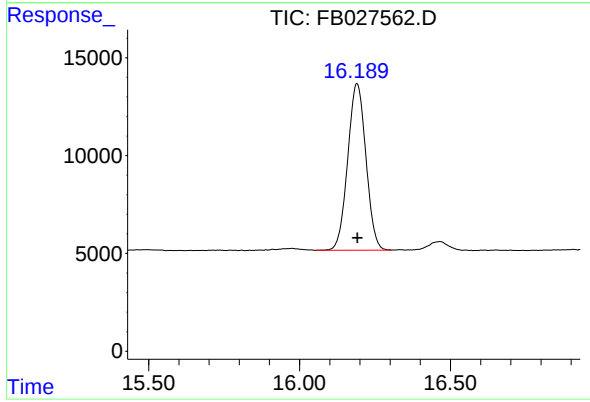

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 357404
Conc: 20.81 ng/ml