

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062725\
 Data File : FB031954.D
 Signal(s) : FID2B.CH
 Acq On : 27 Jun 2025 14:36
 Operator : YP/AJ
 Sample : BSF0627S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0627S2

Integration File: Calibration.e
 Quant Time: Jun 28 05:15:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
 Quant Title :
 QLast Update : Mon Jun 23 13:56:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.796	301517	19.544 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.712	728192	28.623 ng/ml
2) t	2,2,4-Trimethylpentane	7.422	881562	32.689 ng/ml
3) t	n-Heptane	7.755	262010	10.501 ng/ml
4) t	Benzene	7.894	346114	10.180 ng/ml
6) t	Toluene	10.624	1061616	29.689 ng/ml
7) t	Ethylbenzene	13.060	311796	9.874 ng/ml
8) t	m-Xylene	13.193	653267	19.917 ng/ml
9) t	O-Xylene	13.920	620265	19.984 ng/ml
10) t	1,2,4-Trimethylbenzene	16.195	520731	19.694 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062725\
Data File : FB031954.D
Signal(s) : FID2B.CH
Acq On : 27 Jun 2025 14:36
Operator : YP/AJ
Sample : BSF0627S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0627S2

Integration File: Calibration.e
Quant Time: Jun 28 05:15:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

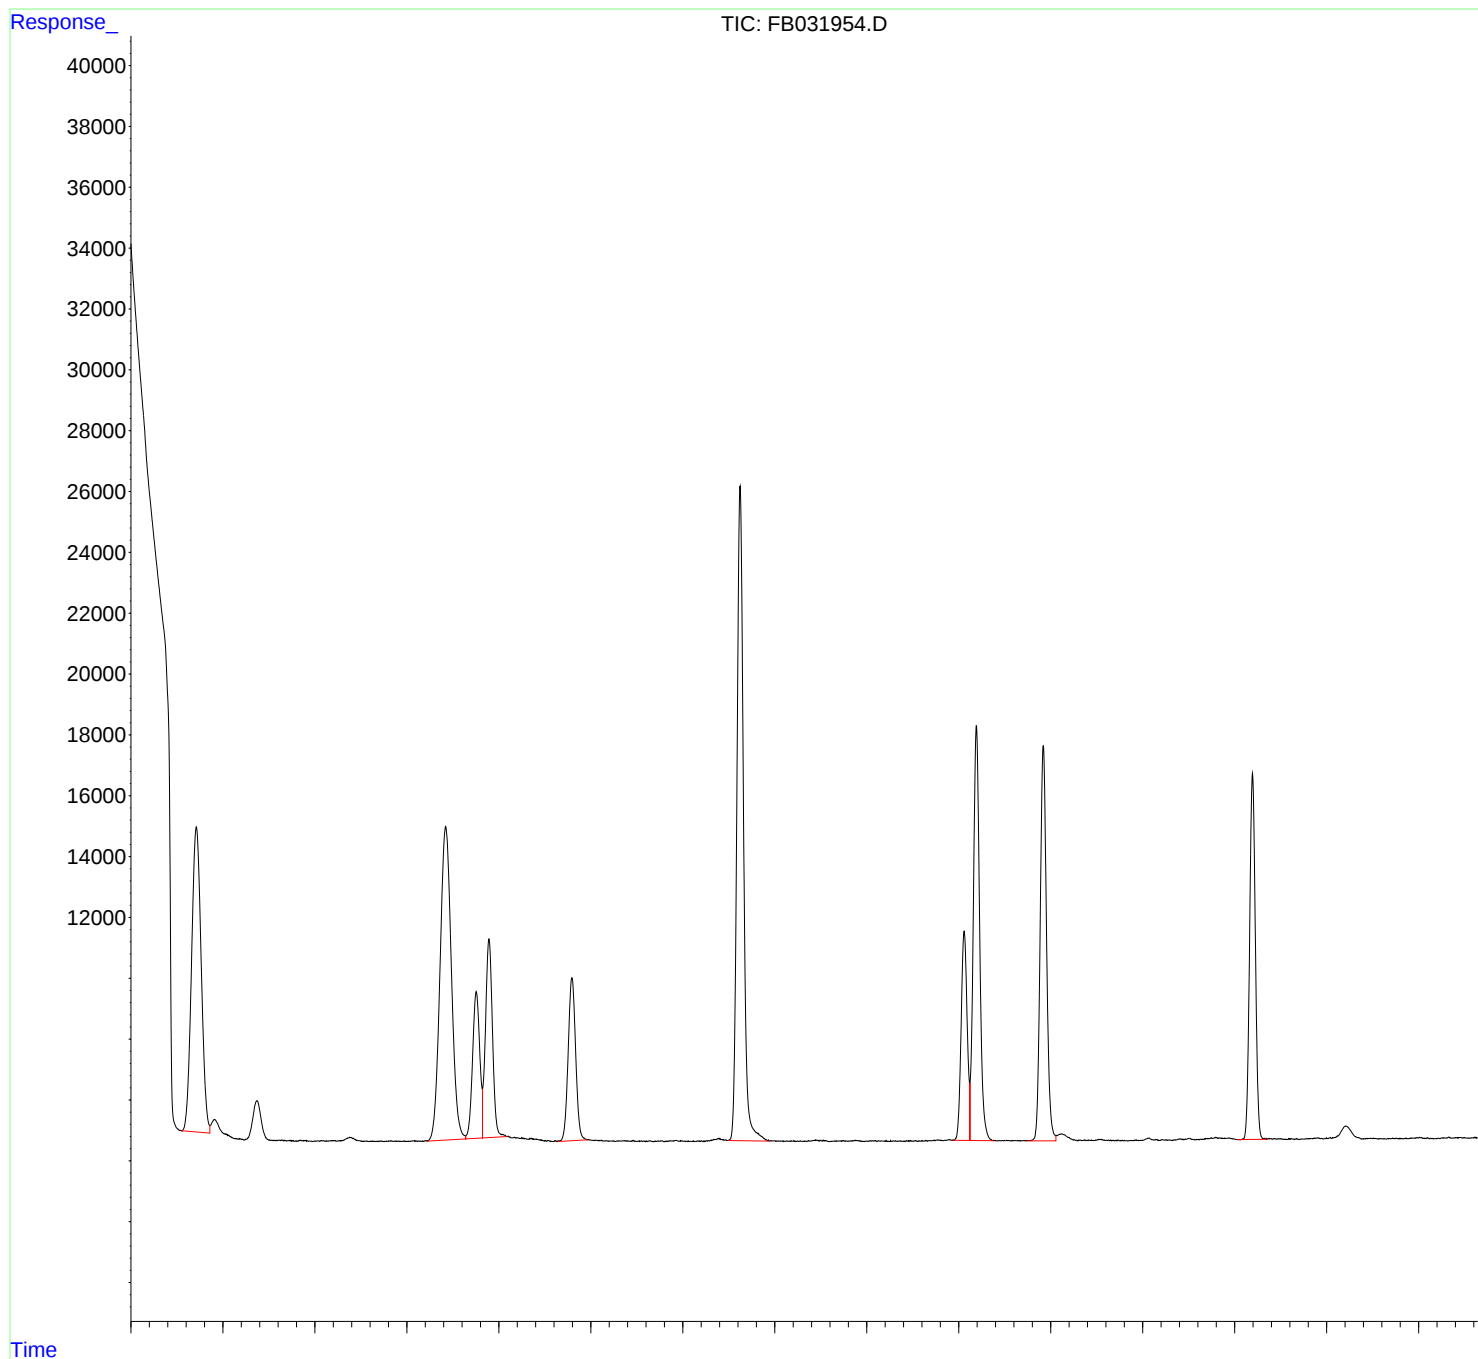


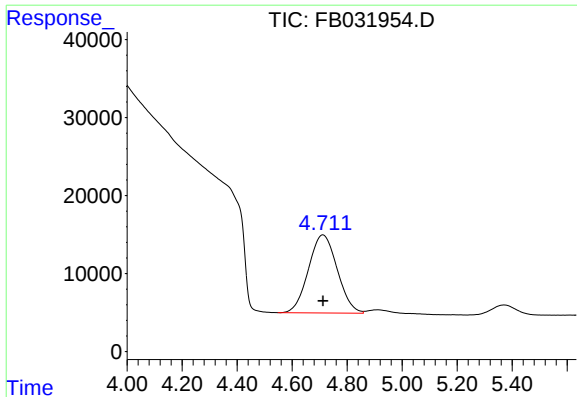

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.000 min
Response: 728192
Conc: 28.62 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0627S2

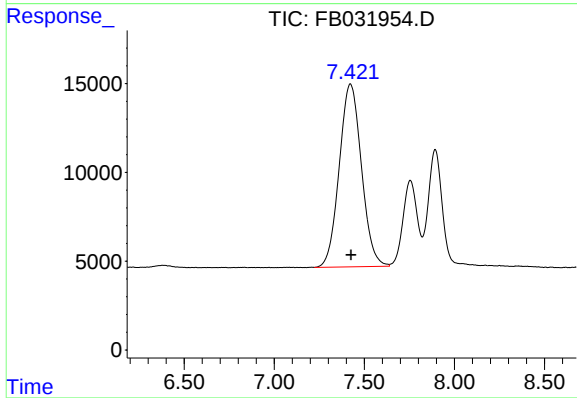


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: -0.003 min
Response: 881562
Conc: 32.69 ng/ml

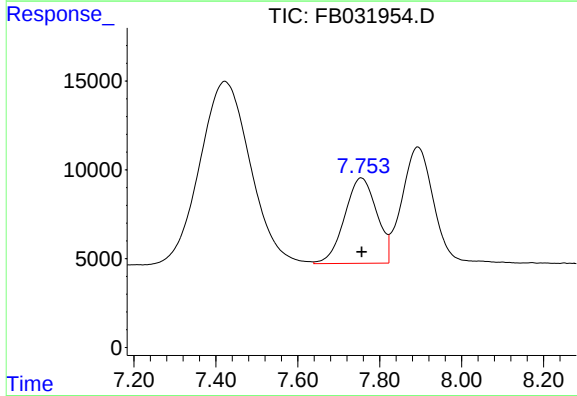


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 262010
Conc: 10.50 ng/ml

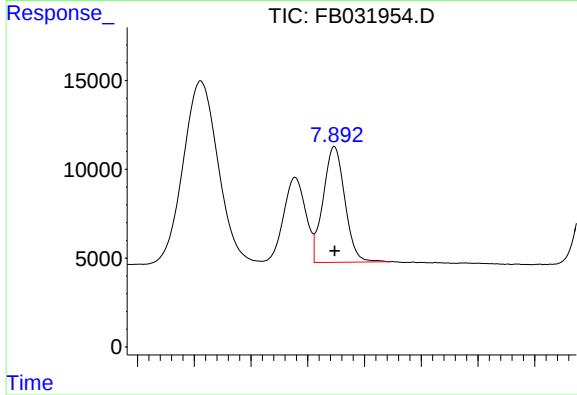

#4 Benzene


R.T.: 7.894 min
Delta R.T.: -0.002 min
Response: 346114
Conc: 10.18 ng/ml

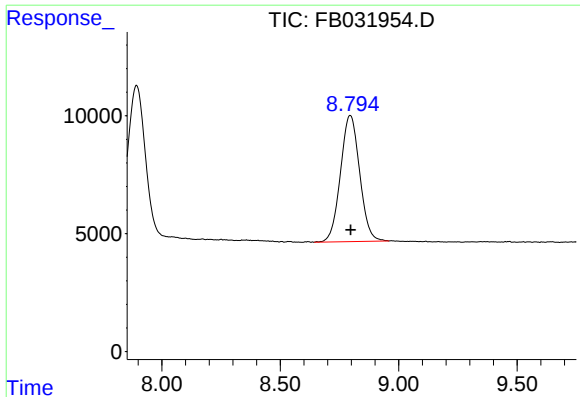

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.002 min
Response: 301517
Conc: 19.54 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0627S2

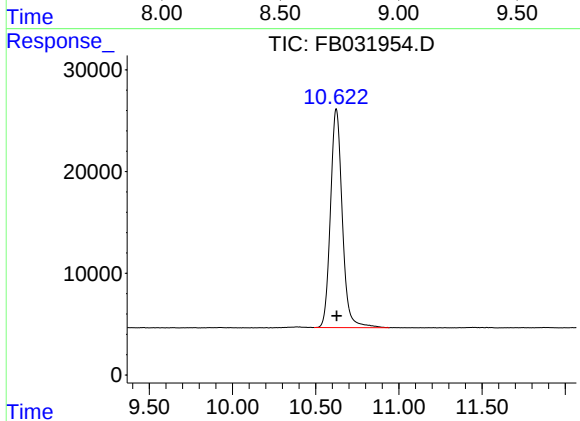


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.003 min
Response: 1061616
Conc: 29.69 ng/ml

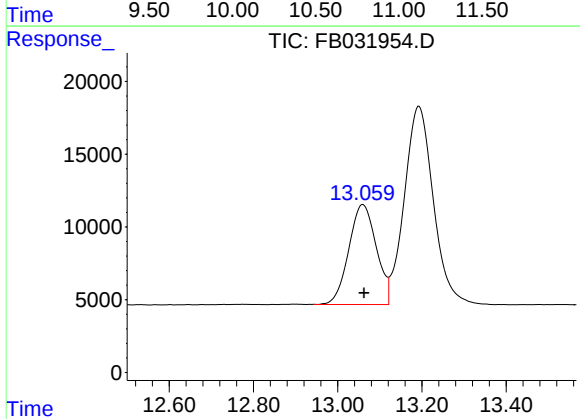


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: -0.003 min
Response: 311796
Conc: 9.87 ng/ml

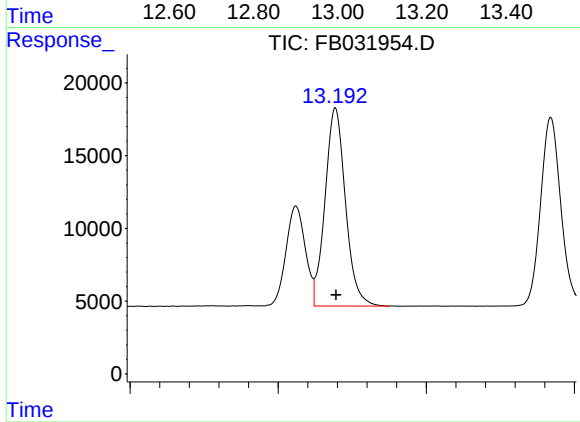

#8 m-Xylene


R.T.: 13.193 min
Delta R.T.: -0.003 min
Response: 653267
Conc: 19.92 ng/ml

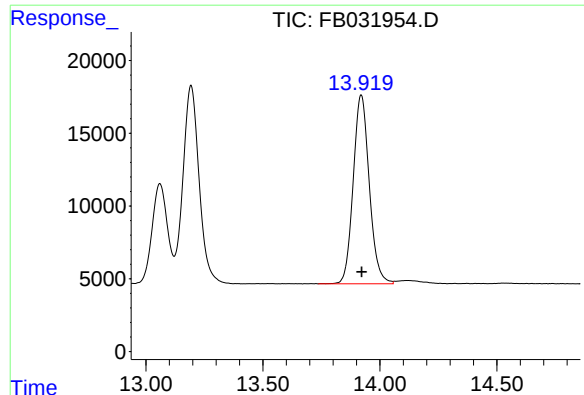

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: -0.002 min
Response: 620265
Conc: 19.98 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0627S2

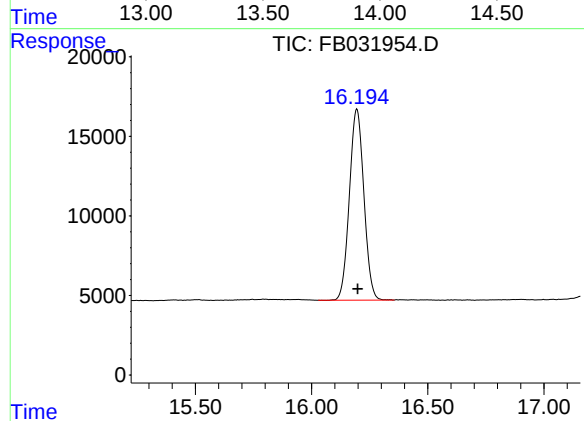

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: -0.003 min
Response: 520731
Conc: 19.69 ng/ml