

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062819\
 Data File : FB021553.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2019 9:02
 Operator : MJ/SJ
 Sample : BSF0628S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0628S1

Integration File: Calibration.e
 Quant Time: Jun 28 23:24:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.988	279870	20.241 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	988390	28.953 ng/ml
2) t 2,2,4-Trimethylpentane	7.608	941195	30.457 ng/ml
3) t n-Heptane	7.947	297448	10.163 ng/ml
4) t Benzene	8.082	338218	10.077 ng/ml
6) t Toluene	10.828	704302	30.833 ng/ml
7) t Ethylbenzene	13.273	243600	10.290 ng/ml
8) t m-Xylene	13.406	518556	20.459 ng/ml
9) t O-Xylene	14.135	530337	20.221 ng/ml
10) t 1,2,4-Trimethylbenzene	16.414	535244	20.372 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062819\
Data File : FB021553.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2019 9:02
Operator : MJ/SJ
Sample : BSF0628S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0628S1

Integration File: Calibration.e
Quant Time: Jun 28 23:24:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

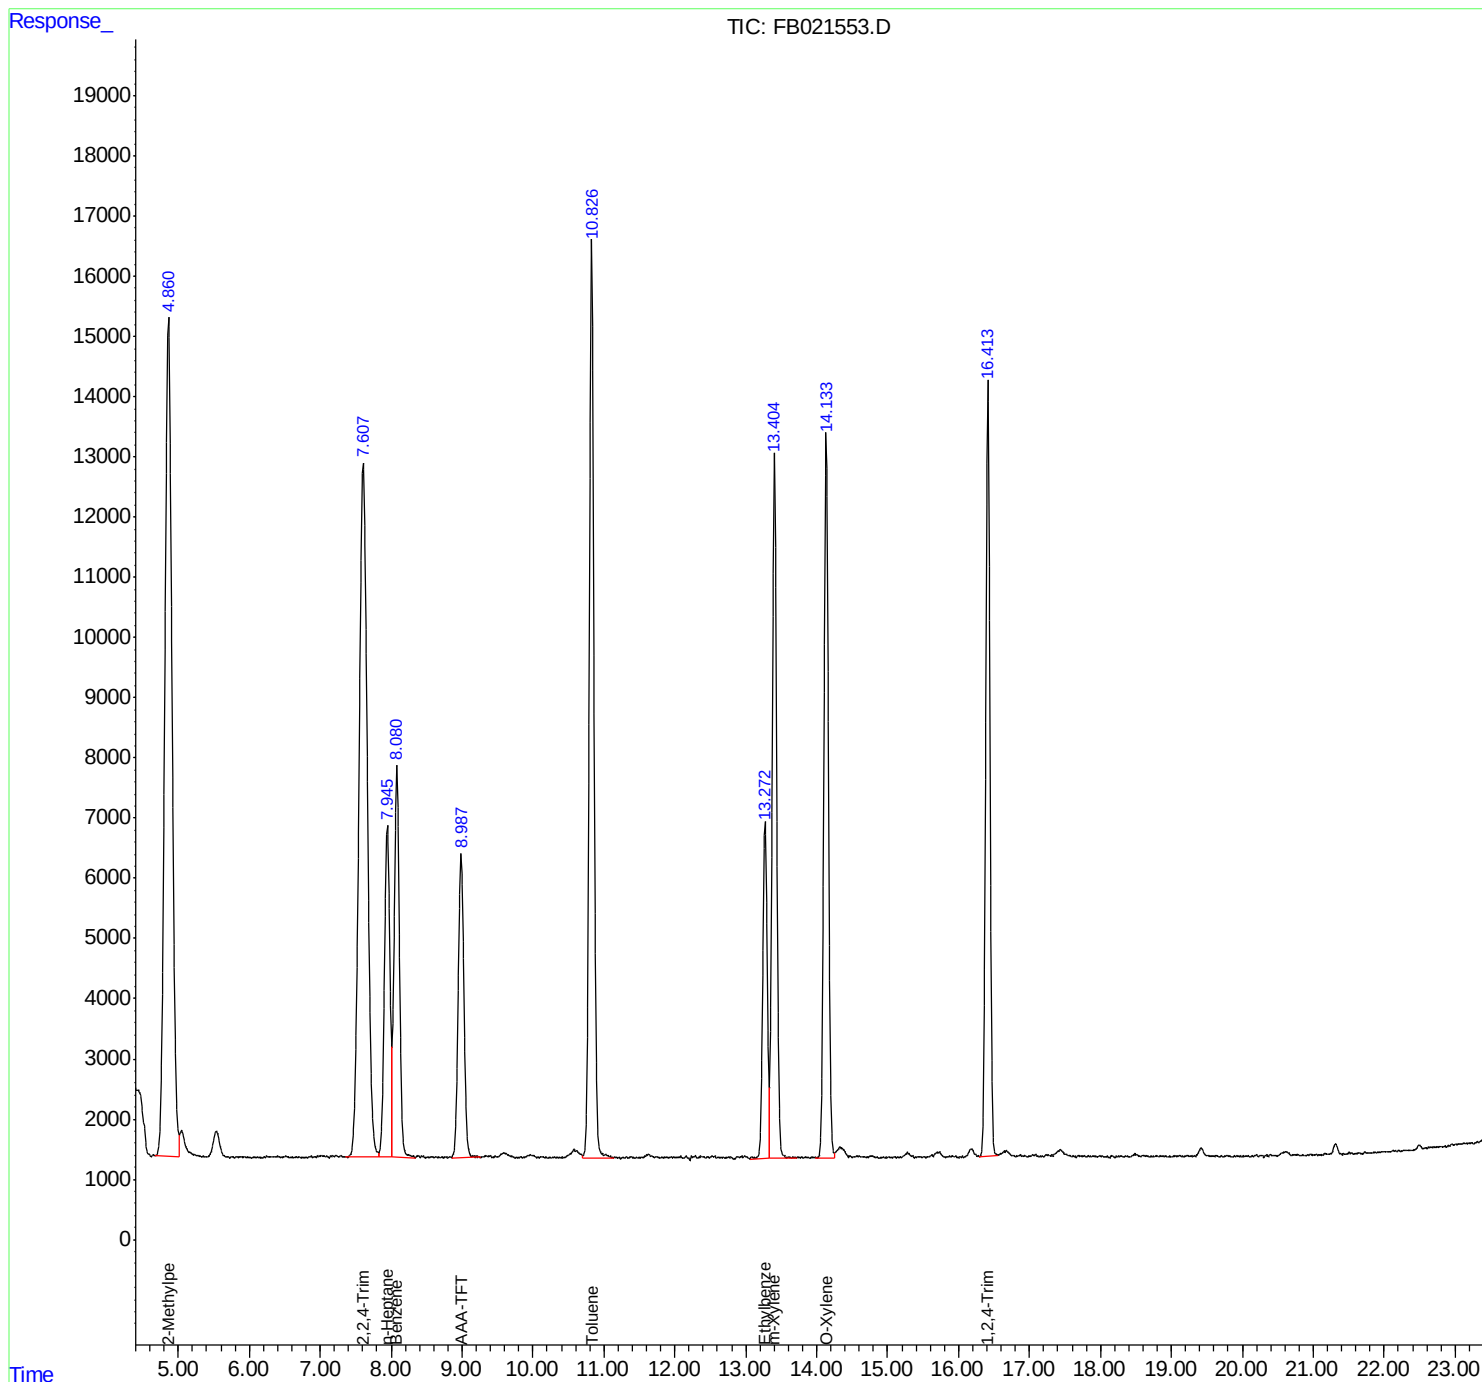


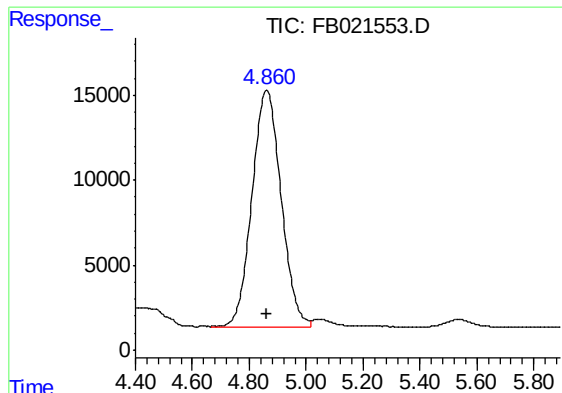

#1 2-Methylpentane


R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 988390
Conc: 28.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0628S1

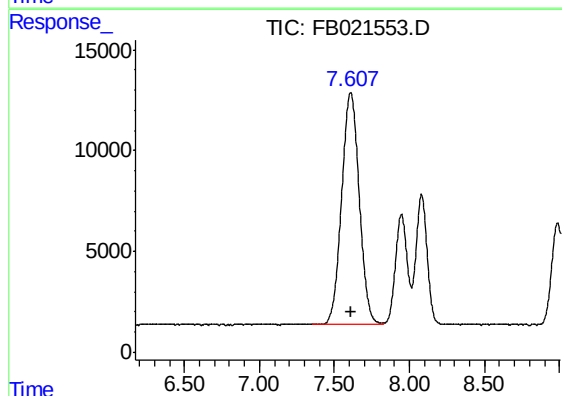


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 941195
Conc: 30.46 ng/ml

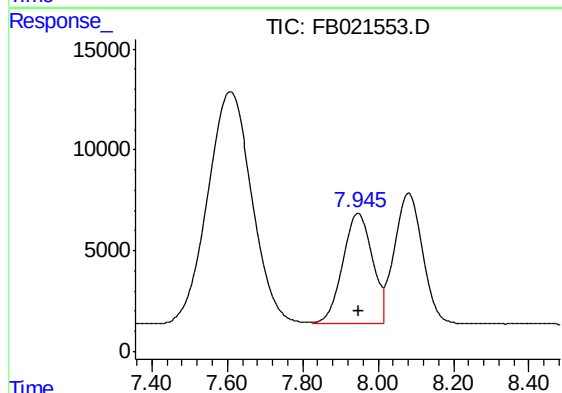


#3 n-Heptane

R.T.: 7.947 min
Delta R.T.: -0.001 min
Response: 297448
Conc: 10.16 ng/ml

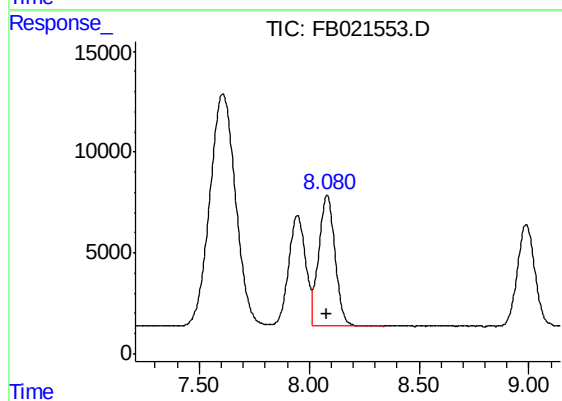

#4 Benzene


R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 338218
Conc: 10.08 ng/ml

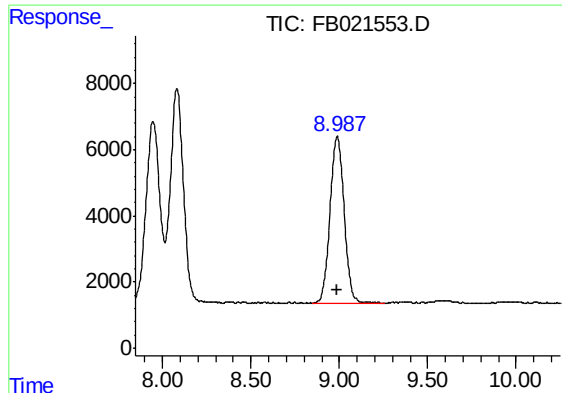

#5 AAA-TFT


R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 279870
Conc: 20.24 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0628S1

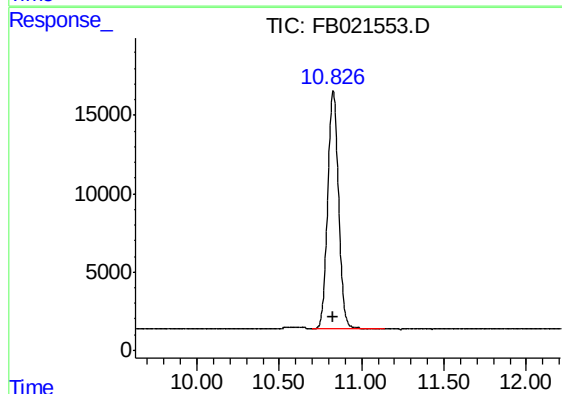


#6 Toluene

R.T.: 10.828 min
Delta R.T.: -0.002 min
Response: 704302
Conc: 30.83 ng/ml

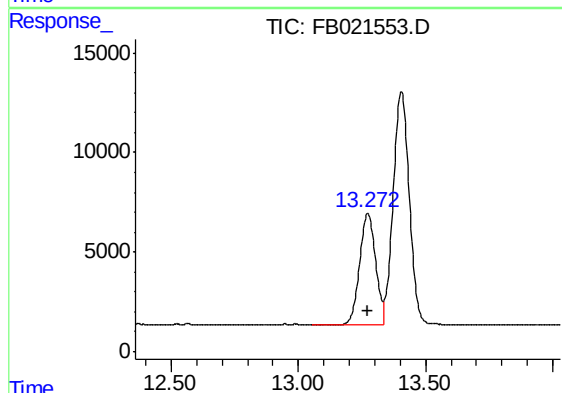


#7 Ethylbenzene

R.T.: 13.273 min
Delta R.T.: -0.002 min
Response: 243600
Conc: 10.29 ng/ml

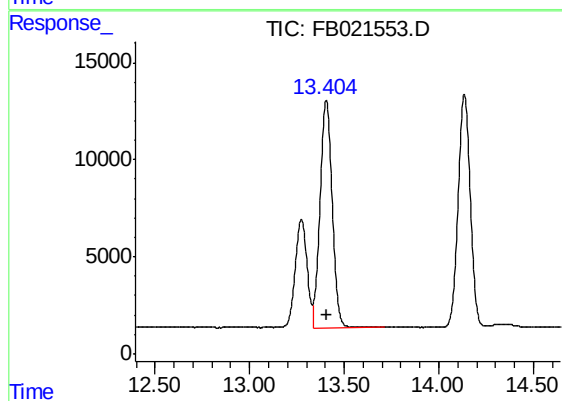

#8 m-Xylene


R.T.: 13.406 min
Delta R.T.: -0.002 min
Response: 518556
Conc: 20.46 ng/ml

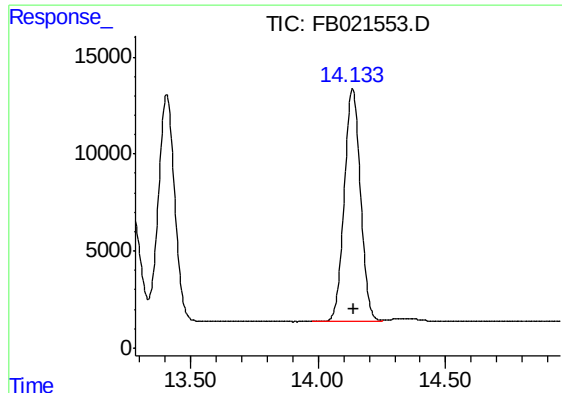

#9 O-Xylene

R.T.: 14.135 min
Delta R.T.: -0.002 min
Response: 530337
Conc: 20.22 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0628S1

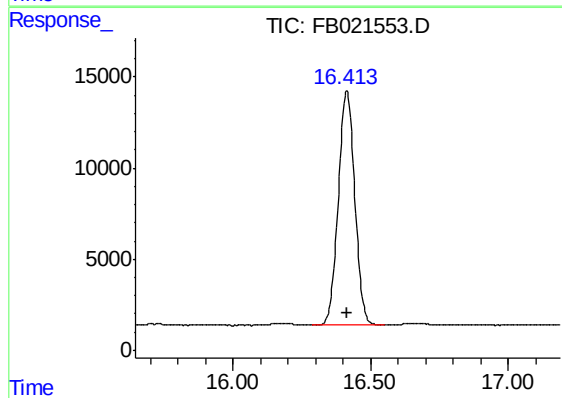

#10 1,2,4-Trimethylbenzene

R.T.: 16.414 min
Delta R.T.: -0.003 min
Response: 535244
Conc: 20.37 ng/ml