

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062819\
 Data File : FB021560.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2019 12:41
 Operator : MJ/SJ
 Sample : K3158-07MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OK-02-062719MS

Integration File: Calibration.e
 Quant Time: Jun 28 23:25:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.988	264132	19.103 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	908101	26.601 ng/ml
2) t 2,2,4-Trimethylpentane	7.608	852200	27.577 ng/ml
3) t n-Heptane	7.948	267976	9.156 ng/ml
4) t Benzene	8.082	305992	9.117 ng/ml
6) t Toluene	10.829	652479	28.564 ng/ml
7) t Ethylbenzene	13.274	226694	9.576 ng/ml
8) t m-Xylene	13.406	488502	19.273 ng/ml
9) t O-Xylene	14.136	503662	19.204 ng/ml
10) t 1,2,4-Trimethylbenzene	16.415	509696	19.399 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062819\
Data File : FB021560.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2019 12:41
Operator : MJ/SJ
Sample : K3158-07MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OK-02-062719MS

Integration File: Calibration.e
Quant Time: Jun 28 23:25:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

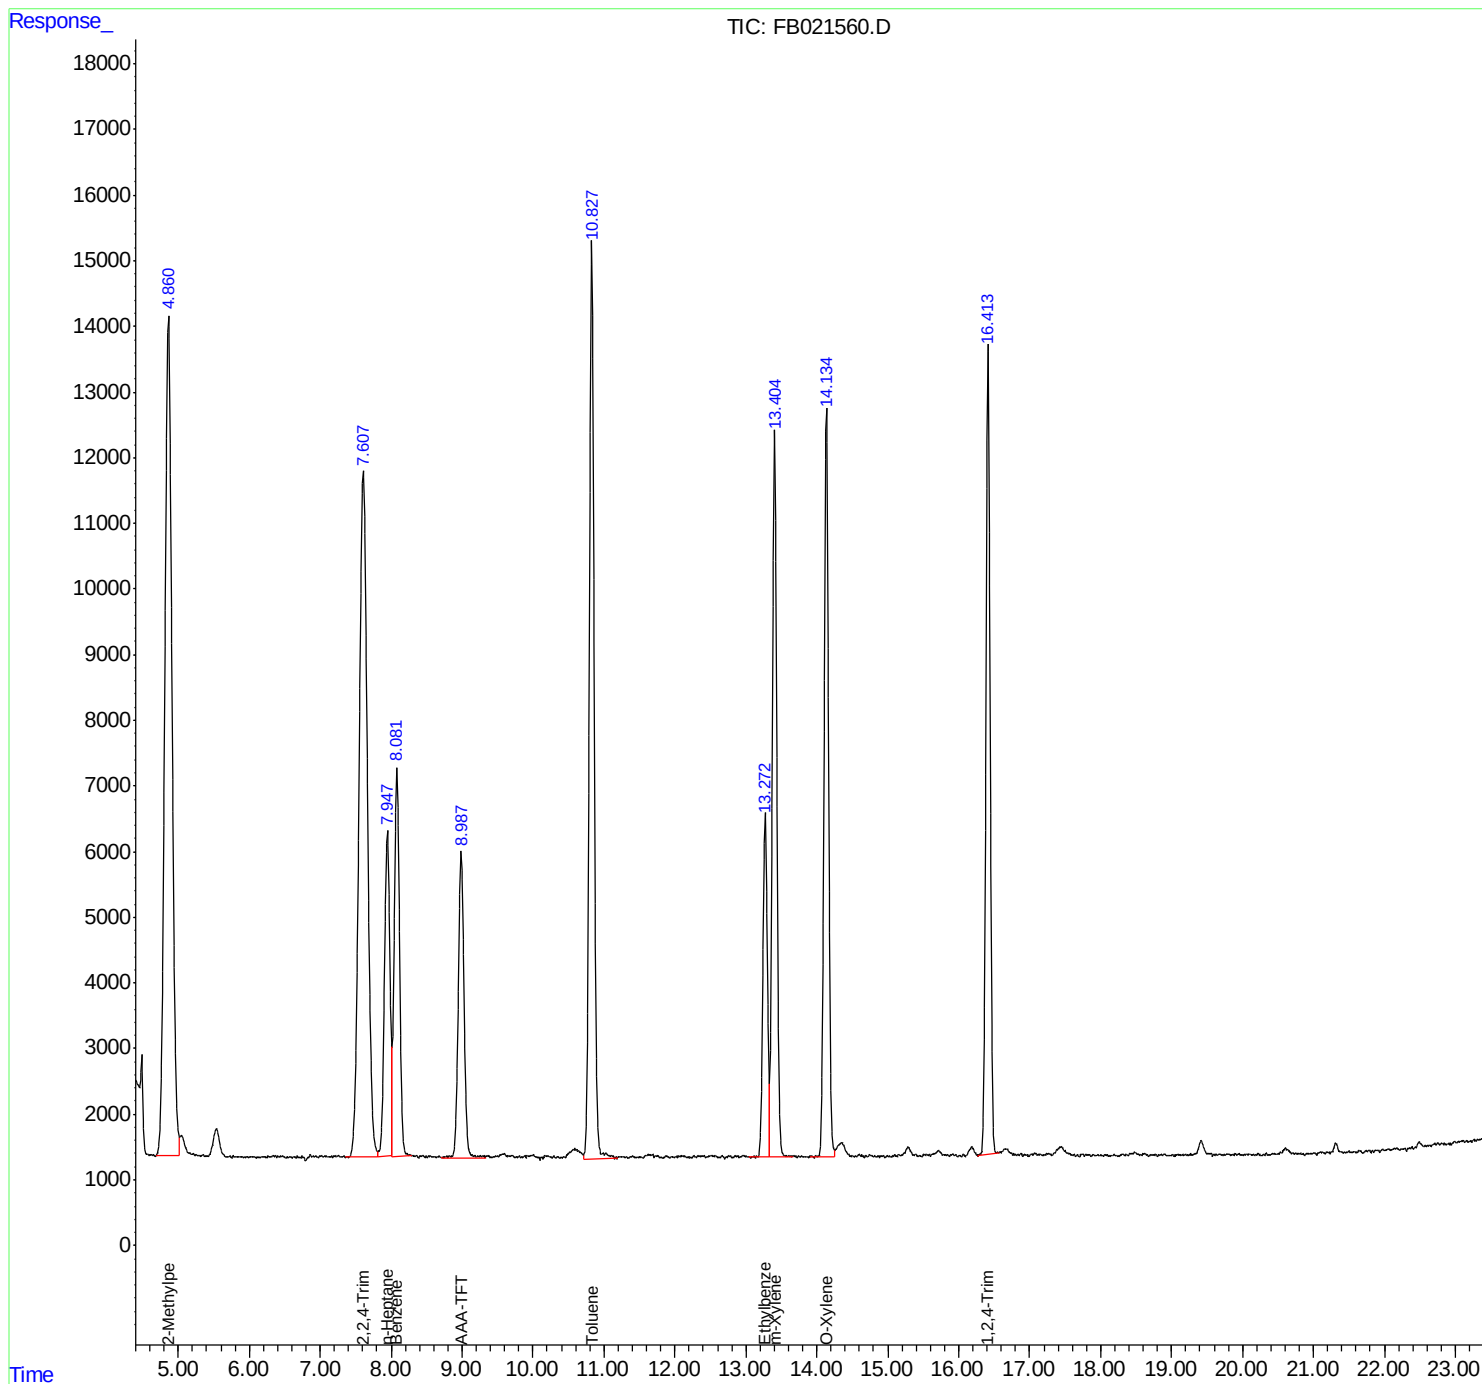


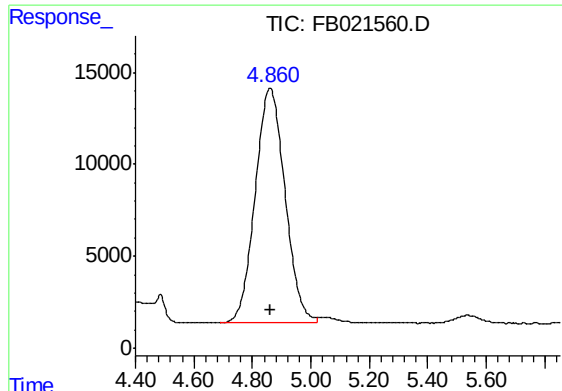

#1 2-Methylpentane


R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 908101
Conc: 26.60 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-062719MS

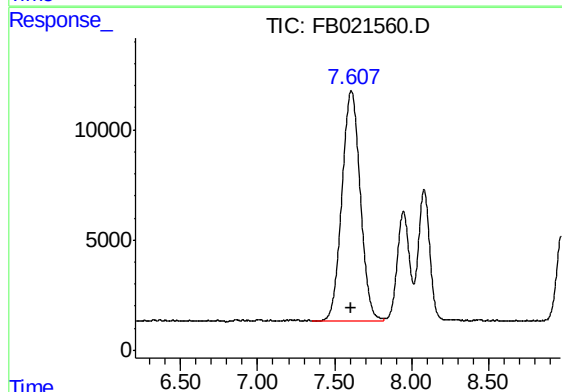


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 852200
Conc: 27.58 ng/ml

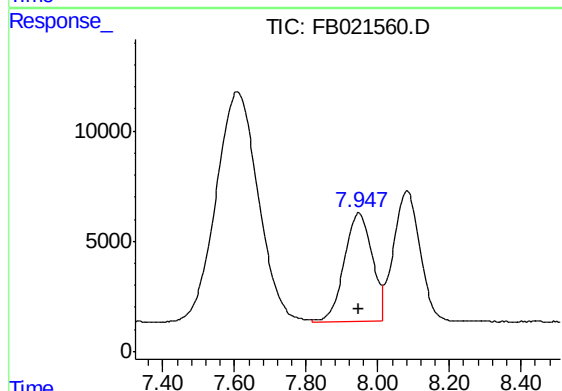


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: 0.000 min
Response: 267976
Conc: 9.16 ng/ml

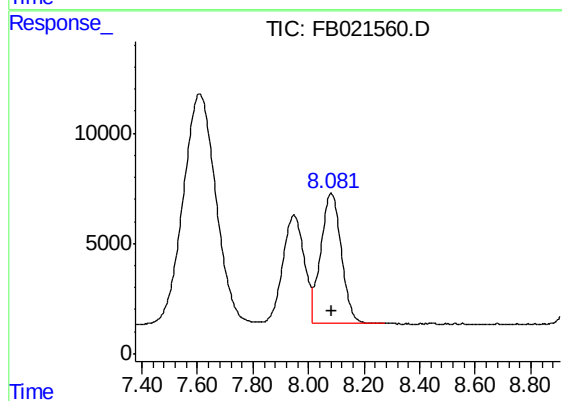

#4 Benzene


R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 305992
Conc: 9.12 ng/ml

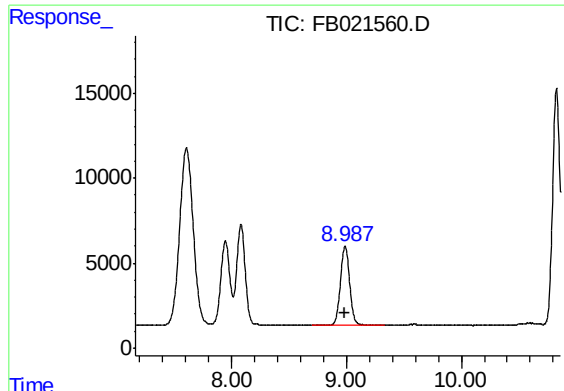

#5 AAA-TFT


R.T.: 8.988 min
Delta R.T.: 0.000 min
Response: 264132
Conc: 19.10 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-062719MS

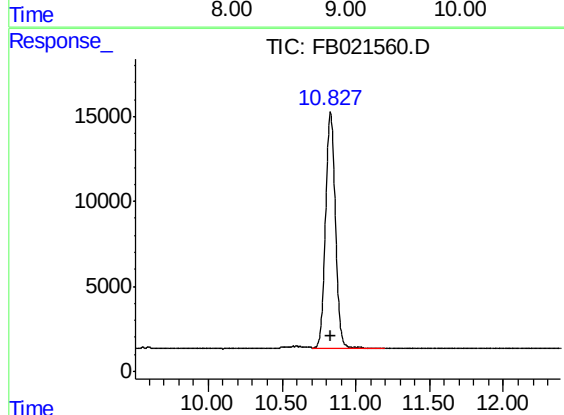


#6 Toluene

R.T.: 10.829 min
Delta R.T.: 0.000 min
Response: 652479
Conc: 28.56 ng/ml

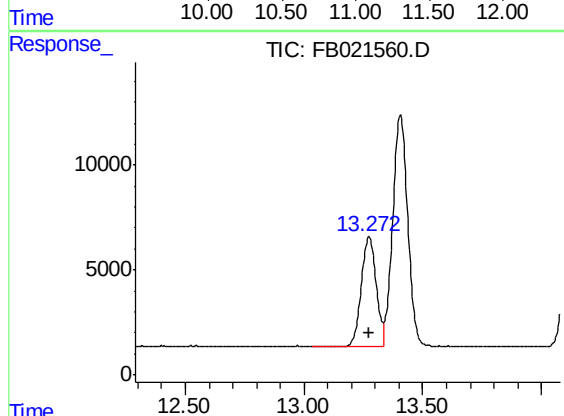


#7 Ethylbenzene

R.T.: 13.274 min
Delta R.T.: -0.001 min
Response: 226694
Conc: 9.58 ng/ml

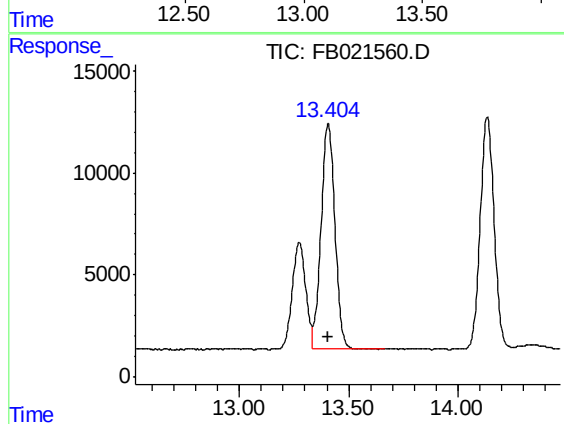

#8 m-Xylene


R.T.: 13.406 min
Delta R.T.: -0.002 min
Response: 488502
Conc: 19.27 ng/ml

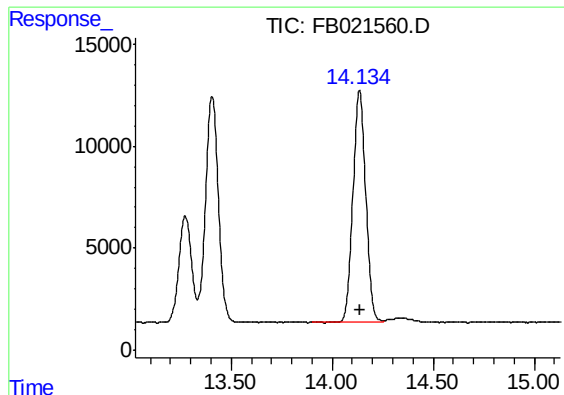

#9 O-Xylene

R.T.: 14.136 min
Delta R.T.: -0.002 min
Response: 503662
Conc: 19.20 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-062719MS

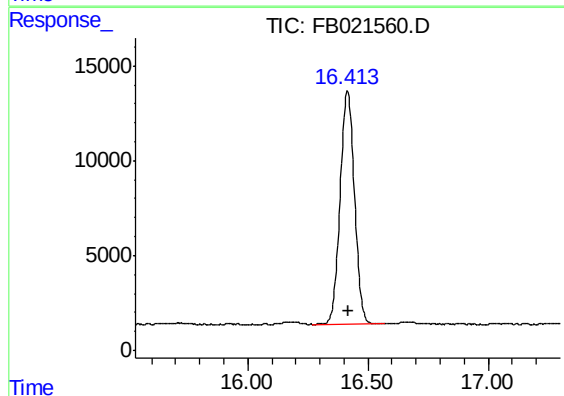

#10 1,2,4-Trimethylbenzene

R.T.: 16.415 min
Delta R.T.: -0.002 min
Response: 509696
Conc: 19.40 ng/ml