

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062821\
 Data File : FB025923.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2021 11:38
 Operator : AJ/MA
 Sample : BSF0628S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 28 14:14:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.226	397356	16.442 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.193	735087	27.932 ng/ml
2) t 2,2,4-Trimethylpentane	7.885	608741	30.218 ng/ml
3) t n-Heptane	8.203	342065	9.516 ng/ml
4) t Benzene	8.353	385413	9.233 ng/ml
6) t Toluene	11.043	1071348	26.035 ng/ml
7) t Ethylbenzene	13.448	326695	8.572 ng/ml
8) t m-Xylene	13.578	633404	16.112 ng/ml
9) t O-Xylene	14.301	576530	18.082 ng/ml
10) t 1,2,4-Trimethylbenzene	16.552	344513	17.503 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062821\
Data File : FB025923.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2021 11:38
Operator : AJ/MA
Sample : BSF0628S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 28 14:14:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

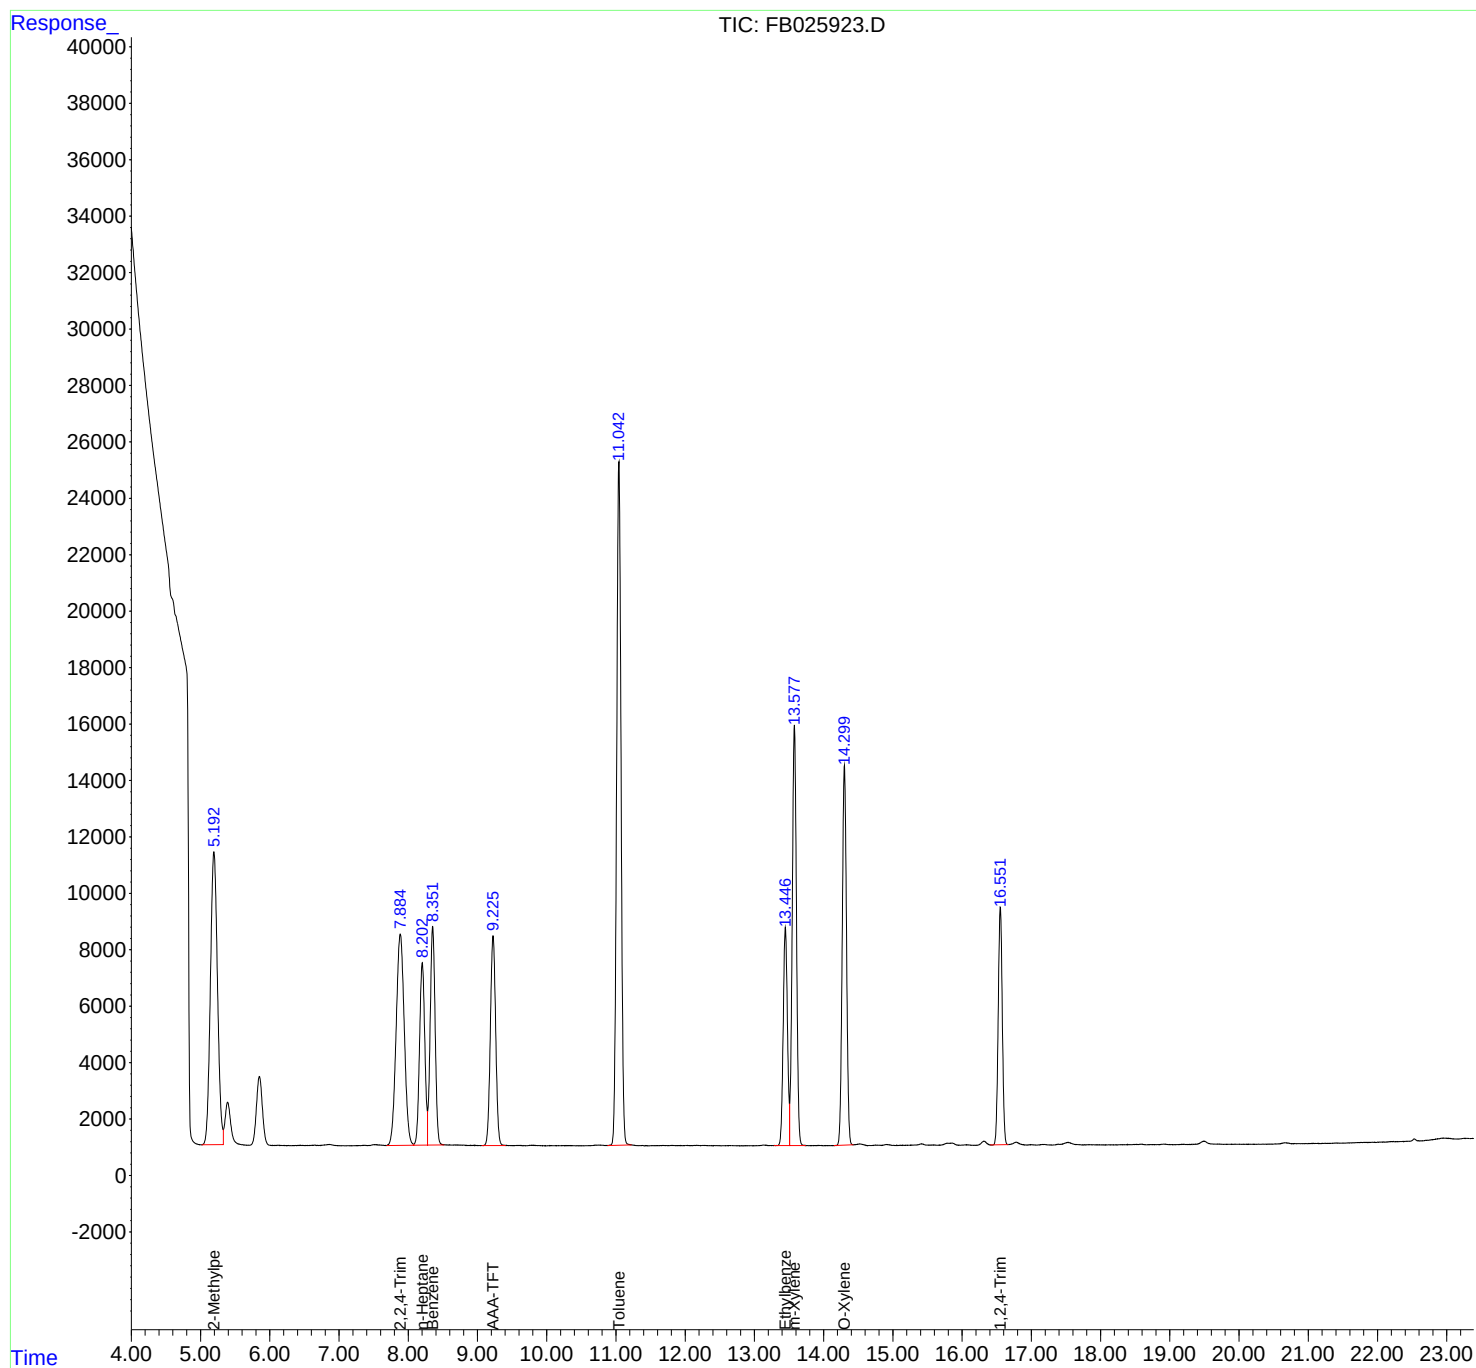

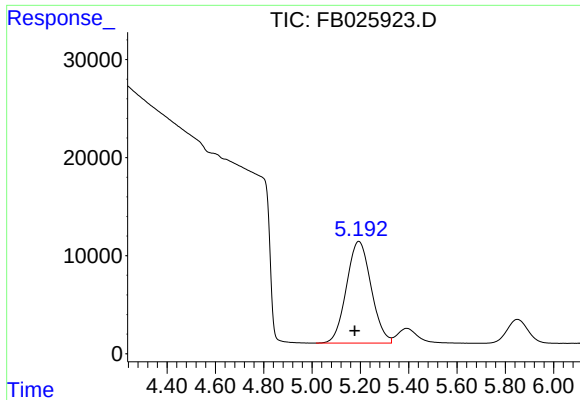


#1 2-Methylpentane

R.T.: 5.193 min
Delta R.T.: 0.016 min
Response: 735087
Conc: 27.93 ng/ml

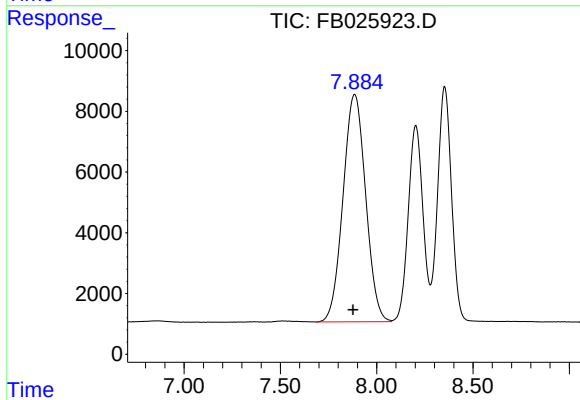


#2 2,2,4-Trimethylpentane

R.T.: 7.885 min
Delta R.T.: 0.007 min
Response: 608741
Conc: 30.22 ng/ml

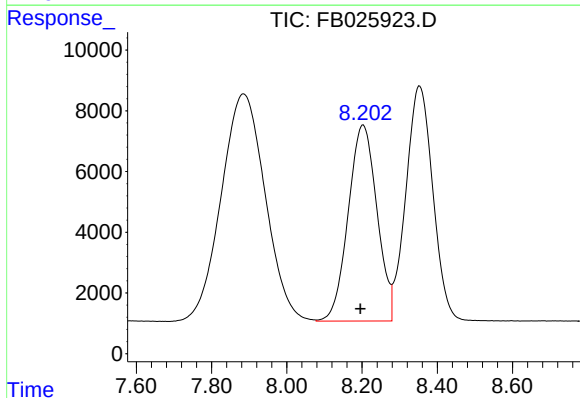


#3 n-Heptane

R.T.: 8.203 min
Delta R.T.: 0.007 min
Response: 342065
Conc: 9.52 ng/ml

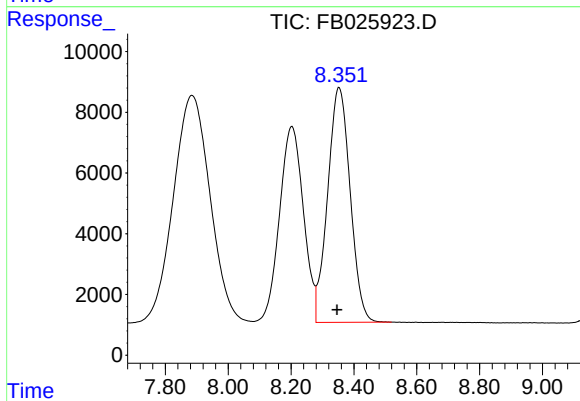


#4 Benzene

R.T.: 8.353 min
Delta R.T.: 0.007 min
Response: 385413
Conc: 9.23 ng/ml

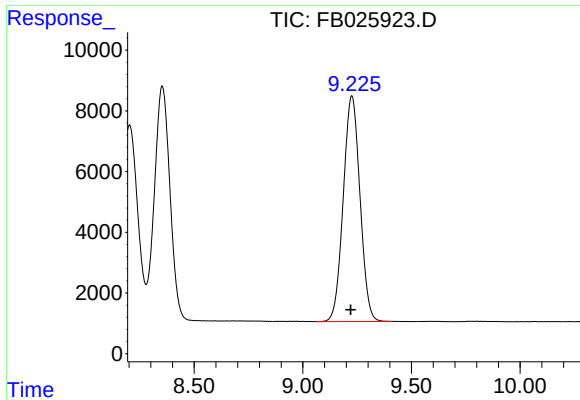


#5 AAA-TFT

R.T.: 9.226 min
Delta R.T.: 0.005 min
Response: 397356
Conc: 16.44 ng/ml

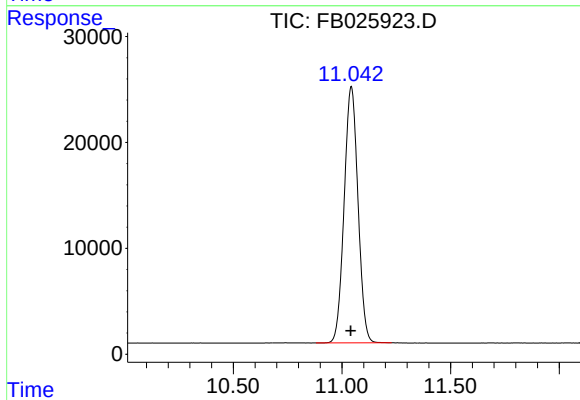


#6 Toluene

R.T.: 11.043 min
Delta R.T.: 0.002 min
Response: 1071348
Conc: 26.03 ng/ml

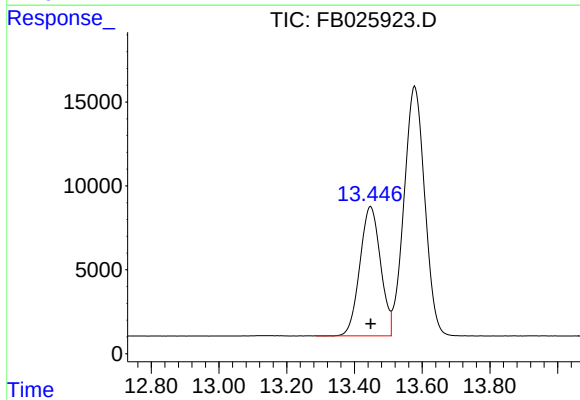


#7 Ethylbenzene

R.T.: 13.448 min
Delta R.T.: 0.000 min
Response: 326695
Conc: 8.57 ng/ml

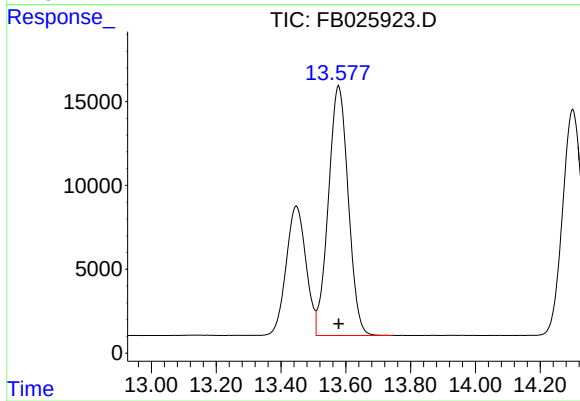


#8 m-Xylene

R.T.: 13.578 min
Delta R.T.: 0.000 min
Response: 633404
Conc: 16.11 ng/ml

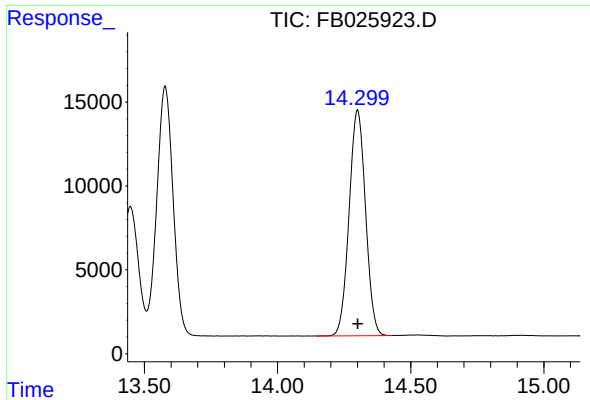

#9 O-Xylene

R.T.: 14.301 min
Delta R.T.: 0.000 min
Response: 576530
Conc: 18.08 ng/ml

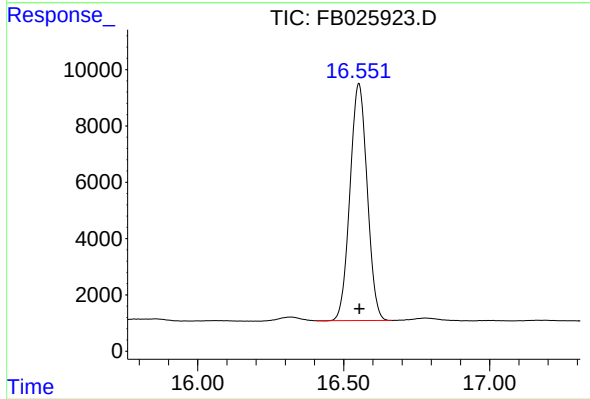

#10 1,2,4-Trimethylbenzene

R.T.: 16.552 min
Delta R.T.: -0.001 min
Response: 344513
Conc: 17.50 ng/ml