

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062821\
 Data File : FB025939.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2021 21:24
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc : 5.05g/5.00 ml DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 29 07:14:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.221	505069	20.899 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.170	704076	26.754 ng/ml
2) t 2,2,4-Trimethylpentane	7.877	542992	26.954 ng/ml
3) t n-Heptane	8.195	326127	9.073 ng/ml
4) t Benzene	8.345	362238	8.677 ng/ml
6) t Toluene	11.041	999757	24.295 ng/ml
7) t Ethylbenzene	13.449	302818	7.946 ng/ml
8) t m-Xylene	13.579	576475	14.664 ng/ml
9) t O-Xylene	14.302	522544	16.388 ng/ml
10) t 1,2,4-Trimethylbenzene	16.555	299838	15.234 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062821\
Data File : FB025939.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2021 21:24
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc : 5.05g/5.00 ml DI WATER
ALS Vial : 19 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 29 07:14:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

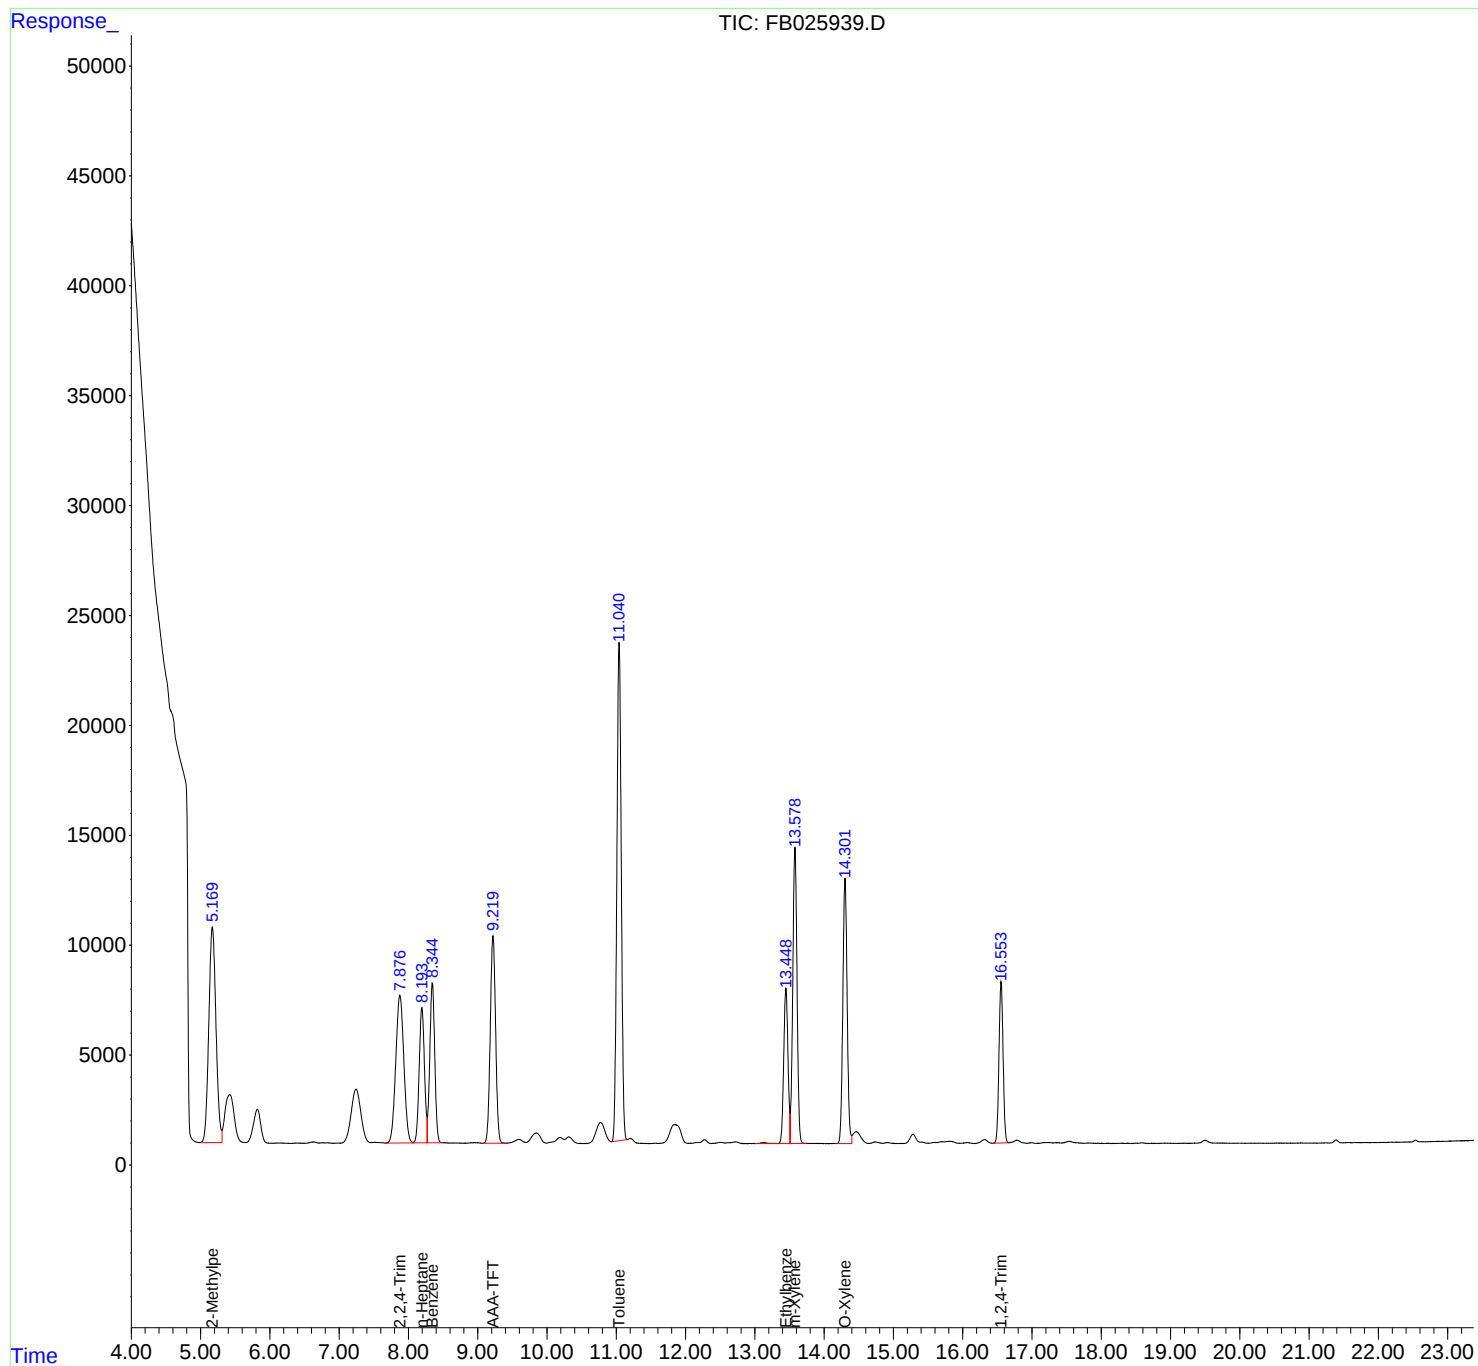

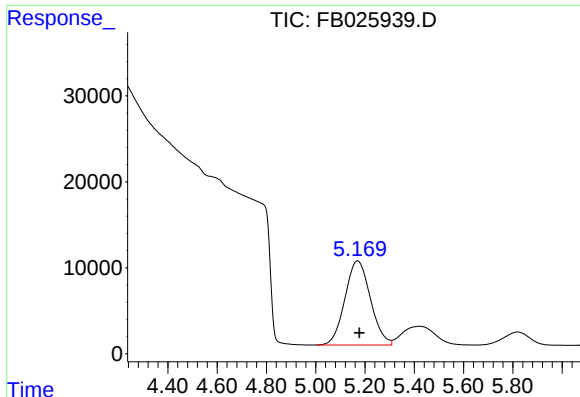


#1 2-Methylpentane

R.T.: 5.170 min
Delta R.T.: -0.007 min
Response: 704076
Conc: 26.75 ng/ml

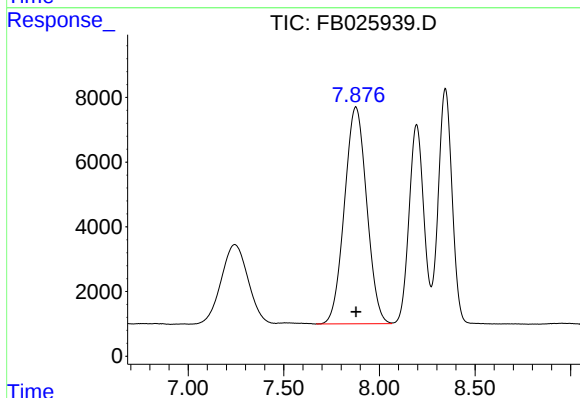


#2 2,2,4-Trimethylpentane

R.T.: 7.877 min
Delta R.T.: -0.001 min
Response: 542992
Conc: 26.95 ng/ml

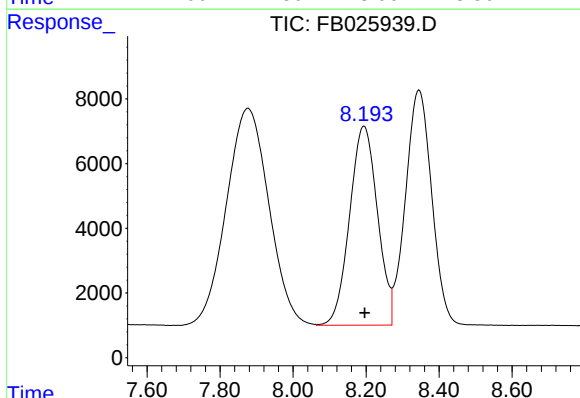


#3 n-Heptane

R.T.: 8.195 min
Delta R.T.: -0.001 min
Response: 326127
Conc: 9.07 ng/ml

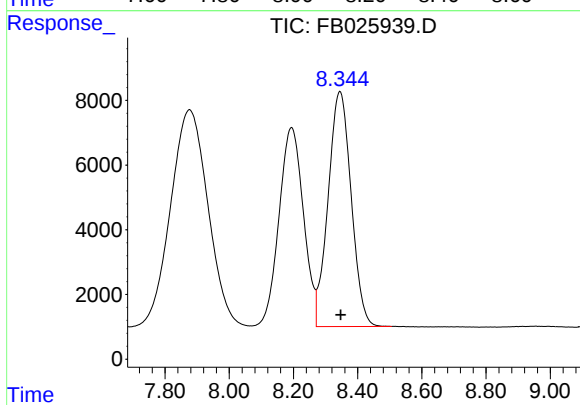


#4 Benzene

R.T.: 8.345 min
Delta R.T.: -0.001 min
Response: 362238
Conc: 8.68 ng/ml

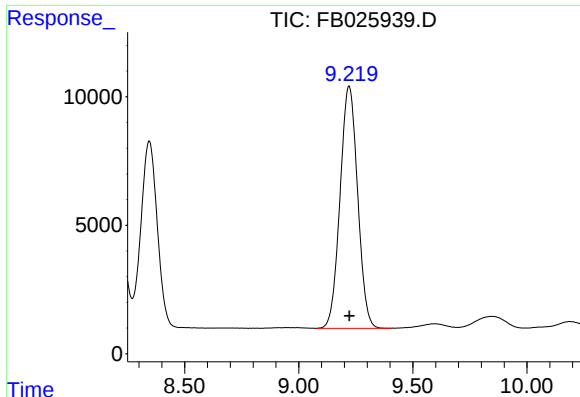


#5 AAA-TFT

R.T.: 9.221 min
Delta R.T.: 0.000 min
Response: 505069
Conc: 20.90 ng/ml

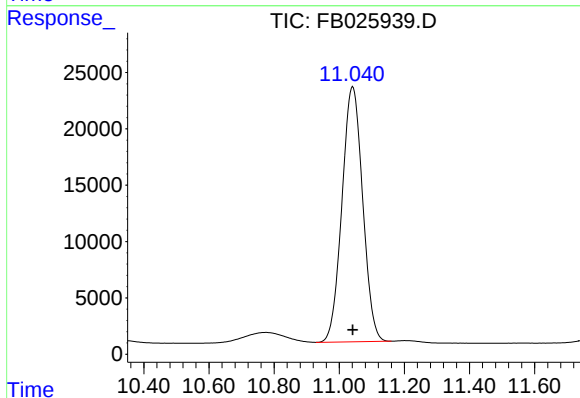


#6 Toluene

R.T.: 11.041 min
Delta R.T.: 0.000 min
Response: 999757
Conc: 24.29 ng/ml

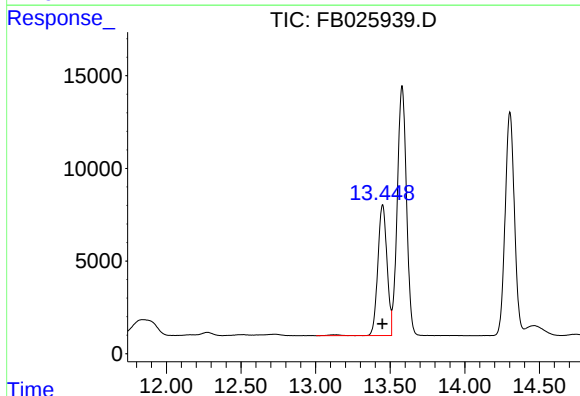


#7 Ethylbenzene

R.T.: 13.449 min
Delta R.T.: 0.000 min
Response: 302818
Conc: 7.95 ng/ml

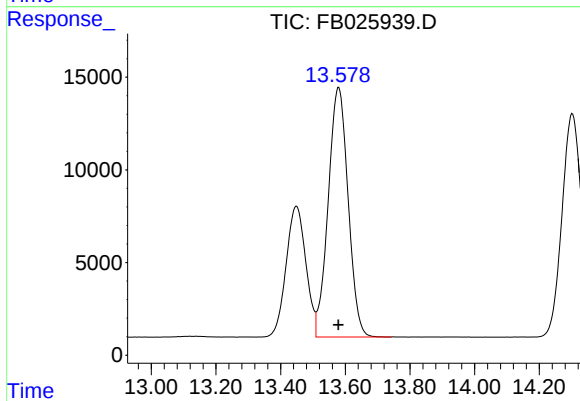

#8 m-Xylene

R.T.: 13.579 min
Delta R.T.: 0.000 min
Response: 576475
Conc: 14.66 ng/ml

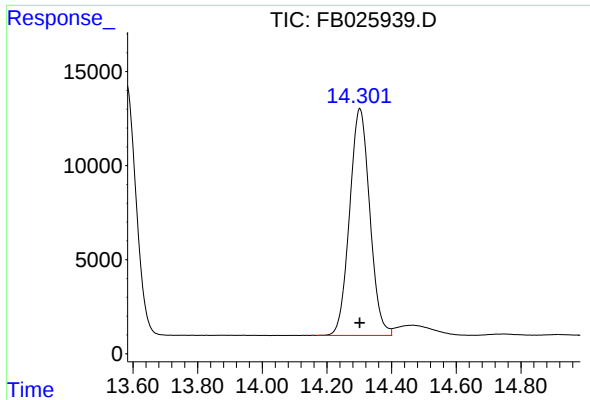


#9 O-Xylene

R.T.: 14.302 min

Delta R.T.: 0.001 min

Response: 522544

Conc: 16.39 ng/ml

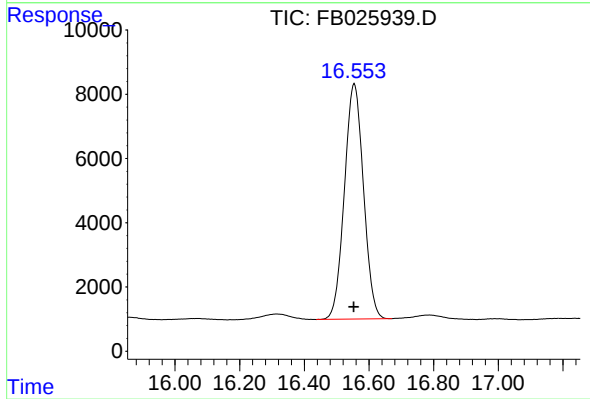

#10 1,2,4-Trimethylbenzene

R.T.: 16.555 min

Delta R.T.: 0.001 min

Response: 299838

Conc: 15.23 ng/ml