

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062822\
 Data File : FB027567.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2022 14:00
 Operator : AJ/MA
 Sample : BSF0628S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 29 03:35:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	274690	24.489 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	563134	33.426 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	573584	32.667 ng/ml
3) t n-Heptane	7.752	192964	11.015 ng/ml
4) t Benzene	7.888	220601	10.818 ng/ml
6) t Toluene	10.621	621200	32.083 ng/ml
7) t Ethylbenzene	13.057	192978	10.656 ng/ml
8) t m-Xylene	13.190	384555	21.573 ng/ml
9) t O-Xylene	13.917	372571	21.442 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	371315	21.615 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062822\
Data File : FB027567.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2022 14:00
Operator : AJ/MA
Sample : BSF0628S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 29 03:35:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

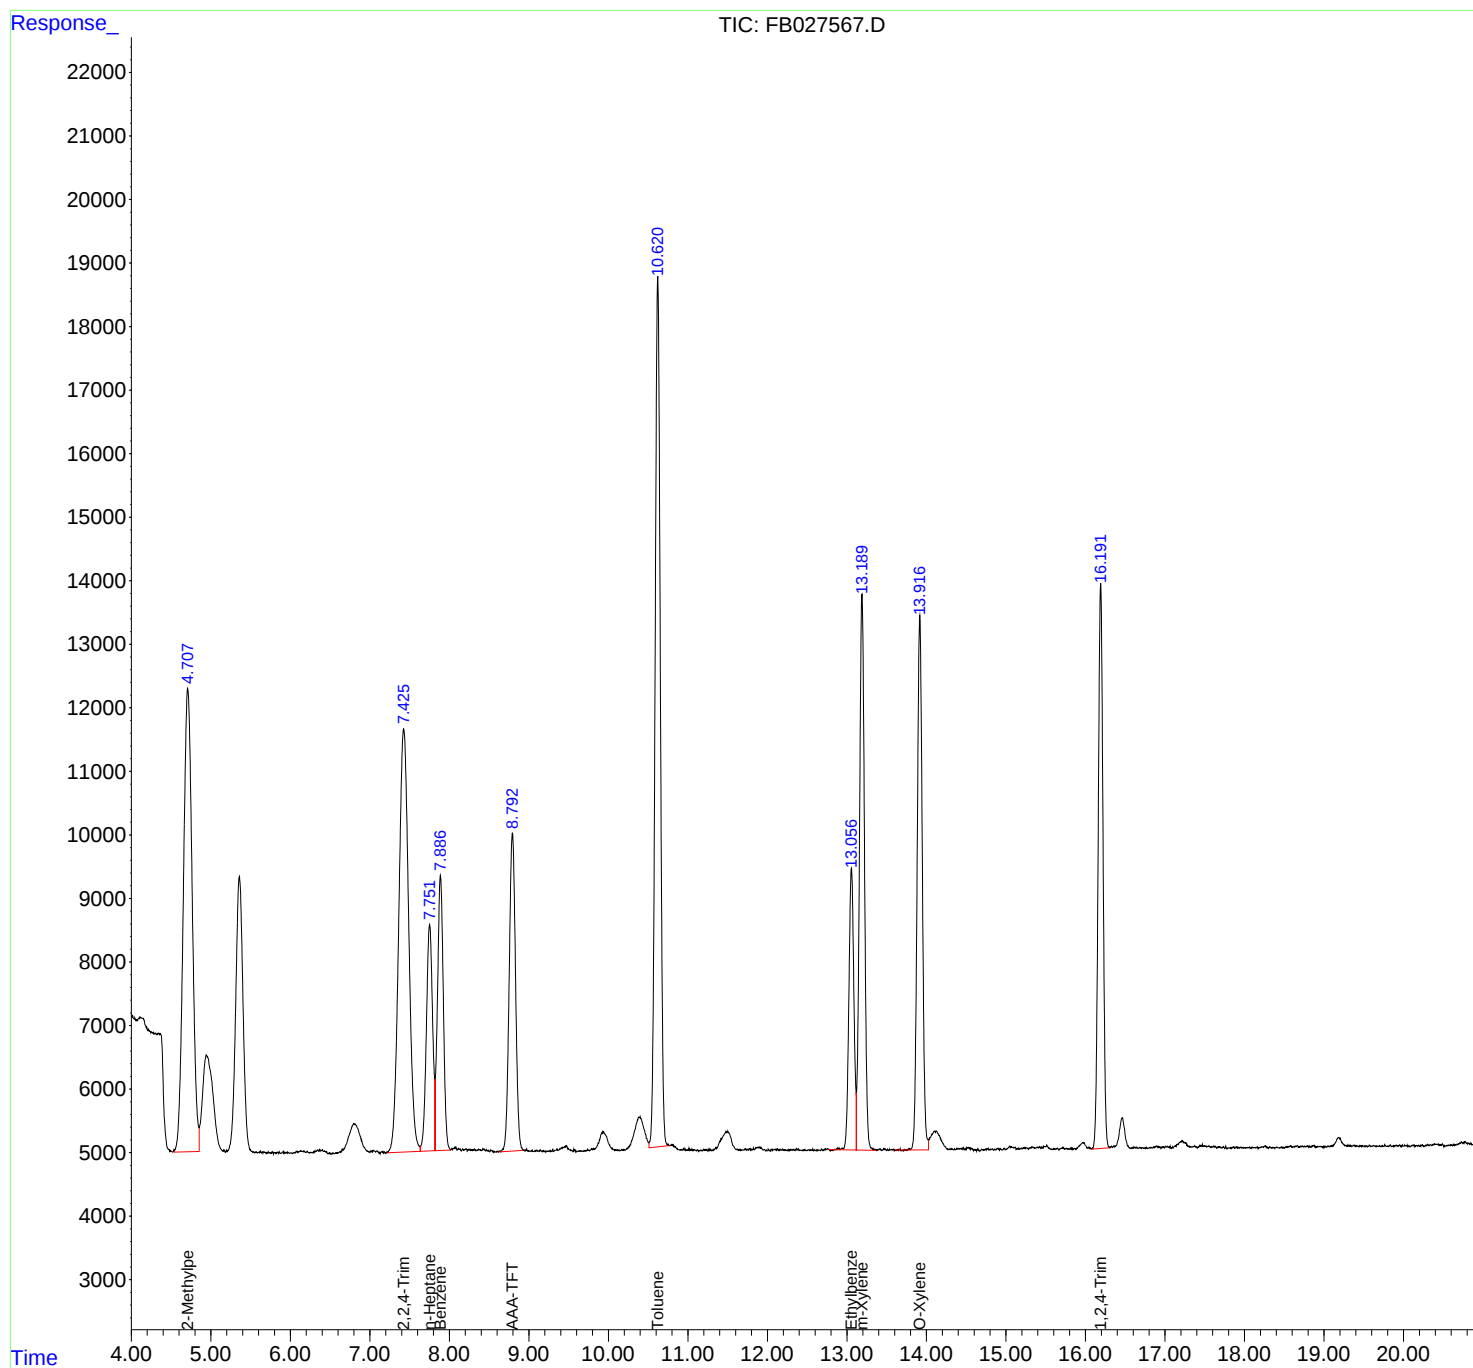


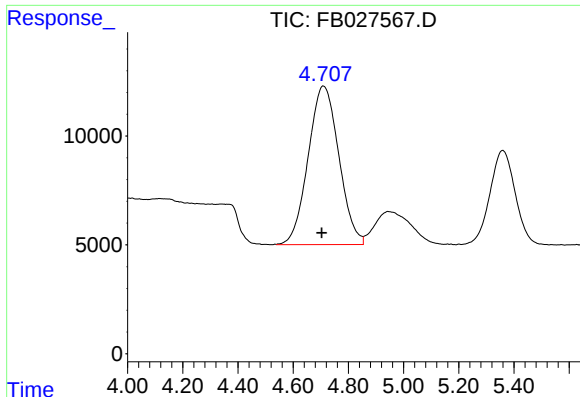

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.005 min
Response: 563134
Conc: 33.43 ng/ml

Instrument :
FID_B
ClientSampleId :

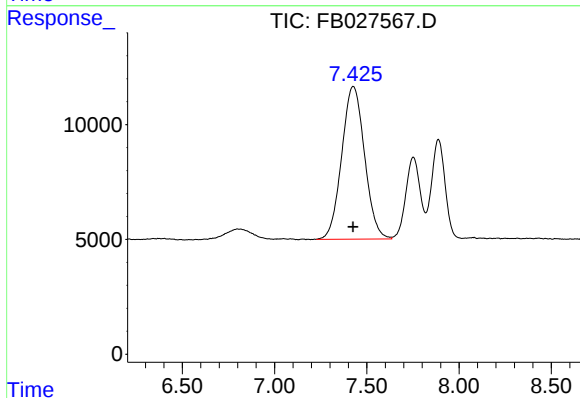


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: 0.000 min
Response: 573584
Conc: 32.67 ng/ml

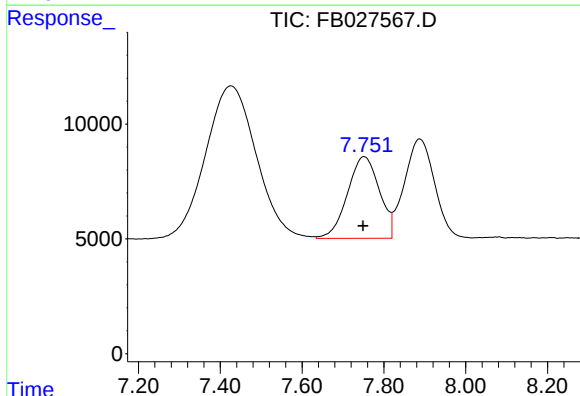


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.003 min
Response: 192964
Conc: 11.01 ng/ml

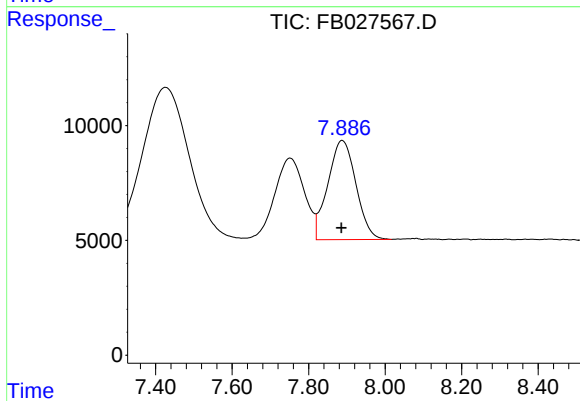

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.002 min
Response: 220601
Conc: 10.82 ng/ml

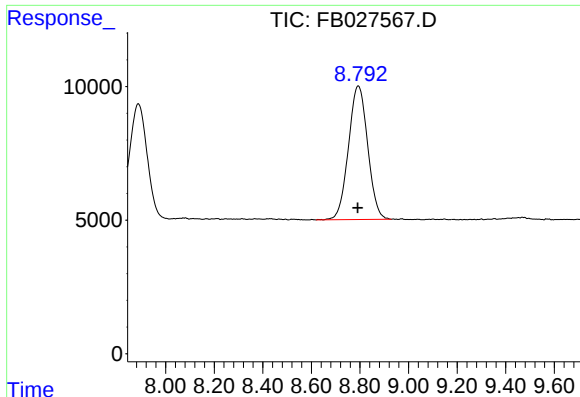

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.003 min
Response: 274690
Conc: 24.49 ng/ml

Instrument :
FID_B
ClientSampleId :

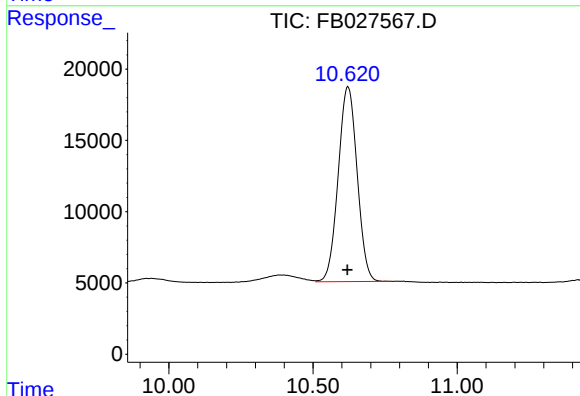


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 621200
Conc: 32.08 ng/ml

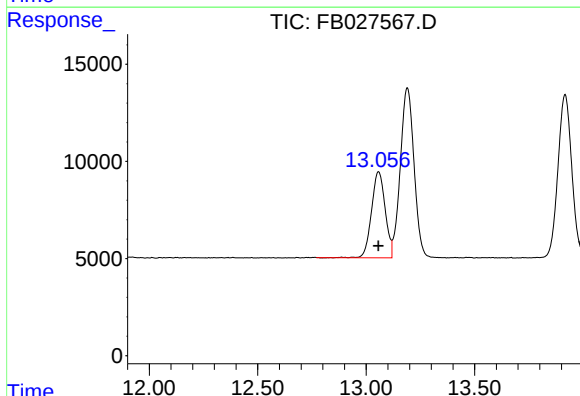


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 192978
Conc: 10.66 ng/ml

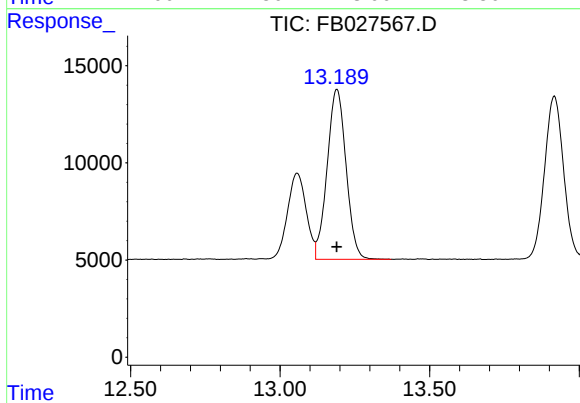

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 384555
Conc: 21.57 ng/ml

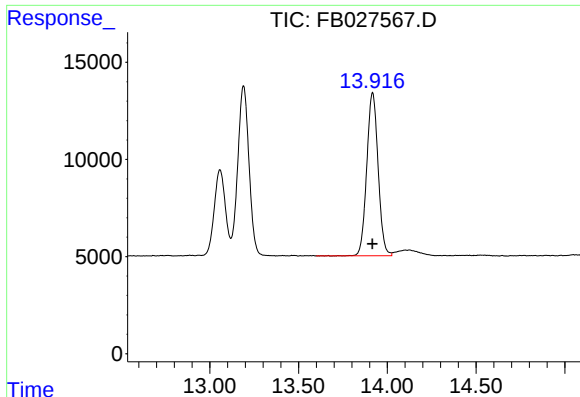

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.001 min
Response: 372571
Conc: 21.44 ng/ml

Instrument :
FID_B
ClientSampleId :

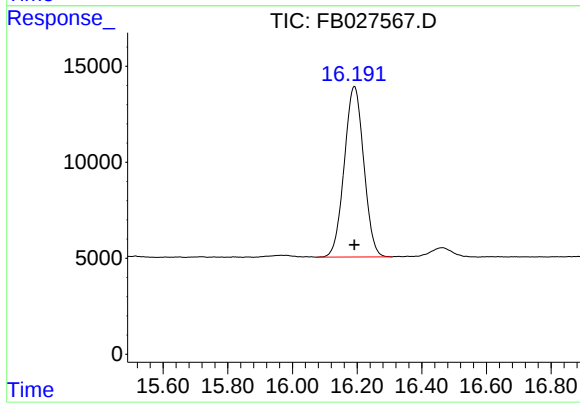

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 371315
Conc: 21.62 ng/ml