

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062822\
 Data File : FB027568.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2022 14:45
 Operator : AJ/MA
 Sample : N3494-14 250X
 Misc : 5.07G/5.00 ML MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 29 03:35:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	236471	21.082 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	274	0.016 ng/ml
2) t 2,2,4-Trimethylpentane	7.374	3464	0.197 ng/ml
3) t n-Heptane	7.740	35073	2.002 ng/ml
4) t Benzene	7.890	18800	0.922 ng/ml
7) t Ethylbenzene	13.019	803011	44.342 ng/ml
9) t O-Xylene	13.937	159049	9.153 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	37517	2.184 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062822\
Data File : FB027568.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2022 14:45
Operator : AJ/MA
Sample : N3494-14 250X
Misc : 5.07G/5.00 ML MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 29 03:35:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

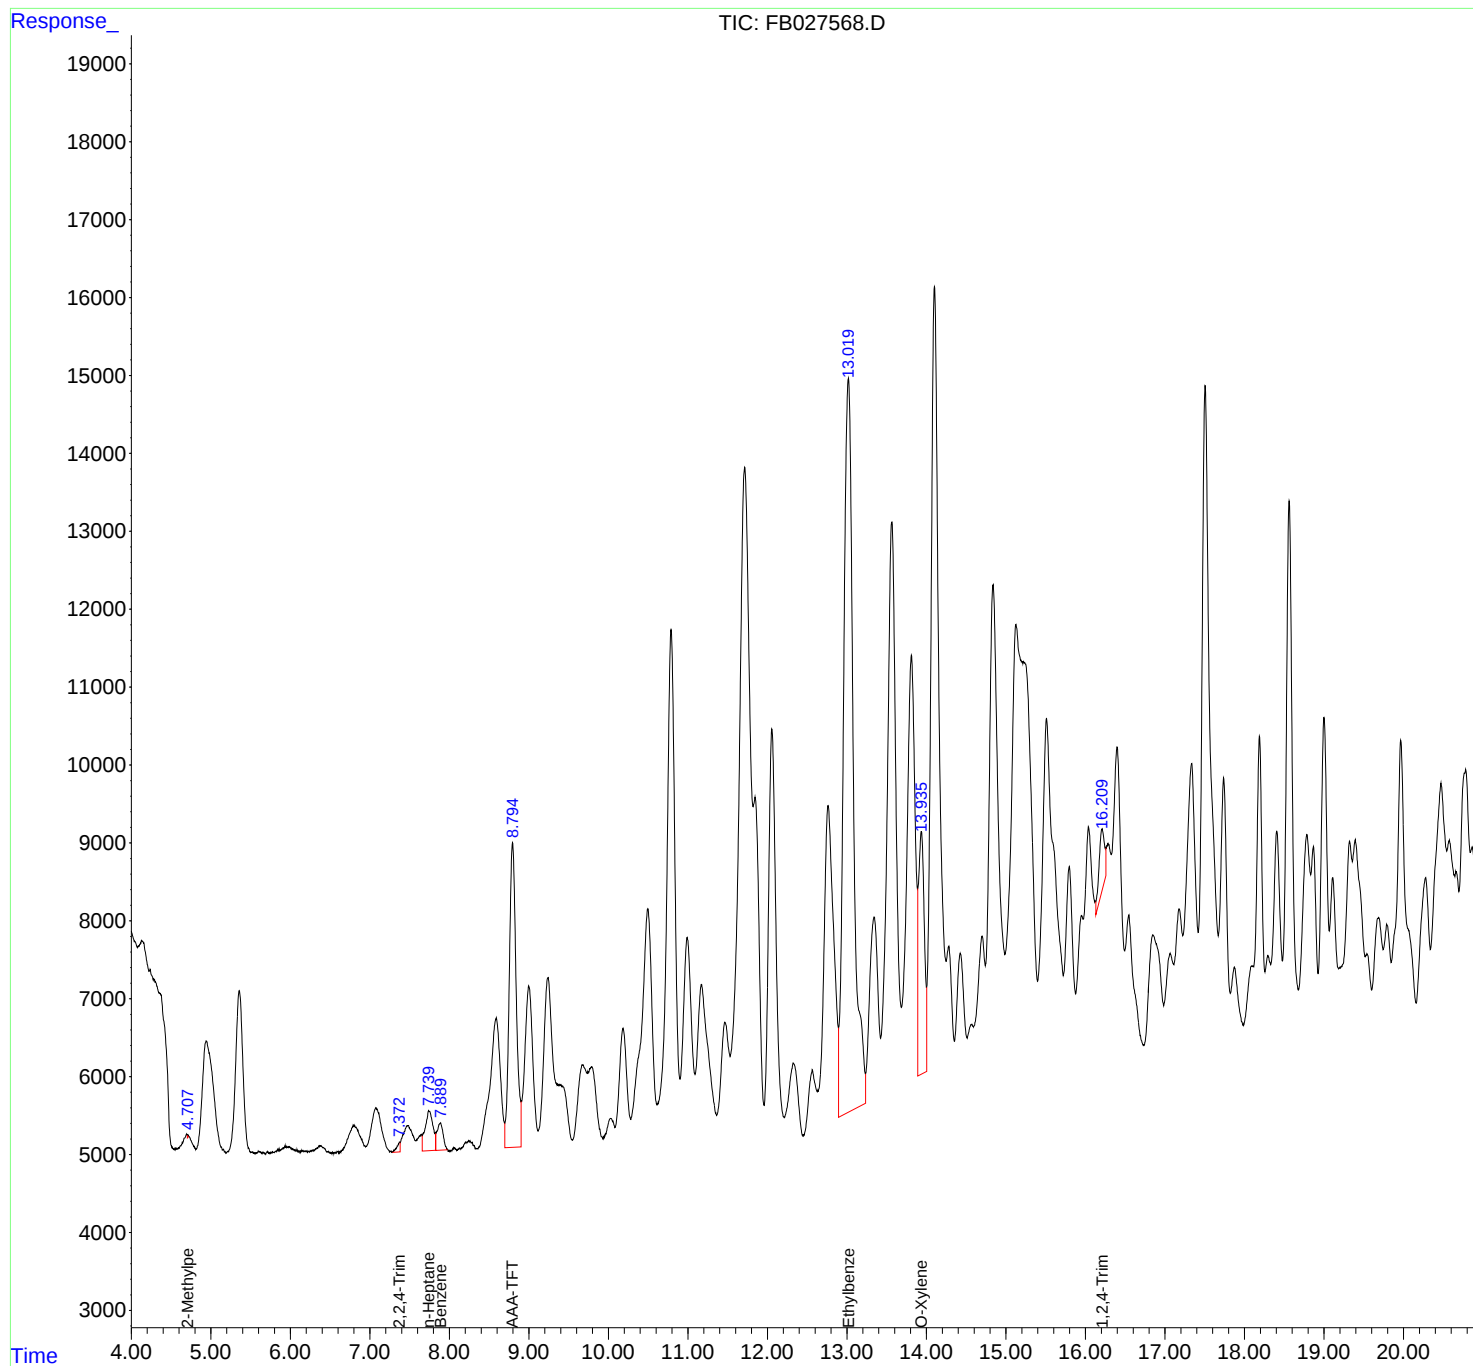


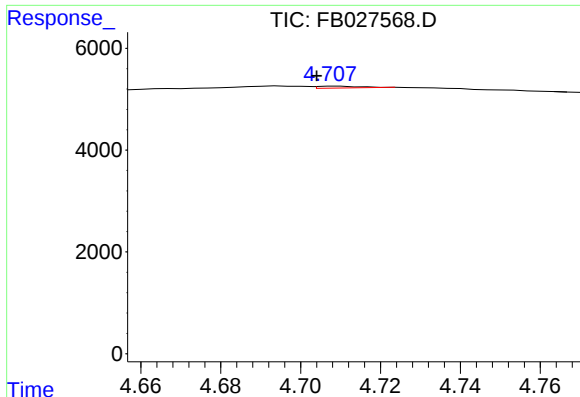

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.005 min
Response: 274
Conc: 0.02 ng/ml

Instrument :
FID_B
ClientSampleId :

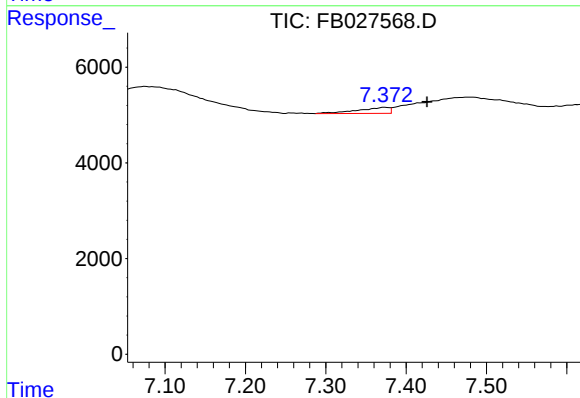


#2 2,2,4-Trimethylpentane

R.T.: 7.374 min
Delta R.T.: -0.052 min
Response: 3464
Conc: 0.20 ng/ml

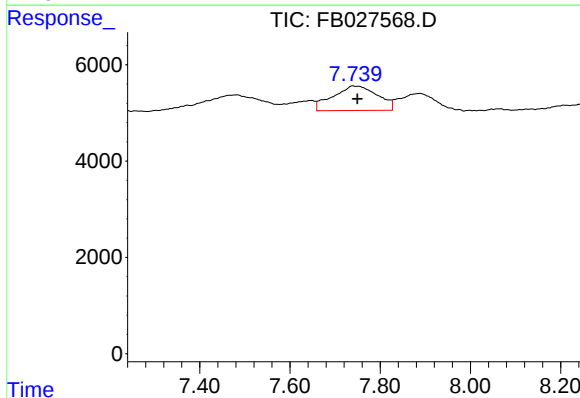


#3 n-Heptane

R.T.: 7.740 min
Delta R.T.: -0.009 min
Response: 35073
Conc: 2.00 ng/ml

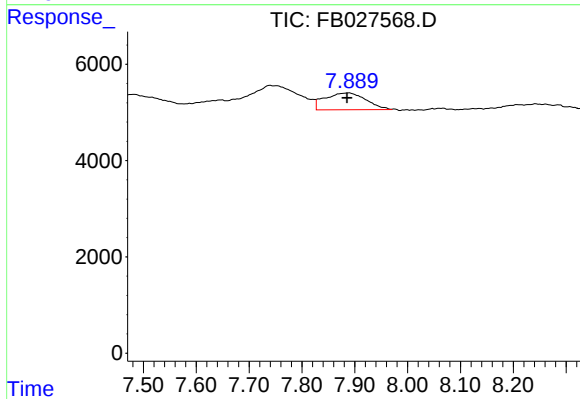

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.005 min
Response: 18800
Conc: 0.92 ng/ml

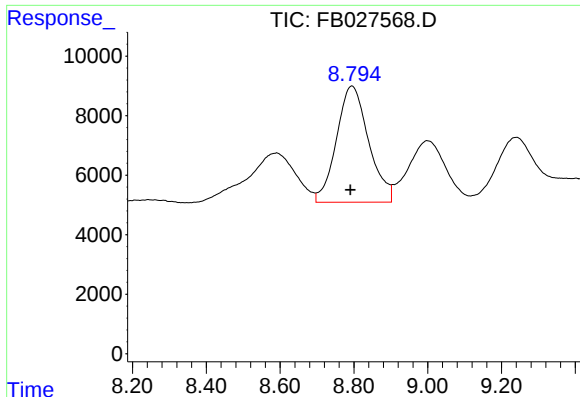

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.005 min
Response: 236471
Conc: 21.08 ng/ml

Instrument :
FID_B
ClientSampleId :

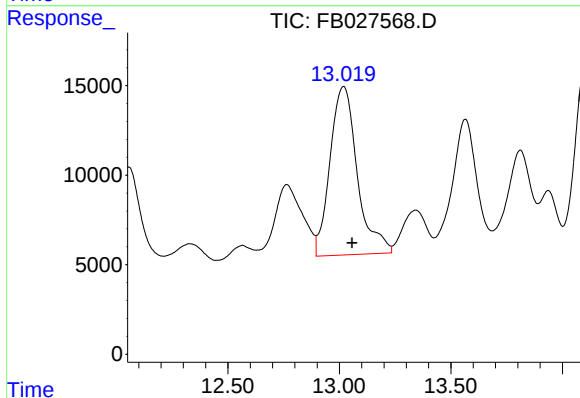


#7 Ethylbenzene

R.T.: 13.019 min
Delta R.T.: -0.037 min
Response: 803011
Conc: 44.34 ng/ml

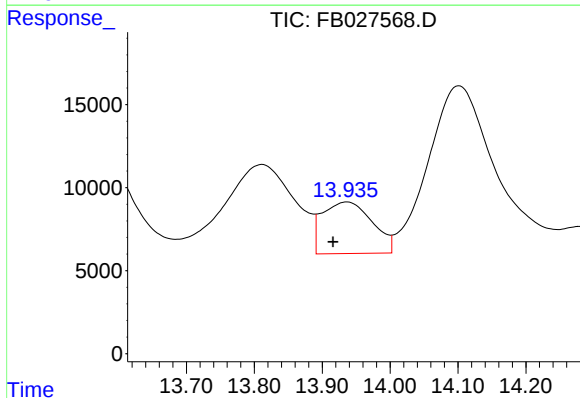

#9 O-Xylene

R.T.: 13.937 min
Delta R.T.: 0.021 min
Response: 159049
Conc: 9.15 ng/ml

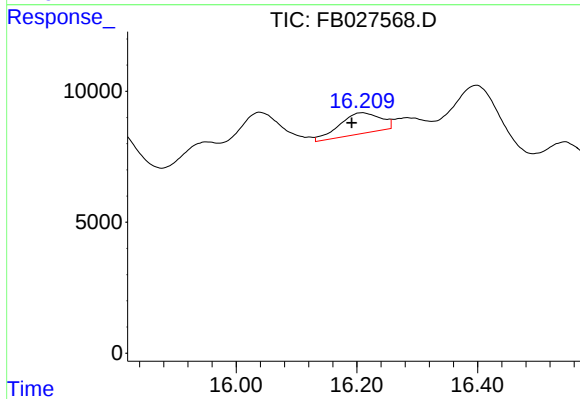

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.018 min
Response: 37517
Conc: 2.18 ng/ml