

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062822\
 Data File : FB027569.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2022 15:22
 Operator : AJ/MA
 Sample : N3494-24 50X
 Misc : 5.07G/5.00 ML MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jun 29 03:35:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	263174	23.463 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	43995	2.611 ng/ml
2) t 2,2,4-Trimethylpentane	7.373	11466	0.653 ng/ml
3) t n-Heptane	7.747	96559	5.512 ng/ml
4) t Benzene	7.885	189177	9.277 ng/ml
6) t Toluene	10.619	42901	2.216 ng/ml
8) t m-Xylene	13.186	96611	5.420 ng/ml
9) t O-Xylene	13.918	26933	1.550 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	58748	3.420 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062822\
Data File : FB027569.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2022 15:22
Operator : AJ/MA
Sample : N3494-24 50X
Misc : 5.07G/5.00 ML MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jun 29 03:35:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

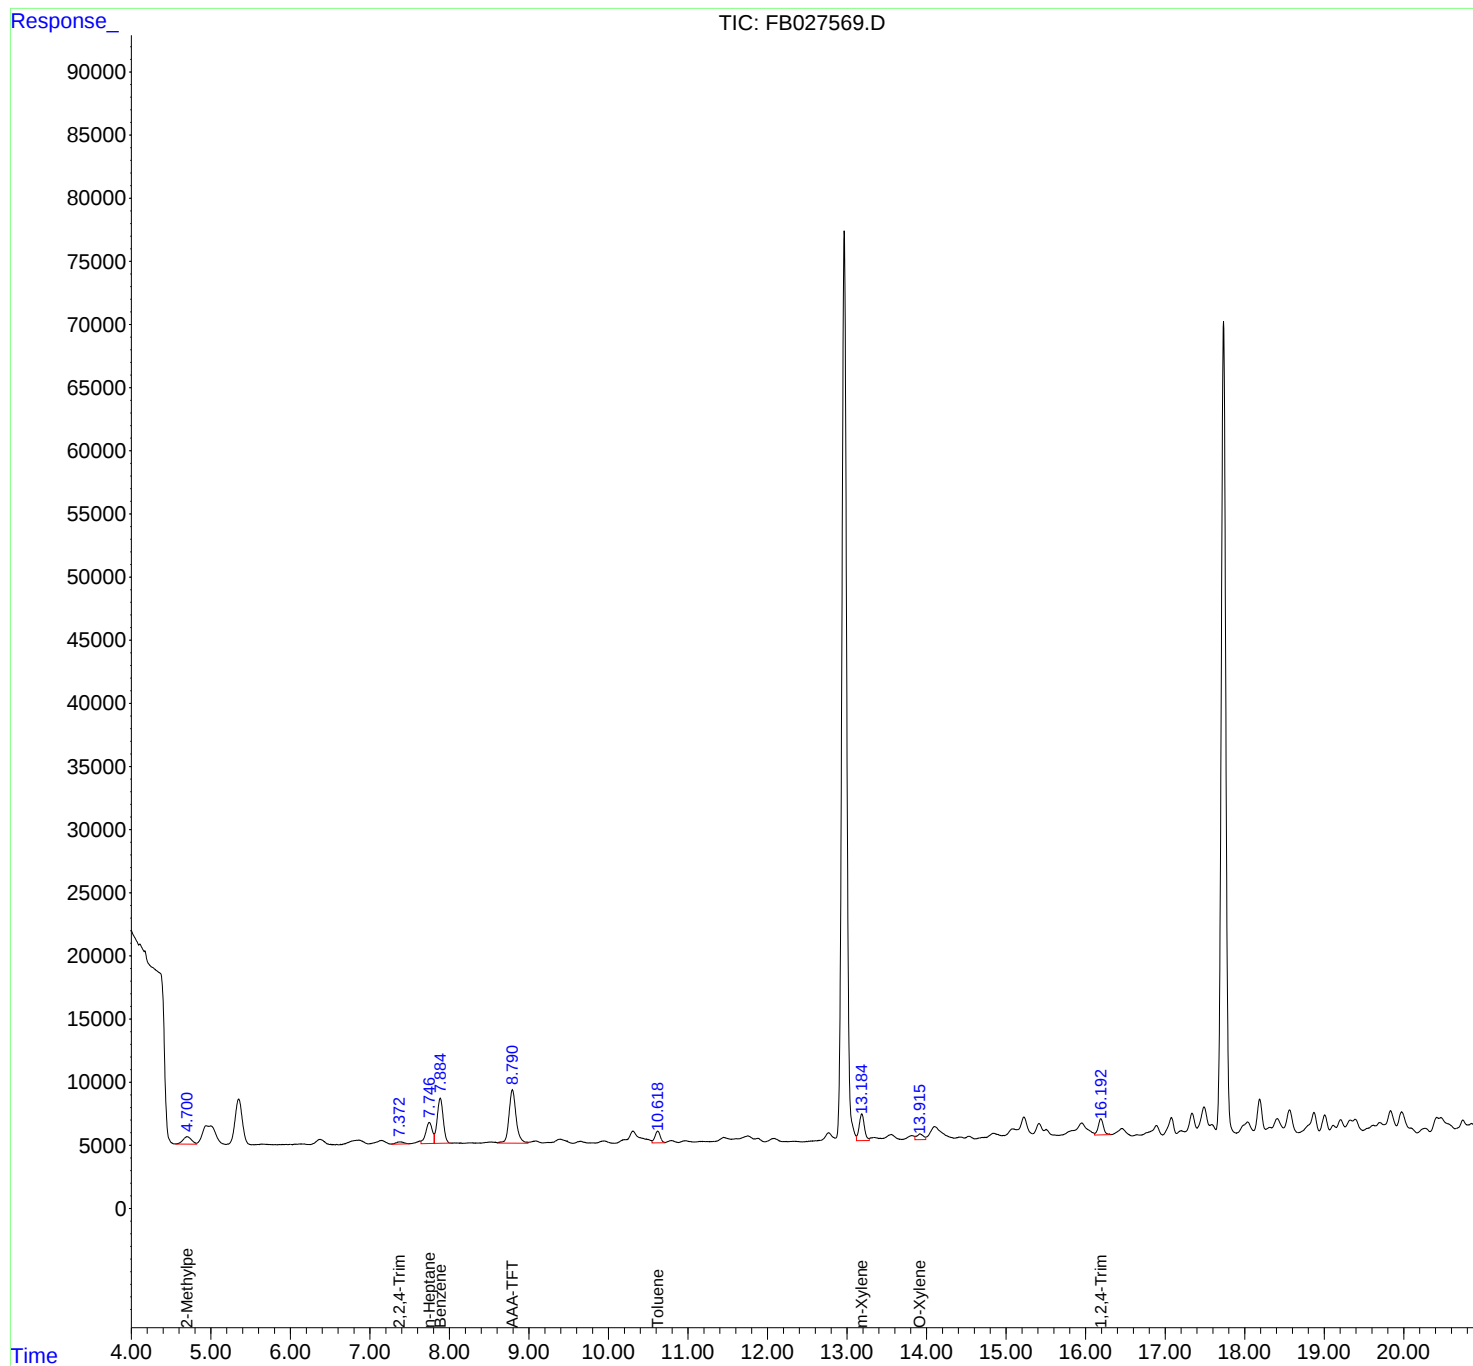


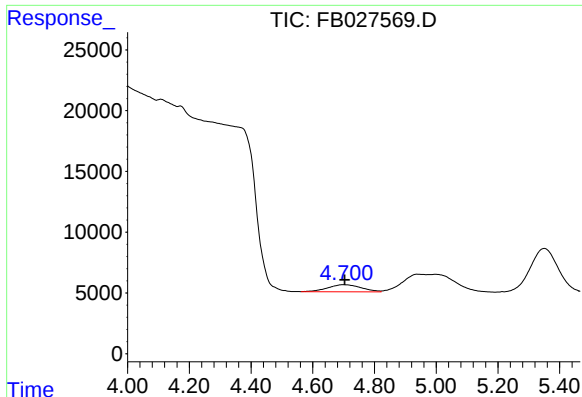

#1 2-Methylpentane


R.T.: 4.702 min
Delta R.T.: -0.002 min
Response: 43995
Conc: 2.61 ng/ml

Instrument :
FID_B
ClientSampleId :

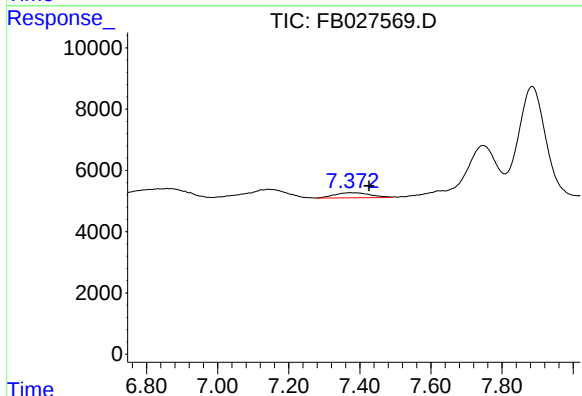


#2 2,2,4-Trimethylpentane

R.T.: 7.373 min
Delta R.T.: -0.053 min
Response: 11466
Conc: 0.65 ng/ml

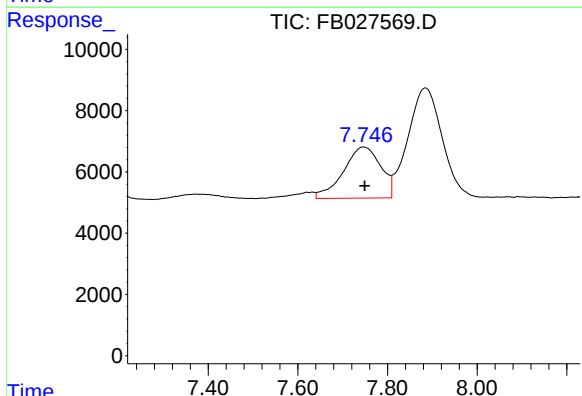


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.002 min
Response: 96559
Conc: 5.51 ng/ml

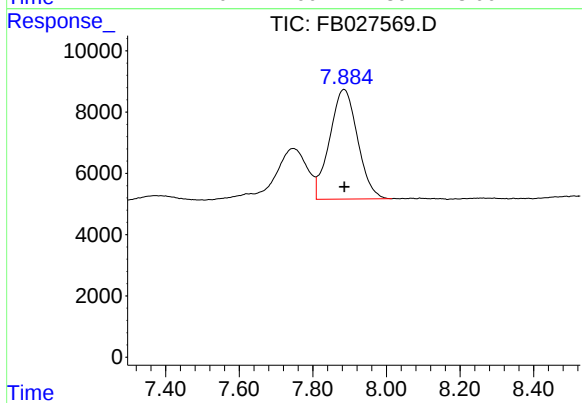

#4 Benzene


R.T.: 7.885 min
Delta R.T.: 0.000 min
Response: 189177
Conc: 9.28 ng/ml

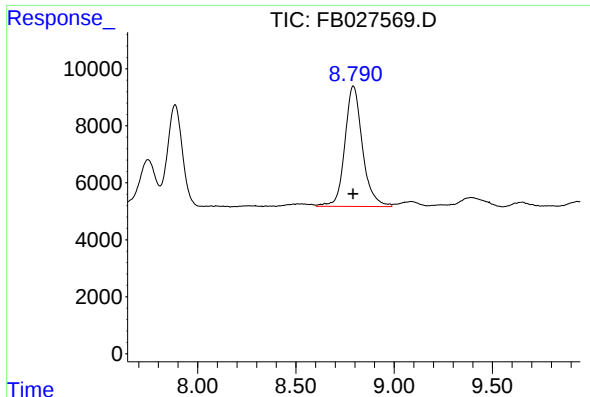

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.001 min
Response: 263174
Conc: 23.46 ng/ml

Instrument :
FID_B
ClientSampleId :

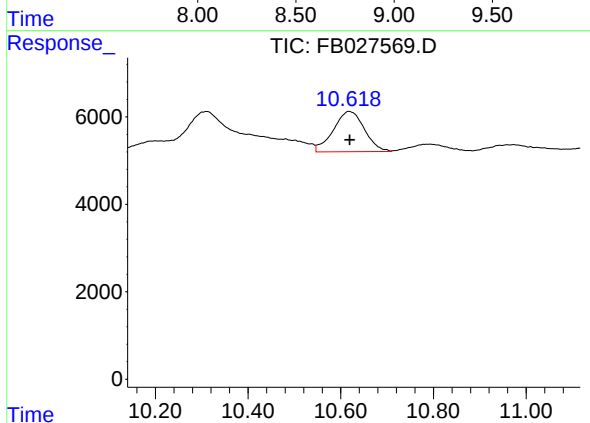


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.000 min
Response: 42901
Conc: 2.22 ng/ml

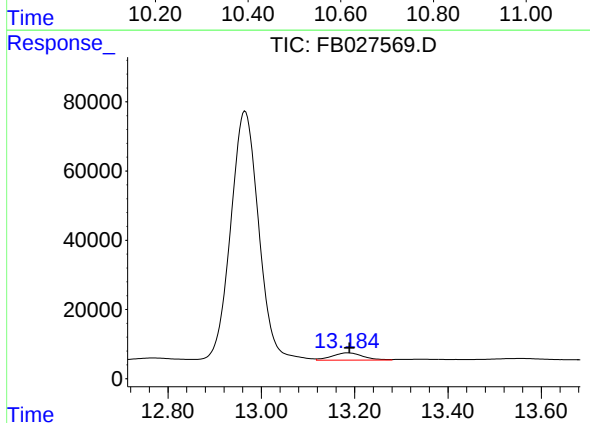


#8 m-Xylene

R.T.: 13.186 min
Delta R.T.: -0.003 min
Response: 96611
Conc: 5.42 ng/ml

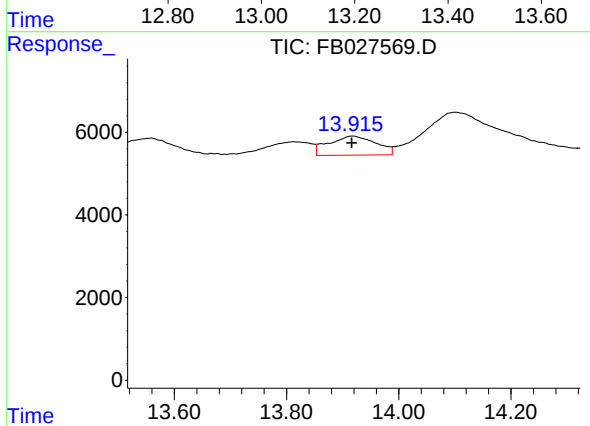

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 26933
Conc: 1.55 ng/ml

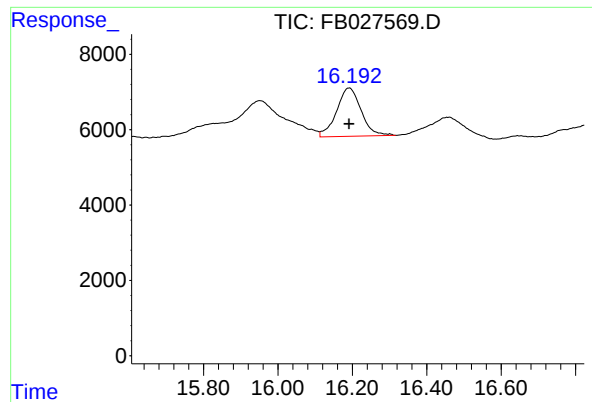

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 58748
Conc: 3.42 ng/ml

Instrument :
FID_B
ClientSampleId :