

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062822\
 Data File : FB027570.D
 Signal(s) : FID2B.CH
 Acq On : 28 Jun 2022 15:59
 Operator : AJ/MA
 Sample : BSF0628S2
 Misc : 5.07G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0628S2

Integration File: SAMPLE.e
 Quant Time: Jun 29 03:35:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	240945	21.481 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	502794	29.844 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	533307	30.373 ng/ml
3) t n-Heptane	7.752	178354	10.181 ng/ml
4) t Benzene	7.889	202153	9.913 ng/ml
6) t Toluene	10.623	590831	30.515 ng/ml
7) t Ethylbenzene	13.059	191357	10.567 ng/ml
8) t m-Xylene	13.192	361326	20.270 ng/ml
9) t O-Xylene	13.919	353004	20.316 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	346746	20.185 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062822\
Data File : FB027570.D
Signal(s) : FID2B.CH
Acq On : 28 Jun 2022 15:59
Operator : AJ/MA
Sample : BSF0628S2
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0628S2

Integration File: SAMPLE.e
Quant Time: Jun 29 03:35:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

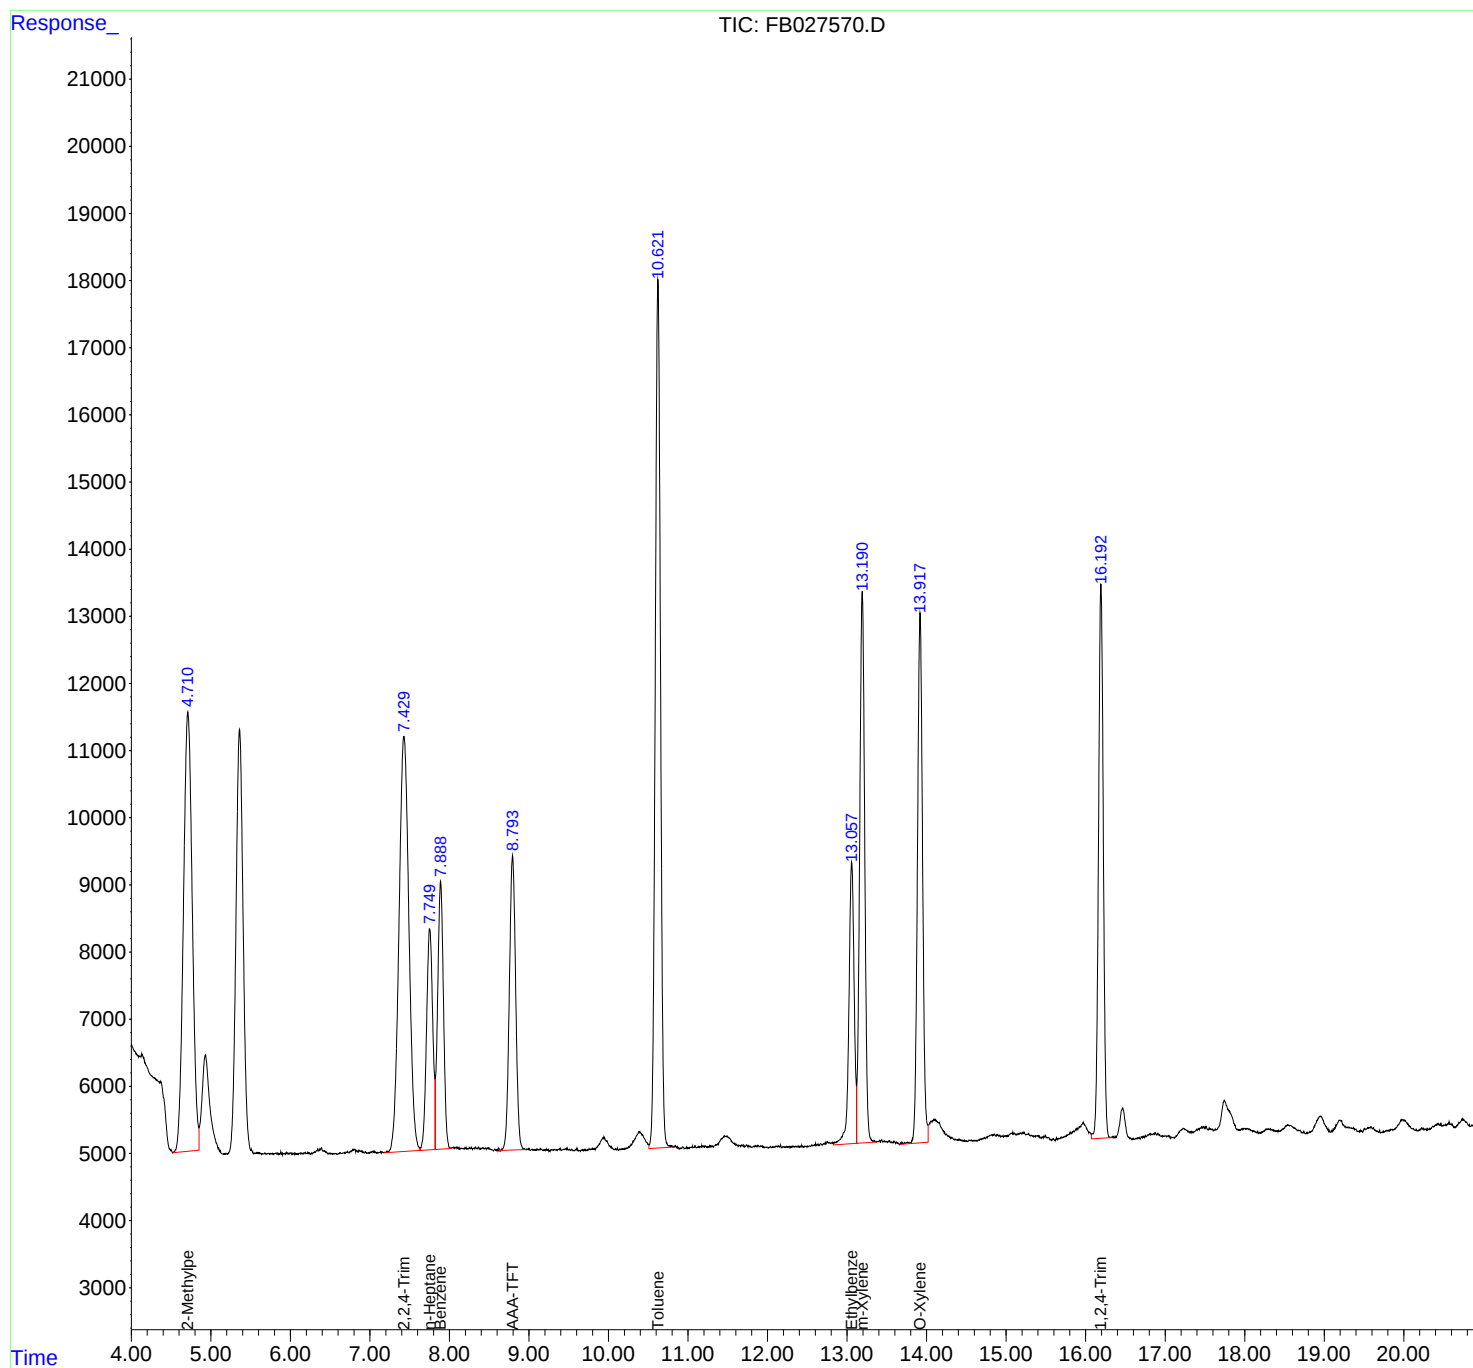


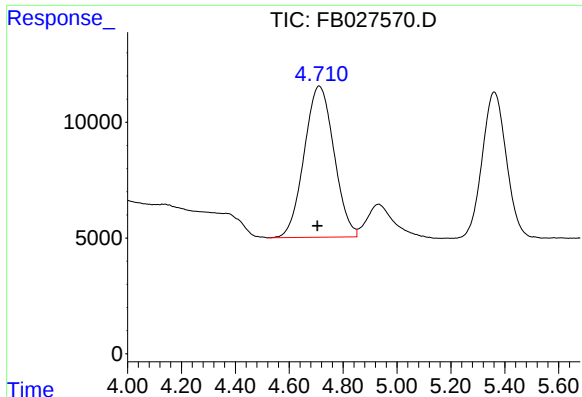

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.007 min
Response: 502794
Conc: 29.84 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0628S2

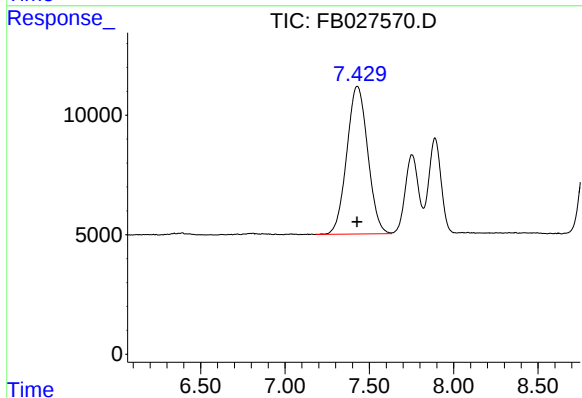


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: 0.003 min
Response: 533307
Conc: 30.37 ng/ml

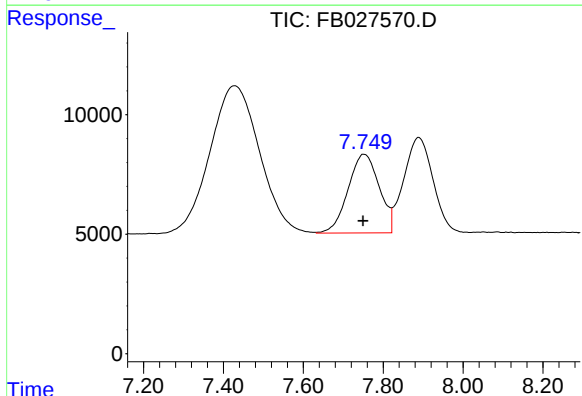


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.002 min
Response: 178354
Conc: 10.18 ng/ml

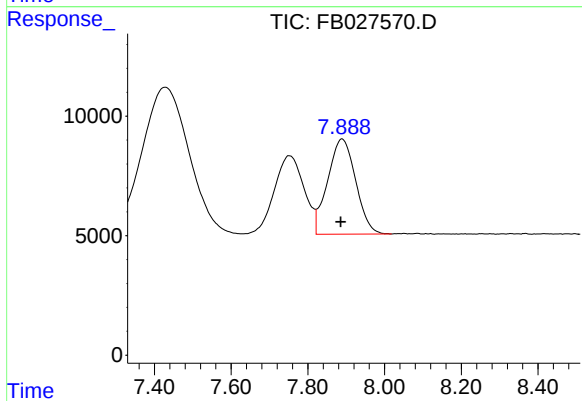

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.004 min
Response: 202153
Conc: 9.91 ng/ml

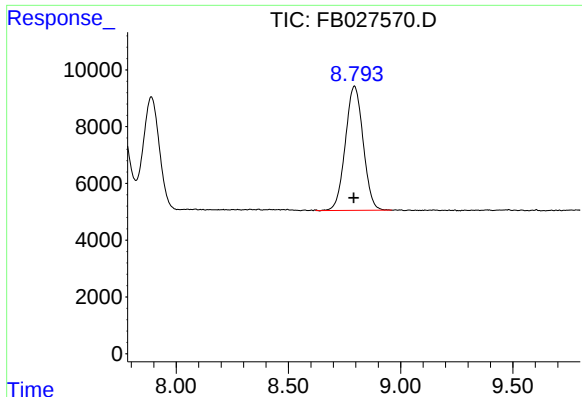

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.004 min
Response: 240945
Conc: 21.48 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0628S2

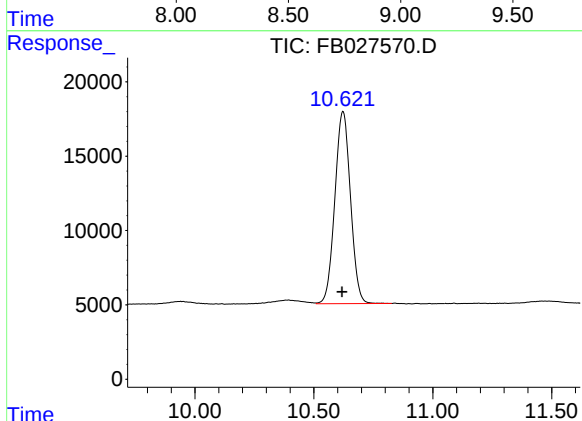


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.003 min
Response: 590831
Conc: 30.51 ng/ml

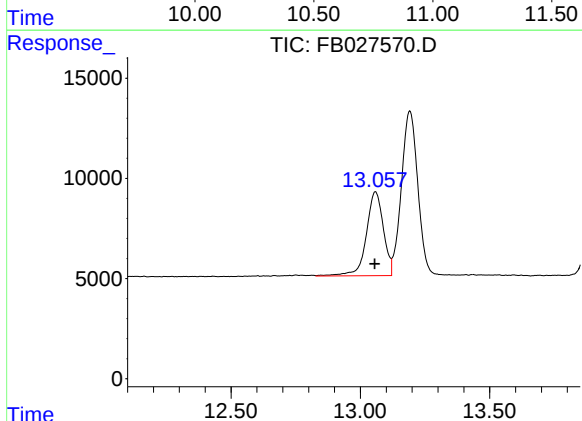


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.002 min
Response: 191357
Conc: 10.57 ng/ml

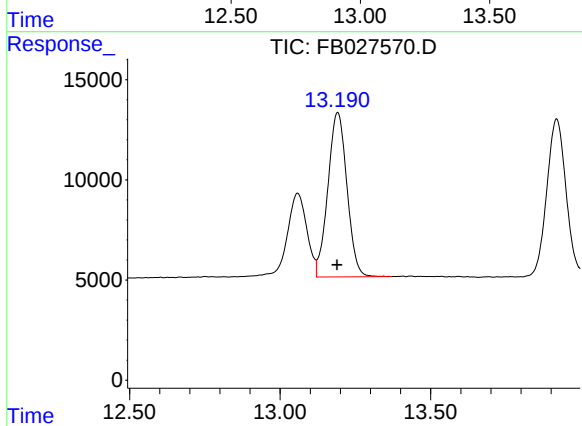

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.003 min
Response: 361326
Conc: 20.27 ng/ml

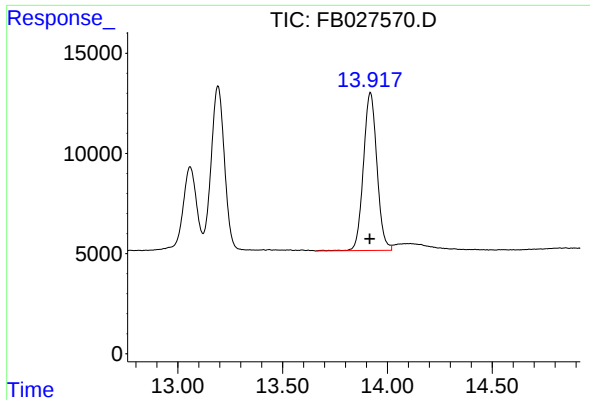

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.003 min
Response: 353004
Conc: 20.32 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0628S2

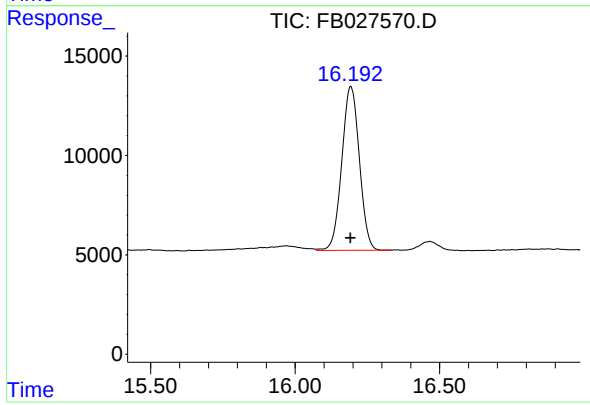

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.002 min
Response: 346746
Conc: 20.19 ng/ml