

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062918\
 Data File : FB016470.D
 Signal(s) : FID2B.CH
 Acq On : 29 Jun 2018 10:00
 Operator : MJ/SJ
 Sample : VBF0629S1
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0629W1

Integration File: Calibration.e
 Quant Time: Jun 29 13:36:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Thu Jun 28 12:22:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.115	152034	21.634 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.968	391128	32.255 ng/ml
2) t 2,2,4-Trimethylpentane	7.731	383823	33.142 ng/ml
3) t n-Heptane	8.070	116221	10.619 ng/ml
4) t Benzene	8.209	164112	11.053 ng/ml
6) t Toluene	10.964	379905	30.606 ng/ml
7) t Ethylbenzene	13.412	147213	10.517 ng/ml
8) t m-Xylene	13.546	316337	20.783 ng/ml
9) t O-Xylene	14.277	333348	21.361 ng/ml
10) t 1,2,4-Trimethylbenzene	16.560	355431	20.637 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062918\
Data File : FB016470.D
Signal(s) : FID2B.CH
Acq On : 29 Jun 2018 10:00
Operator : MJ/SJ
Sample : VBF0629S1
Misc : 5.01g/5.00mL DI Water
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0629W1

Integration File: Calibration.e
Quant Time: Jun 29 13:36:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Thu Jun 28 12:22:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

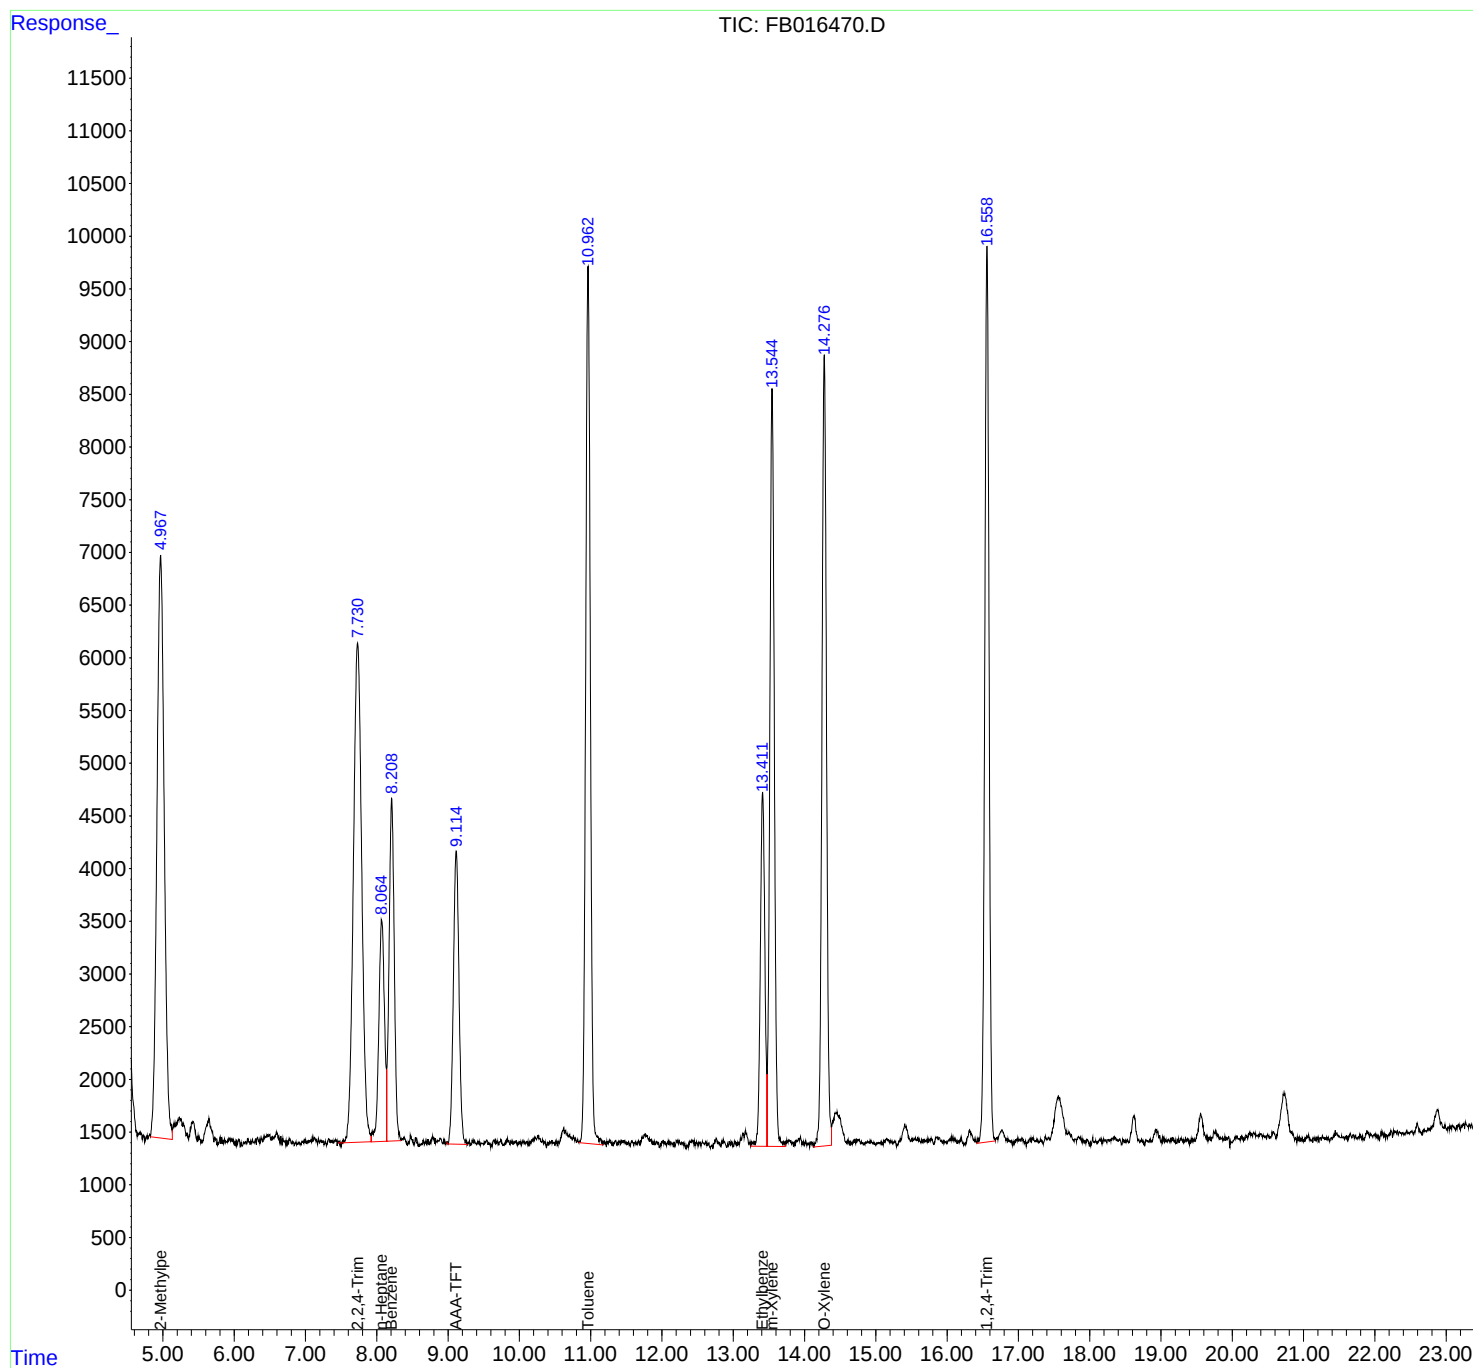


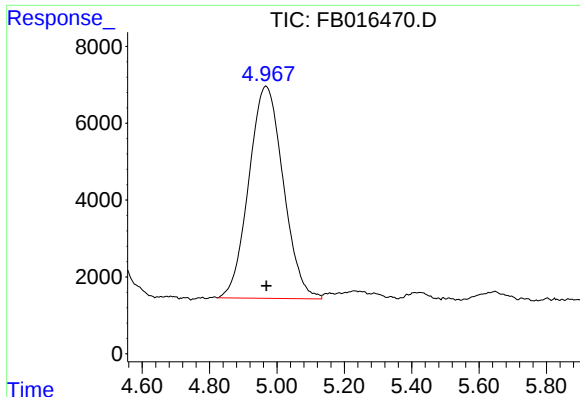

#1 2-Methylpentane


R.T.: 4.968 min
Delta R.T.: -0.001 min
Response: 391128
Conc: 32.25 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0629W1

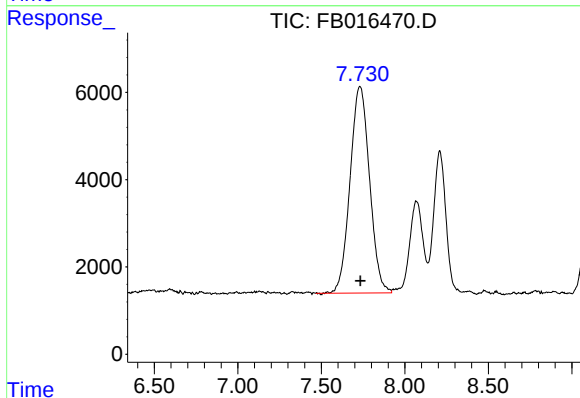


#2 2,2,4-Trimethylpentane

R.T.: 7.731 min
Delta R.T.: -0.002 min
Response: 383823
Conc: 33.14 ng/ml

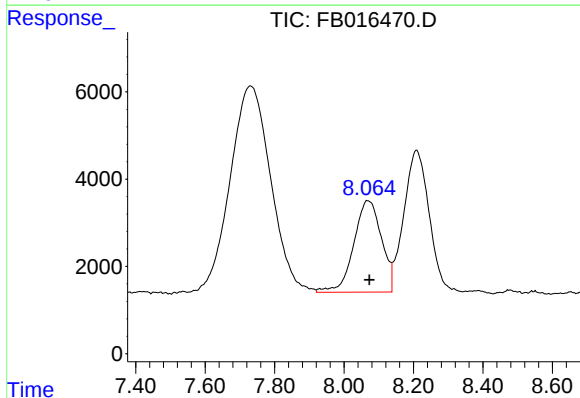


#3 n-Heptane

R.T.: 8.070 min
Delta R.T.: -0.003 min
Response: 116221
Conc: 10.62 ng/ml

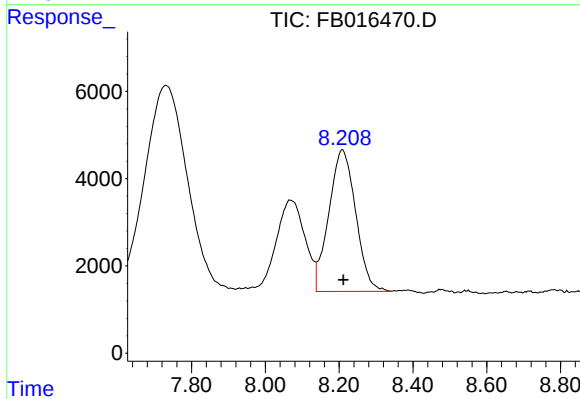

#4 Benzene


R.T.: 8.209 min
Delta R.T.: -0.002 min
Response: 164112
Conc: 11.05 ng/ml

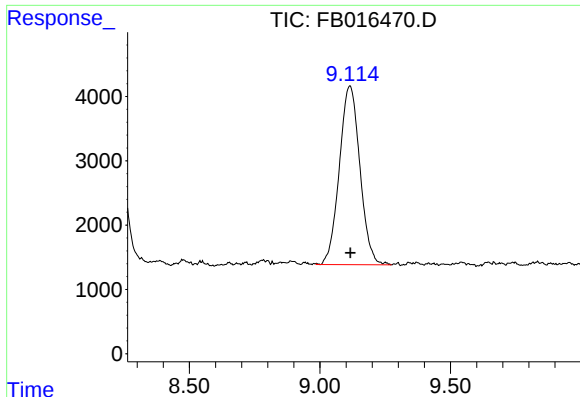

#5 AAA-TFT


R.T.: 9.115 min
Delta R.T.: -0.002 min
Response: 152034
Conc: 21.63 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0629W1

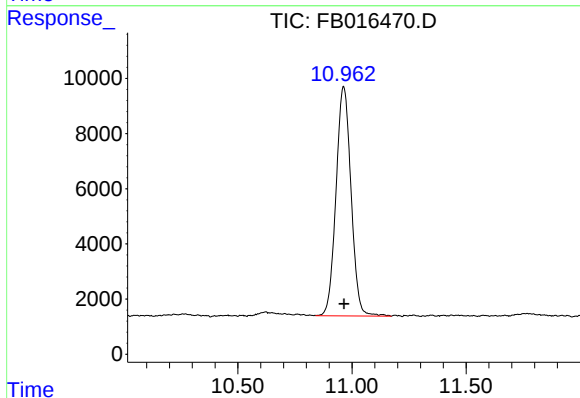


#6 Toluene

R.T.: 10.964 min
Delta R.T.: -0.002 min
Response: 379905
Conc: 30.61 ng/ml

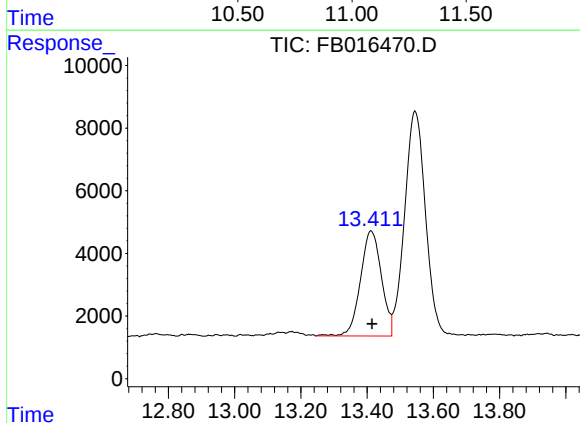


#7 Ethylbenzene

R.T.: 13.412 min
Delta R.T.: -0.002 min
Response: 147213
Conc: 10.52 ng/ml

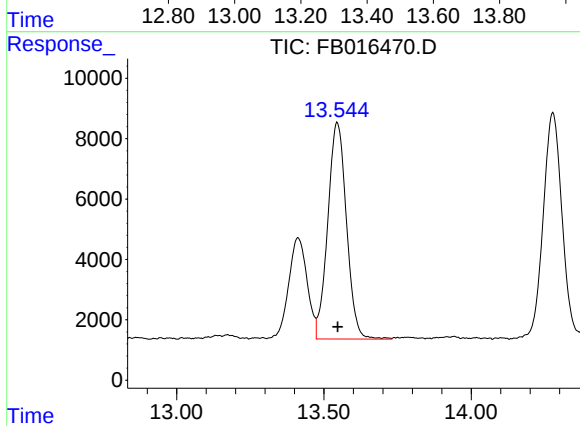

#8 m-Xylene


R.T.: 13.546 min
Delta R.T.: -0.002 min
Response: 316337
Conc: 20.78 ng/ml

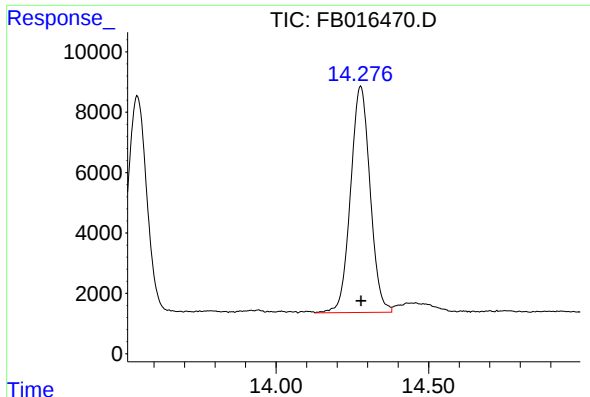

#9 O-Xylene

R.T.: 14.277 min
Delta R.T.: -0.001 min
Response: 333348
Conc: 21.36 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0629W1

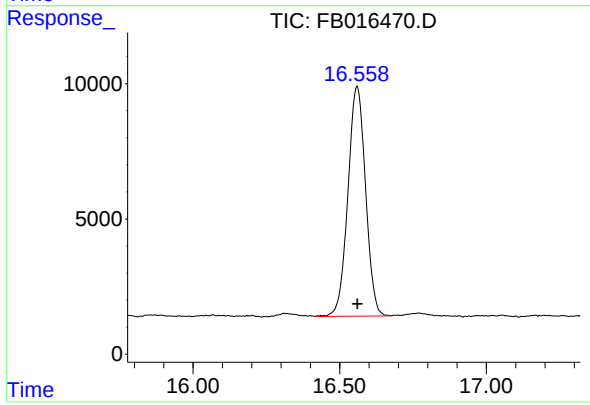

#10 1,2,4-Trimethylbenzene

R.T.: 16.560 min
Delta R.T.: 0.000 min
Response: 355431
Conc: 20.64 ng/ml