

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062918\
Data File : FB016477.D
Signal(s) : FID2B.CH
Acq On : 29 Jun 2018 14:29
Operator : MJ/SJ
Sample : J3631-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 02 09:38:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Thu Jun 28 12:22:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.118	146369	20.827 ng/ml
Target Compounds			
4) t Benzene	8.214	10836	0.730 ng/ml
7) t Ethylbenzene	13.417	8437	0.603 ng/ml
8) t m-Xylene	13.549	11607	0.763 ng/ml
10) t 1,2,4-Trimethylbenzene	16.561	11653	0.677 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062918\
Data File : FB016477.D
Signal(s) : FID2B.CH
Acq On : 29 Jun 2018 14:29
Operator : MJ/SJ
Sample : J3631-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 02 09:38:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Thu Jun 28 12:22:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

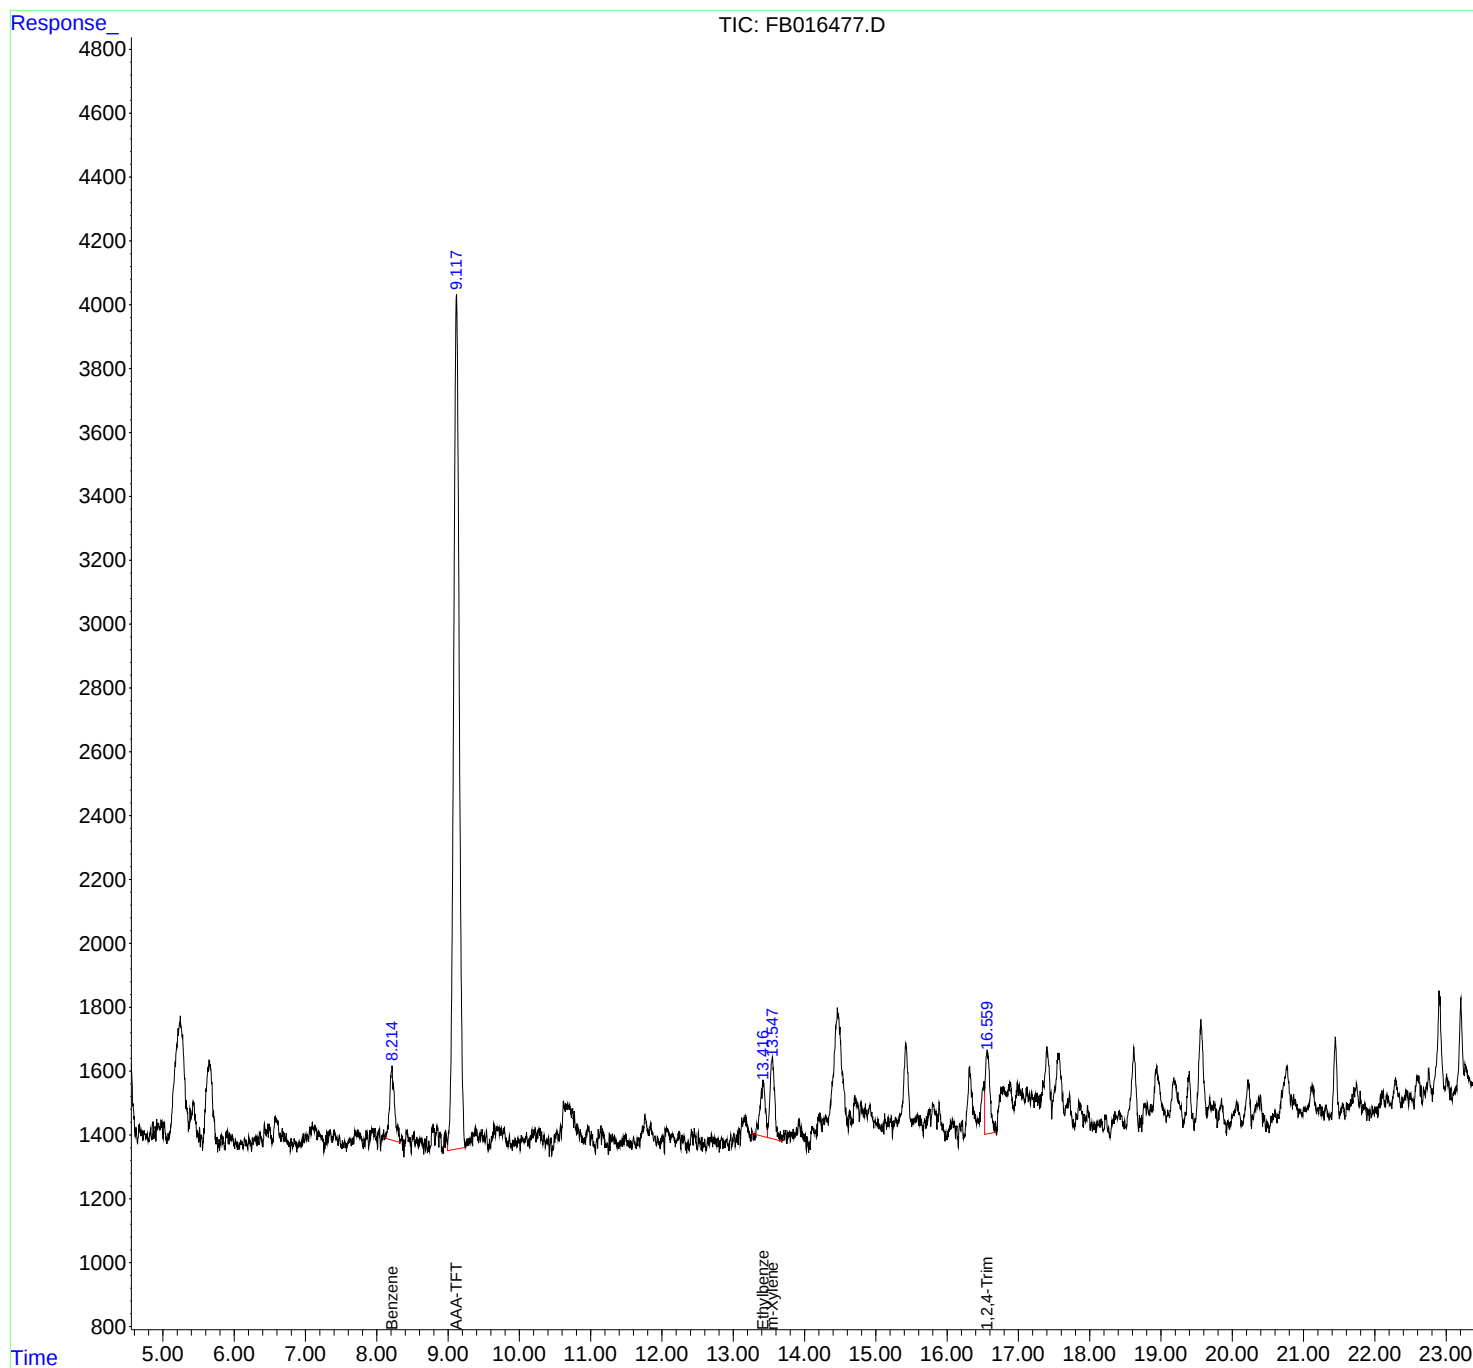


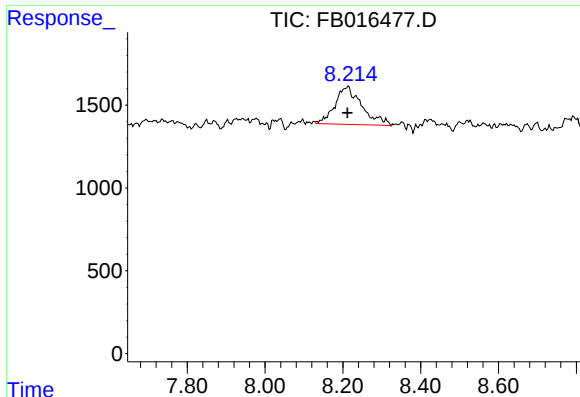

#4 Benzene


R.T.: 8.214 min
Delta R.T.: 0.003 min
Response: 10836
Conc: 0.73 ng/ml

Instrument :
FID_B
ClientSampleId :

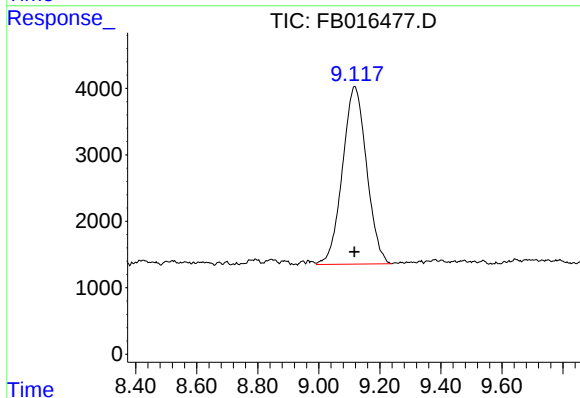


#5 AAA-TFT

R.T.: 9.118 min
Delta R.T.: 0.001 min
Response: 146369
Conc: 20.83 ng/ml

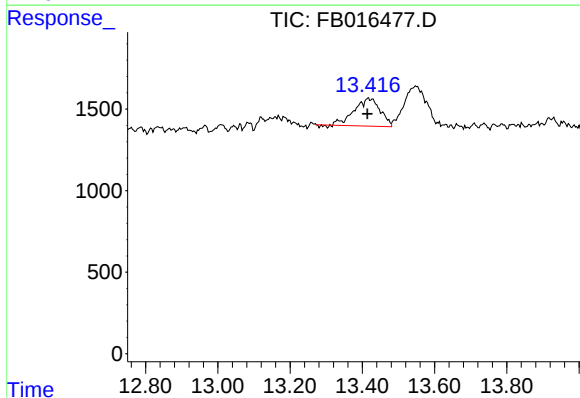


#7 Ethylbenzene

R.T.: 13.417 min
Delta R.T.: 0.002 min
Response: 8437
Conc: 0.60 ng/ml

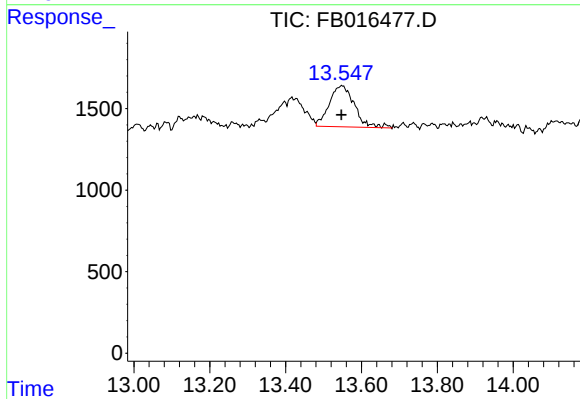

#8 m-Xylene

R.T.: 13.549 min
Delta R.T.: 0.002 min
Response: 11607
Conc: 0.76 ng/ml

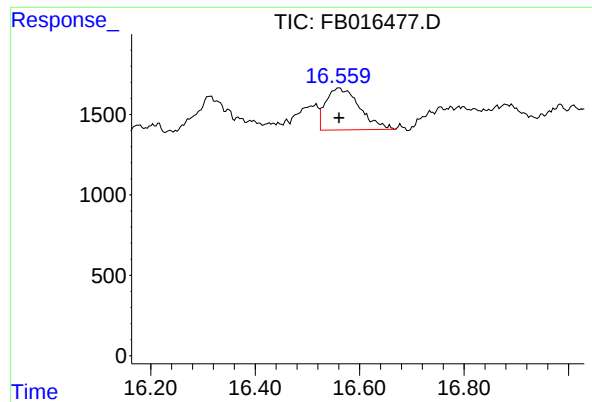

#10 1,2,4-Trimethylbenzene

R.T.: 16.561 min
Delta R.T.: 0.000 min
Response: 11653
Conc: 0.68 ng/ml

Instrument :
FID_B
ClientSampleId :