

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062918\
 Data File : FB016491.D
 Signal(s) : FID2B.CH
 Acq On : 29 Jun 2018 23:44
 Operator : MJ/SJ
 Sample : J3774-03MS
 Misc : 5.00g/5.00mL DI Water
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jul 02 09:39:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Thu Jun 28 12:22:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.116	144838	20.610 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.968	350010	28.864 ng/ml
2) t 2,2,4-Trimethylpentane	7.733	344796	29.772 ng/ml
3) t n-Heptane	8.071	100845	9.214 ng/ml
4) t Benzene	8.211	146936	9.896 ng/ml
6) t Toluene	10.965	343862	27.703 ng/ml
7) t Ethylbenzene	13.414	133817	9.560 ng/ml
8) t m-Xylene	13.547	284146	18.668 ng/ml
9) t O-Xylene	14.278	296582	19.005 ng/ml
10) t 1,2,4-Trimethylbenzene	16.560	323509	18.784 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062918\
Data File : FB016491.D
Signal(s) : FID2B.CH
Acq On : 29 Jun 2018 23:44
Operator : MJ/SJ
Sample : J3774-03MS
Misc : 5.00g/5.00mL DI Water
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 02 09:39:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Thu Jun 28 12:22:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

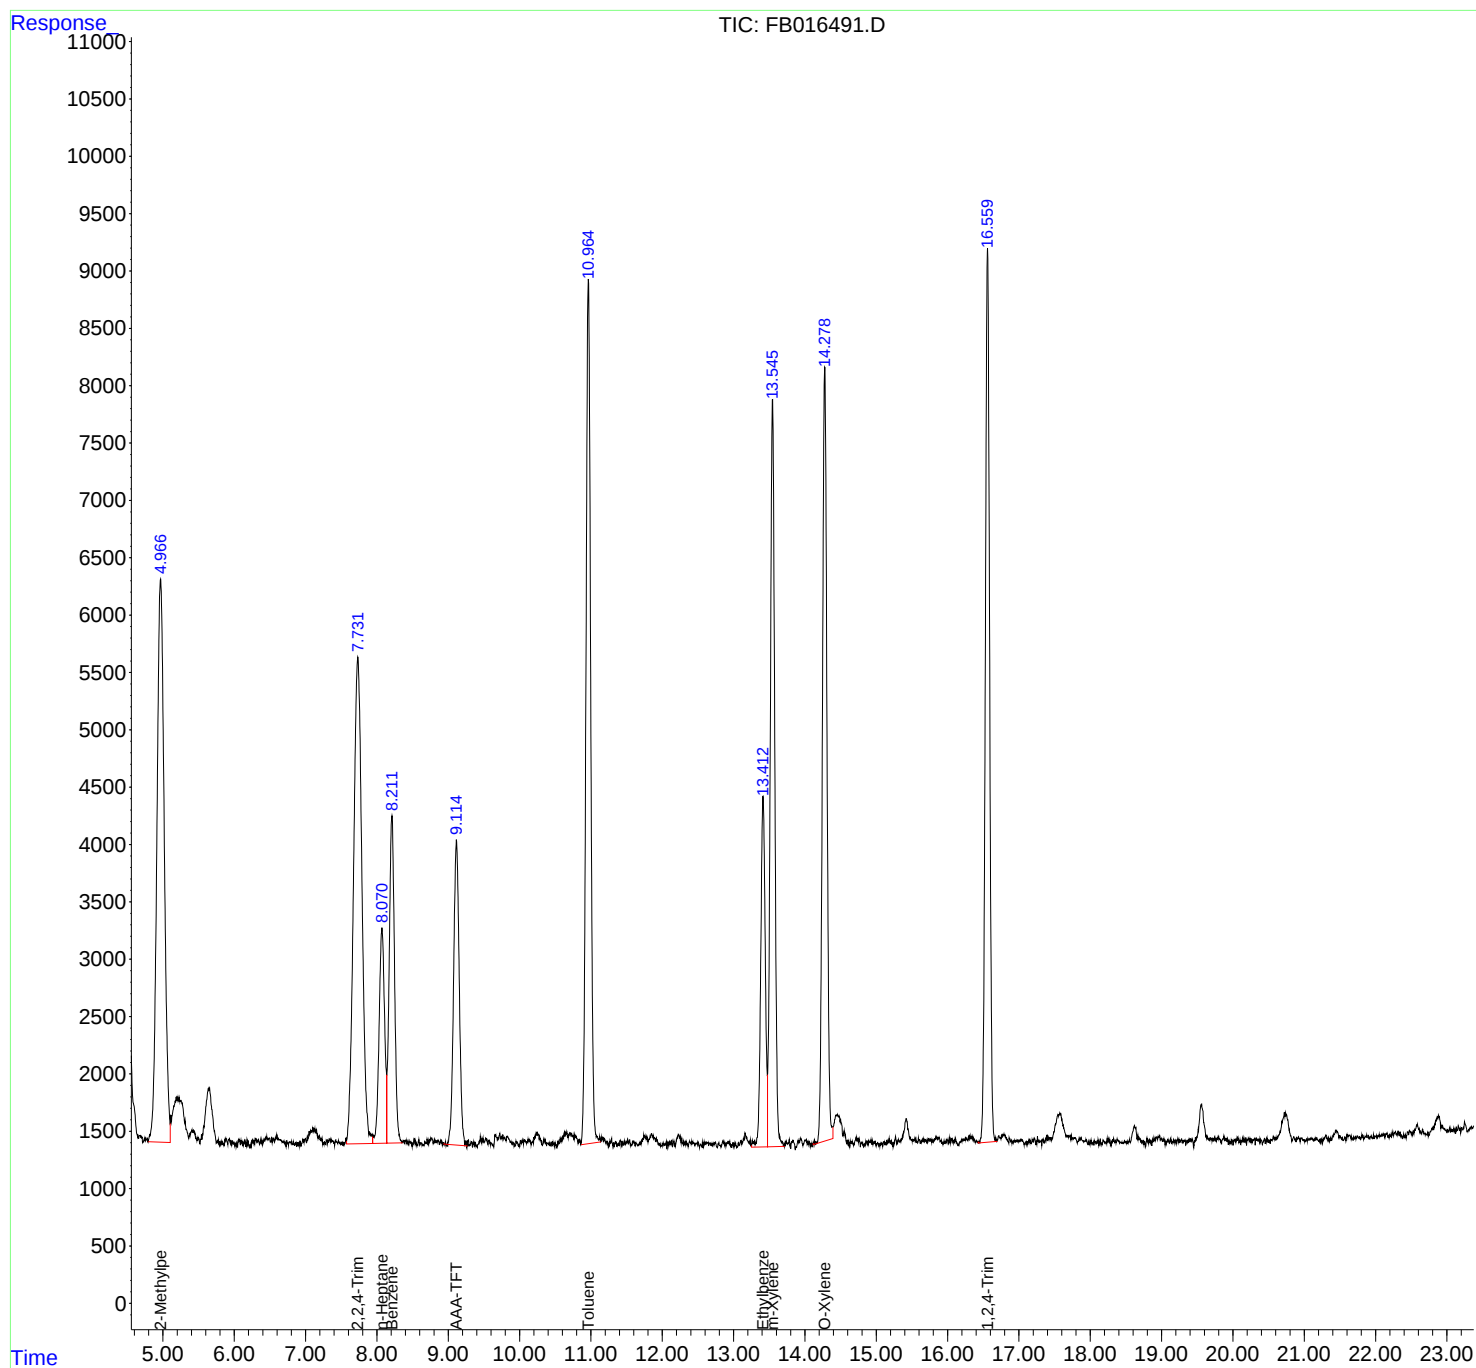


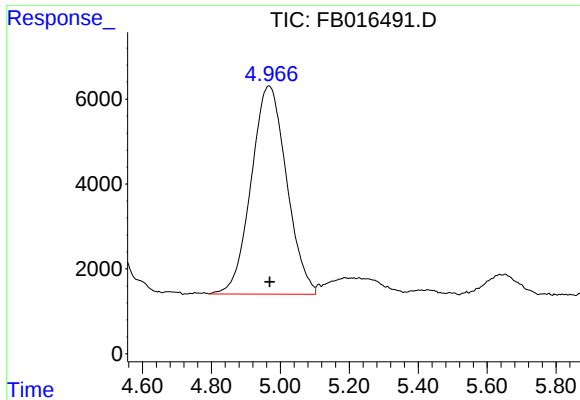

#1 2-Methylpentane


R.T.: 4.968 min
Delta R.T.: -0.001 min
Response: 350010
Conc: 28.86 ng/ml

Instrument :
FID_B
ClientSampleId :

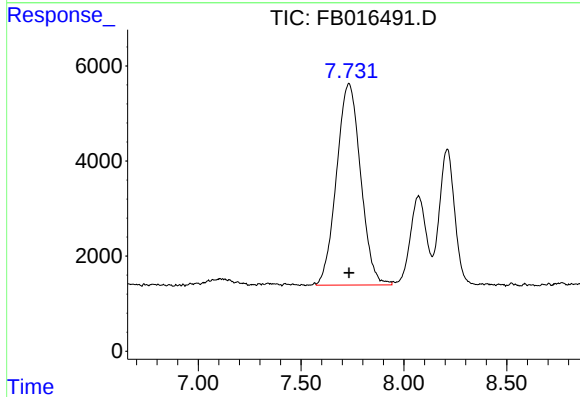


#2 2,2,4-Trimethylpentane

R.T.: 7.733 min
Delta R.T.: 0.000 min
Response: 344796
Conc: 29.77 ng/ml

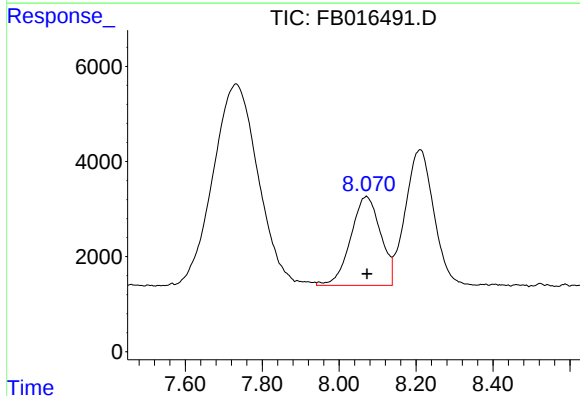


#3 n-Heptane

R.T.: 8.071 min
Delta R.T.: -0.002 min
Response: 100845
Conc: 9.21 ng/ml

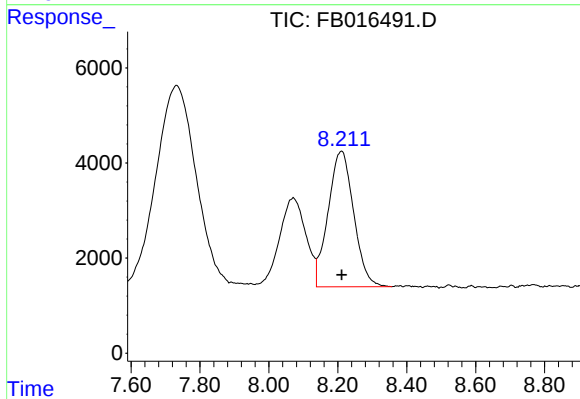

#4 Benzene


R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 146936
Conc: 9.90 ng/ml

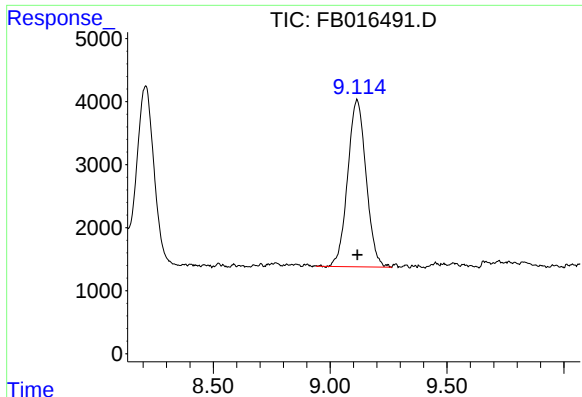

#5 AAA-TFT


R.T.: 9.116 min
Delta R.T.: -0.001 min
Response: 144838
Conc: 20.61 ng/ml

Instrument :
FID_B
ClientSampleId :

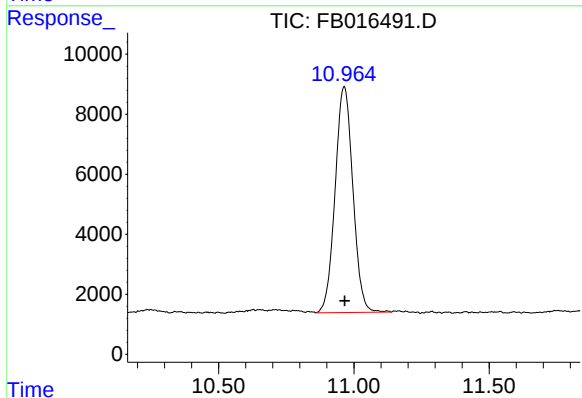


#6 Toluene

R.T.: 10.965 min
Delta R.T.: -0.001 min
Response: 343862
Conc: 27.70 ng/ml

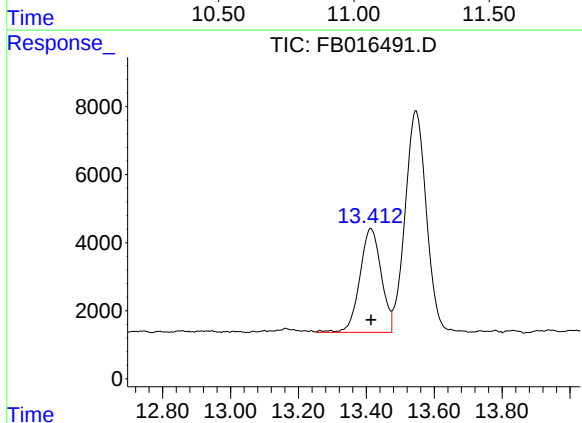


#7 Ethylbenzene

R.T.: 13.414 min
Delta R.T.: 0.000 min
Response: 133817
Conc: 9.56 ng/ml

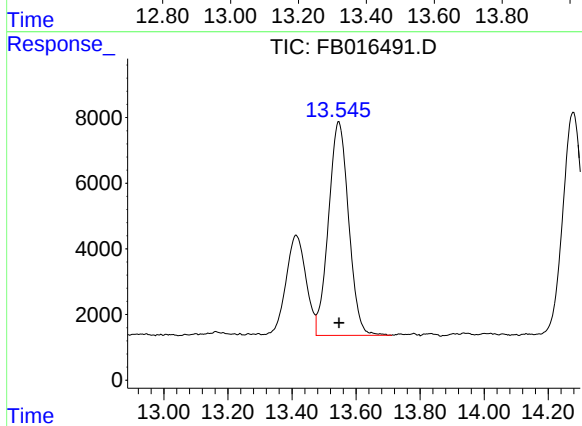

#8 m-Xylene


R.T.: 13.547 min
Delta R.T.: 0.000 min
Response: 284146
Conc: 18.67 ng/ml

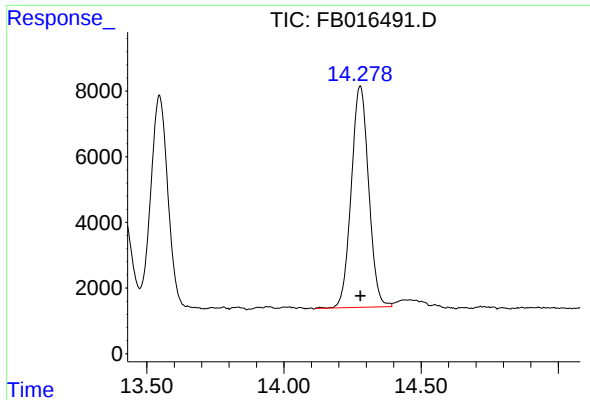

#9 O-Xylene

R.T.: 14.278 min
Delta R.T.: 0.000 min
Response: 296582
Conc: 19.01 ng/ml

Instrument :
FID_B
ClientSampleId :

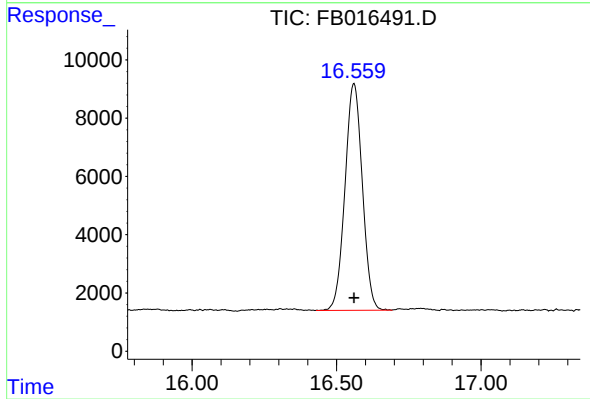

#10 1,2,4-Trimethylbenzene

R.T.: 16.560 min
Delta R.T.: 0.000 min
Response: 323509
Conc: 18.78 ng/ml