

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062918\
 Data File : FB016471.D
 Signal(s) : FID2B.CH
 Acq On : 29 Jun 2018 10:31
 Operator : MJ/SJ
 Sample : BSF0629S1
 Misc : 5.01g/5.00mL DI Water
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0629S1

Integration File: Calibration.e
 Quant Time: Jun 29 13:36:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Thu Jun 28 12:22:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.116	166942	23.755 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.967	387036	31.917 ng/ml
2) t 2,2,4-Trimethylpentane	7.733	375545	32.428 ng/ml
3) t n-Heptane	8.070	116820	10.674 ng/ml
4) t Benzene	8.210	156578	10.545 ng/ml
6) t Toluene	10.965	357430	28.796 ng/ml
7) t Ethylbenzene	13.413	136856	9.777 ng/ml
8) t m-Xylene	13.546	292804	19.237 ng/ml
9) t O-Xylene	14.278	306689	19.653 ng/ml
10) t 1,2,4-Trimethylbenzene	16.561	338567	19.658 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062918\
Data File : FB016471.D
Signal(s) : FID2B.CH
Acq On : 29 Jun 2018 10:31
Operator : MJ/SJ
Sample : BSF0629S1
Misc : 5.01g/5.00mL DI Water
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0629S1

Integration File: Calibration.e
Quant Time: Jun 29 13:36:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Thu Jun 28 12:22:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

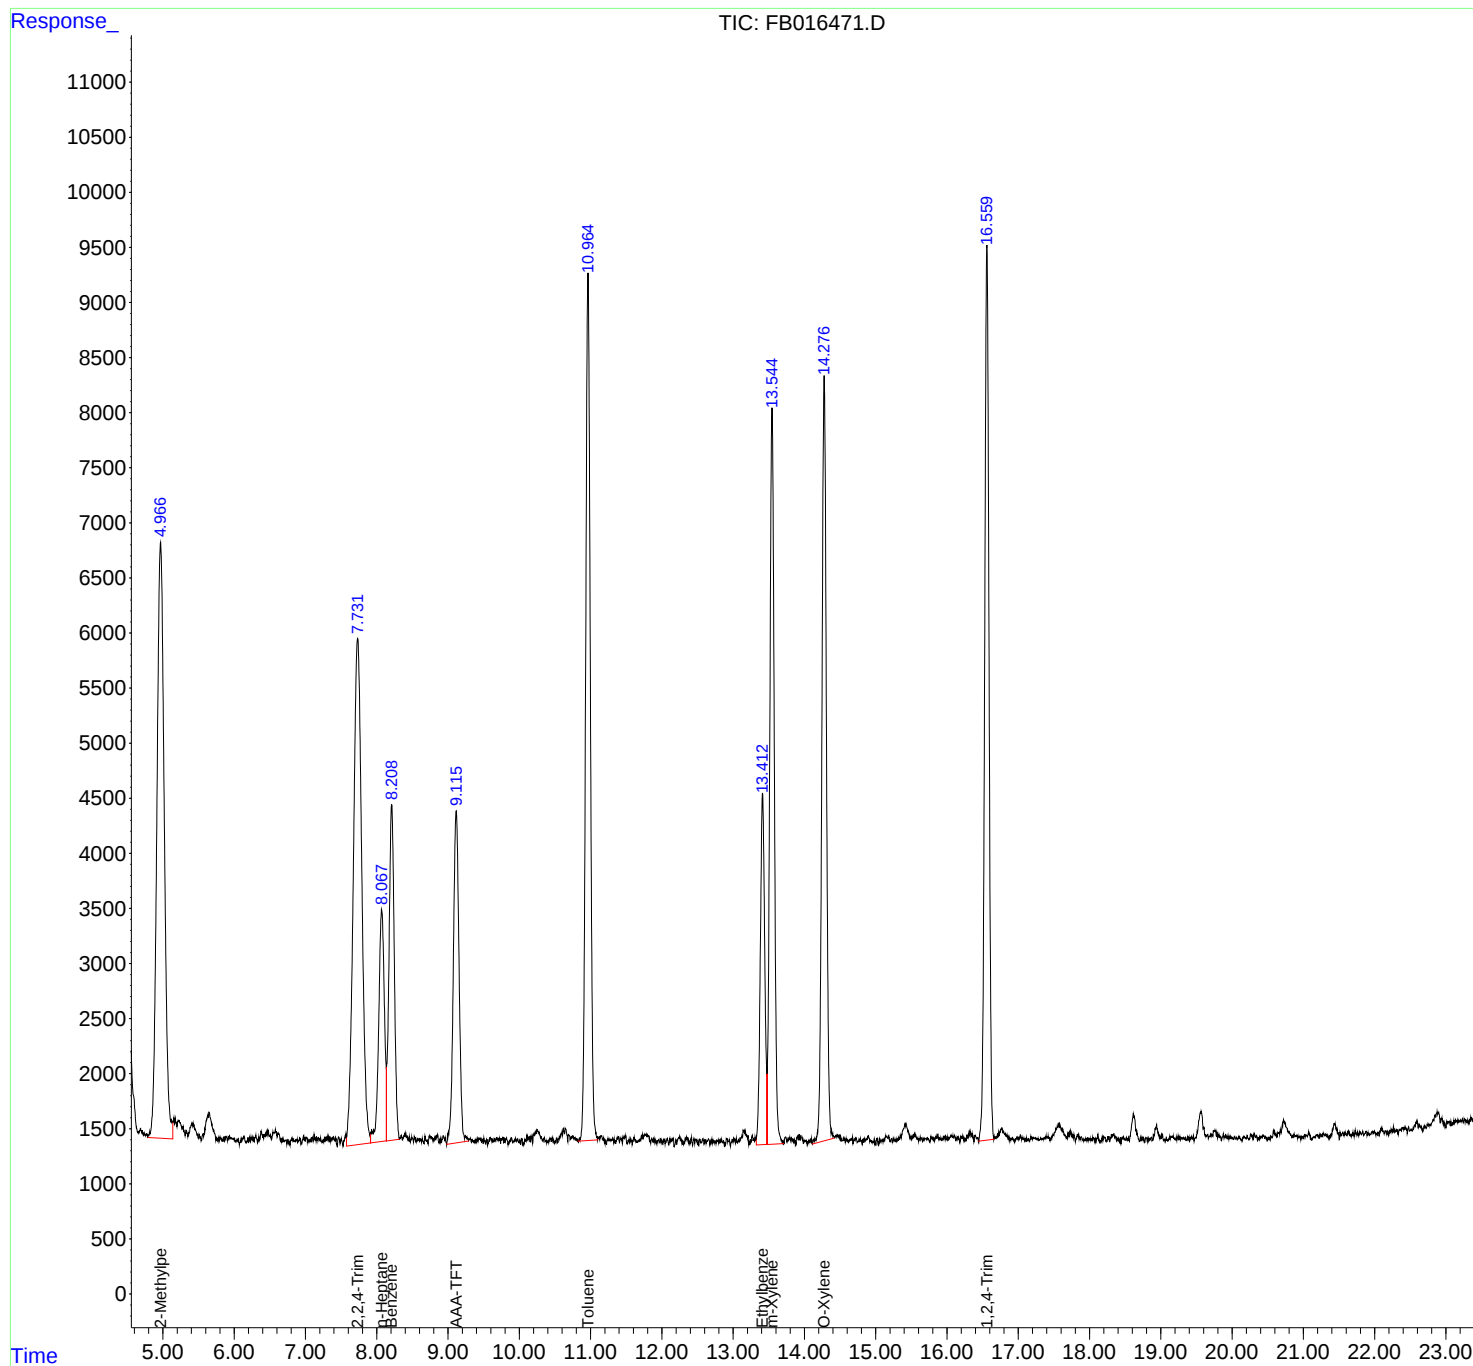


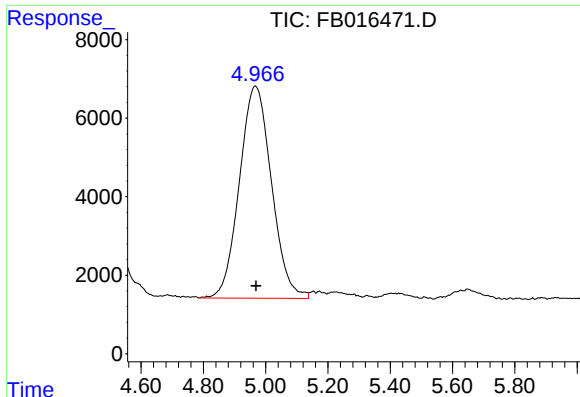

#1 2-Methylpentane


R.T.: 4.967 min
Delta R.T.: -0.002 min
Response: 387036
Conc: 31.92 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0629S1

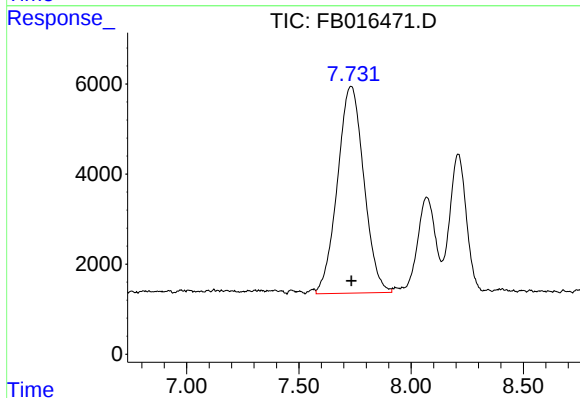


#2 2,2,4-Trimethylpentane

R.T.: 7.733 min
Delta R.T.: 0.000 min
Response: 375545
Conc: 32.43 ng/ml

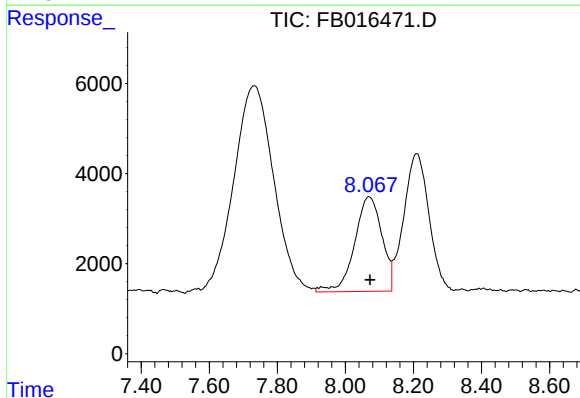


#3 n-Heptane

R.T.: 8.070 min
Delta R.T.: -0.003 min
Response: 116820
Conc: 10.67 ng/ml

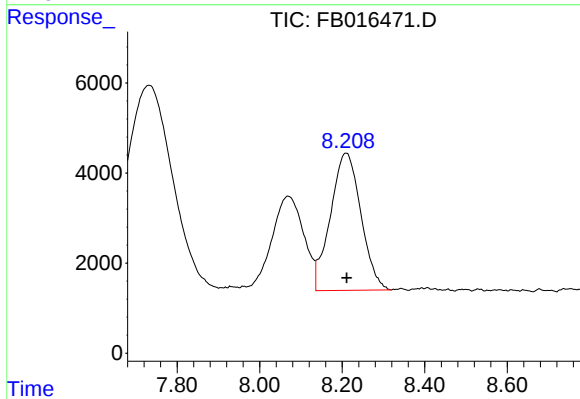

#4 Benzene


R.T.: 8.210 min
Delta R.T.: -0.001 min
Response: 156578
Conc: 10.55 ng/ml

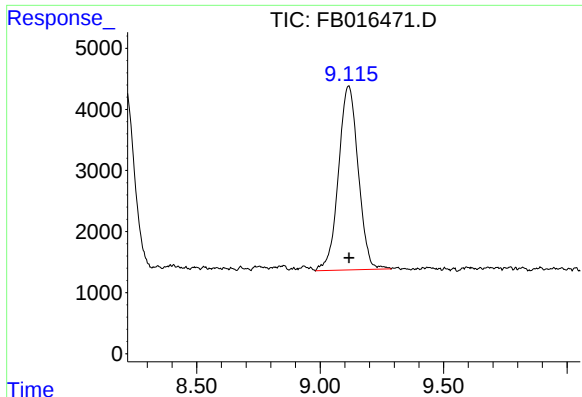

#5 AAA-TFT


R.T.: 9.116 min
Delta R.T.: -0.001 min
Response: 166942
Conc: 23.75 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0629S1

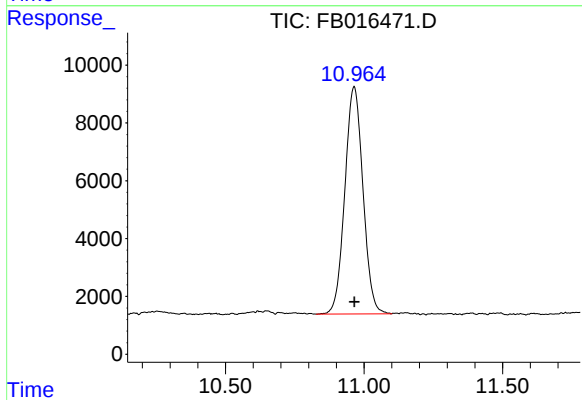


#6 Toluene

R.T.: 10.965 min
Delta R.T.: -0.001 min
Response: 357430
Conc: 28.80 ng/ml

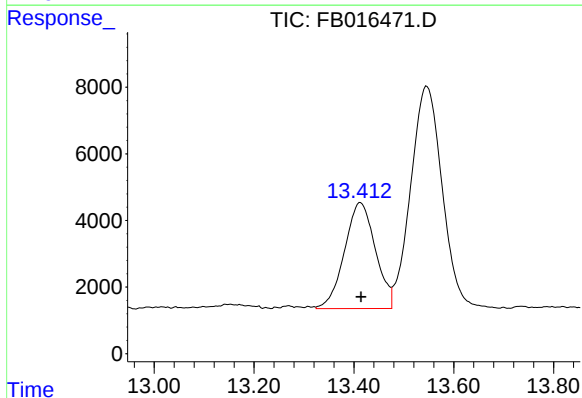


#7 Ethylbenzene

R.T.: 13.413 min
Delta R.T.: -0.001 min
Response: 136856
Conc: 9.78 ng/ml

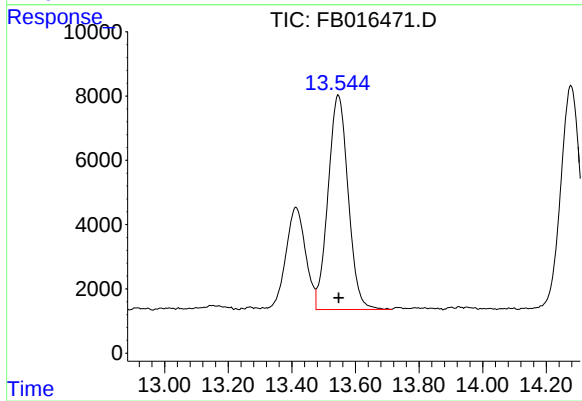

#8 m-Xylene


R.T.: 13.546 min
Delta R.T.: 0.000 min
Response: 292804
Conc: 19.24 ng/ml

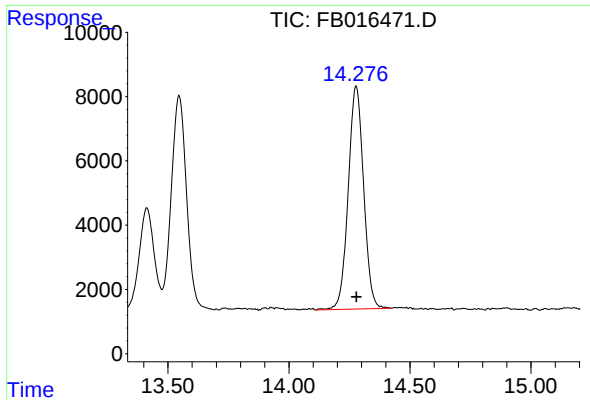

#9 O-Xylene

R.T.: 14.278 min
Delta R.T.: 0.000 min
Response: 306689
Conc: 19.65 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0629S1

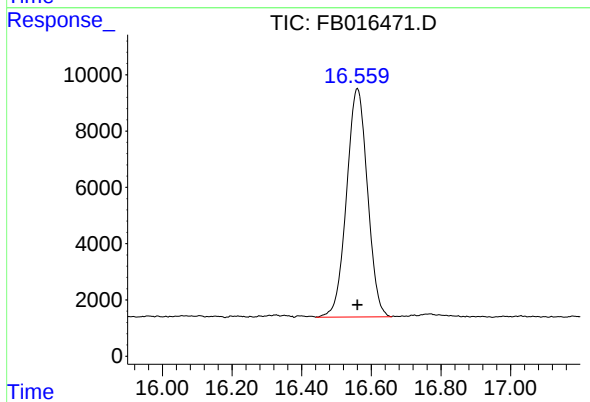

#10 1,2,4-Trimethylbenzene

R.T.: 16.561 min
Delta R.T.: 0.000 min
Response: 338567
Conc: 19.66 ng/ml