

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062918\
 Data File : FB016474.D
 Signal(s) : FID2B.CH
 Acq On : 29 Jun 2018 12:23
 Operator : MJ/SJ
 Sample : J3631-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 S83-0020MSD

Integration File: Calibration.e
 Quant Time: Jun 29 13:37:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Thu Jun 28 12:22:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.120	188005	26.752 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.968	453249	37.378 ng/ml
2) t 2,2,4-Trimethylpentane	7.728	469067	40.503 ng/ml
3) t n-Heptane	8.072	174740	15.966 ng/ml
4) t Benzene	8.211	169653	11.426 ng/ml
6) t Toluene	10.966	399055	32.149 ng/ml
7) t Ethylbenzene	13.414	342944	24.500 ng/ml
8) t m-Xylene	13.547	344780	22.652 ng/ml
9) t O-Xylene	14.279	349032	22.366 ng/ml
10) t 1,2,4-Trimethylbenzene	16.562	611071	35.480 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062918\
Data File : FB016474.D
Signal(s) : FID2B.CH
Acq On : 29 Jun 2018 12:23
Operator : MJ/SJ
Sample : J3631-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
S83-0020MSD

Integration File: Calibration.e
Quant Time: Jun 29 13:37:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Thu Jun 28 12:22:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

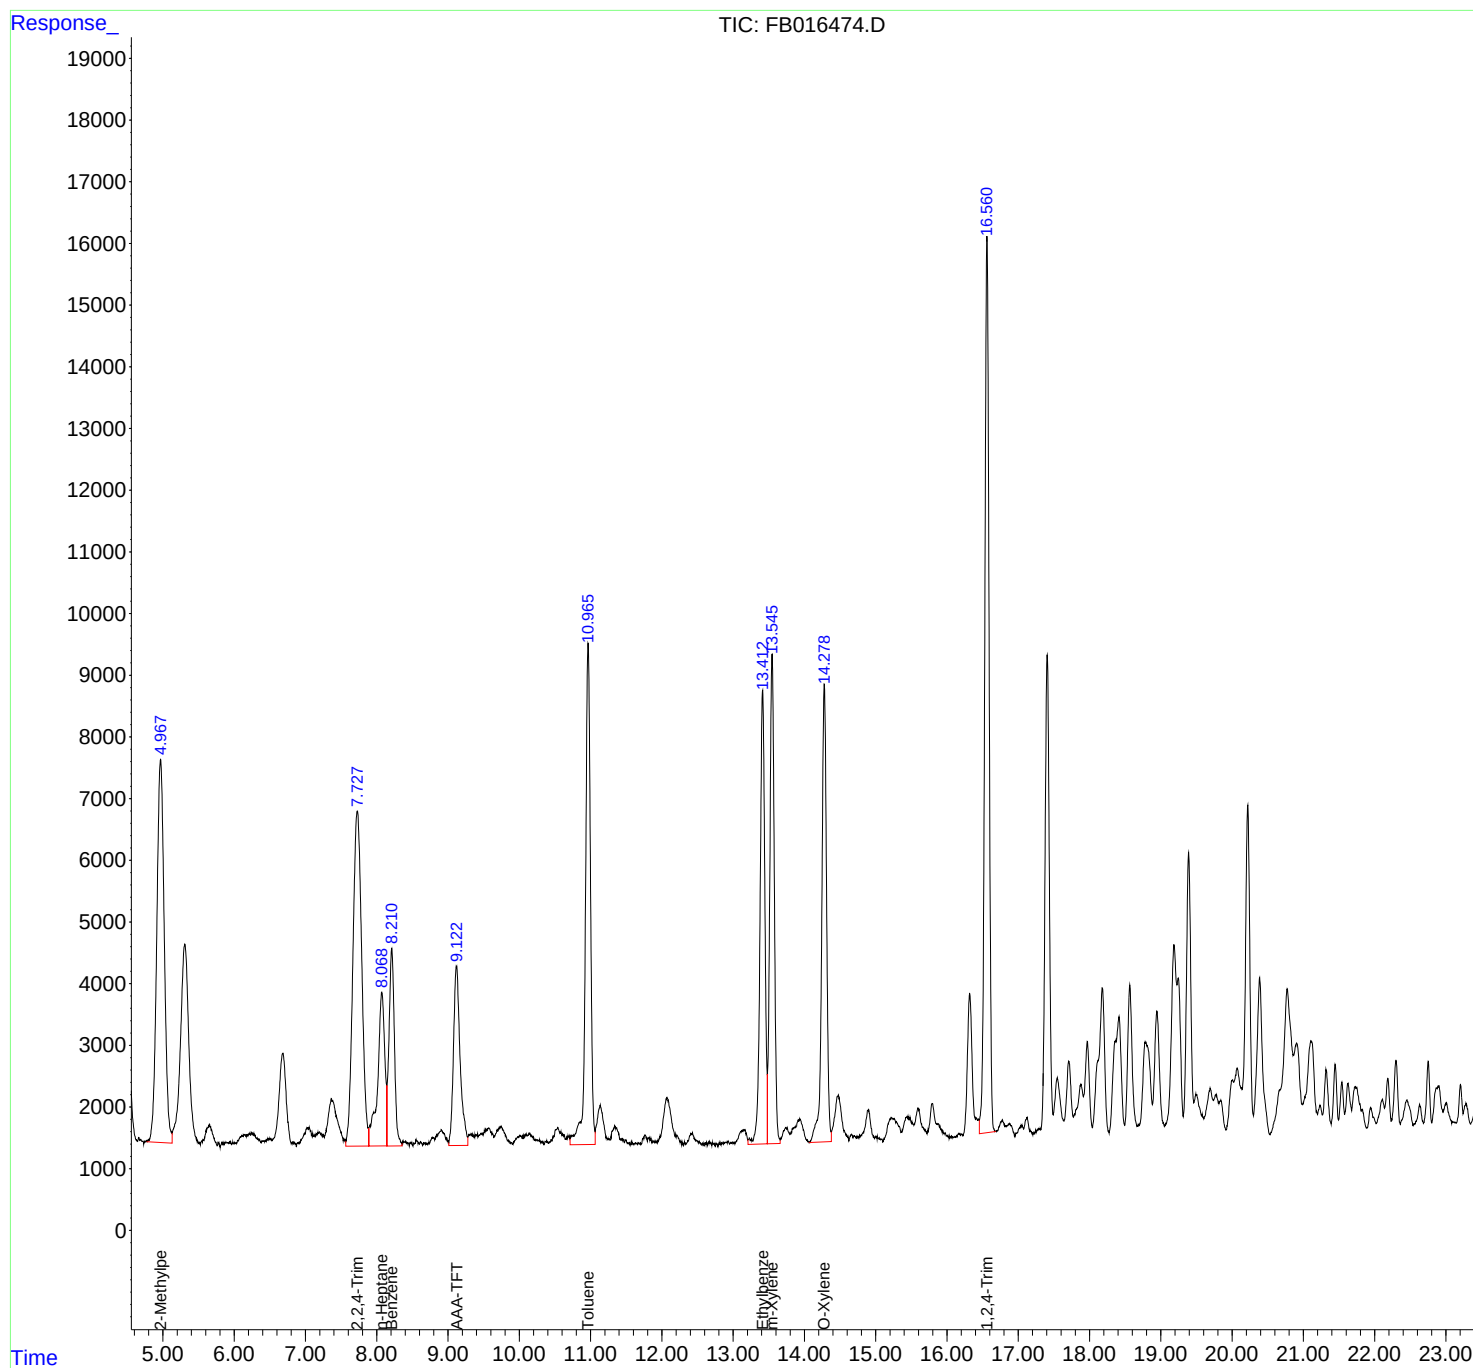


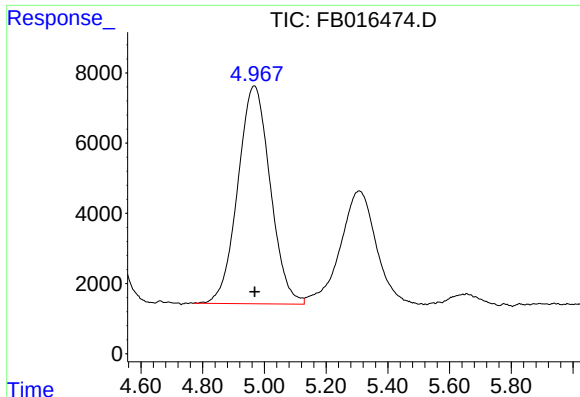

#1 2-Methylpentane


R.T.: 4.968 min
Delta R.T.: 0.000 min
Response: 453249
Conc: 37.38 ng/ml

Instrument :
FID_B
ClientSampleId :
S83-0020MSD

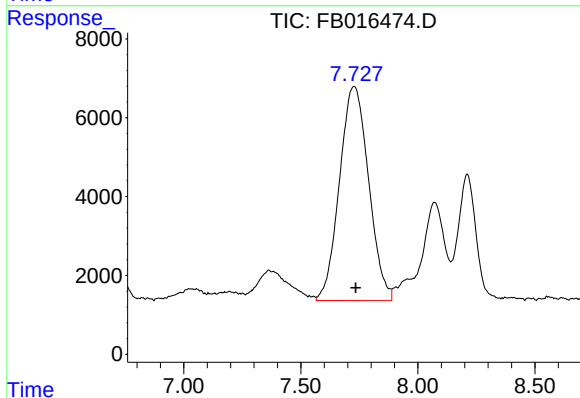


#2 2,2,4-Trimethylpentane

R.T.: 7.728 min
Delta R.T.: -0.006 min
Response: 469067
Conc: 40.50 ng/ml

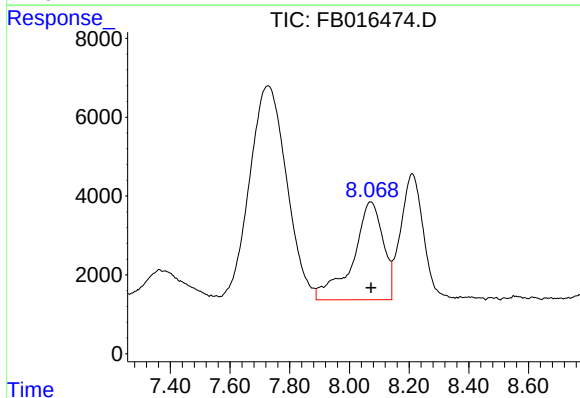


#3 n-Heptane

R.T.: 8.072 min
Delta R.T.: -0.001 min
Response: 174740
Conc: 15.97 ng/ml

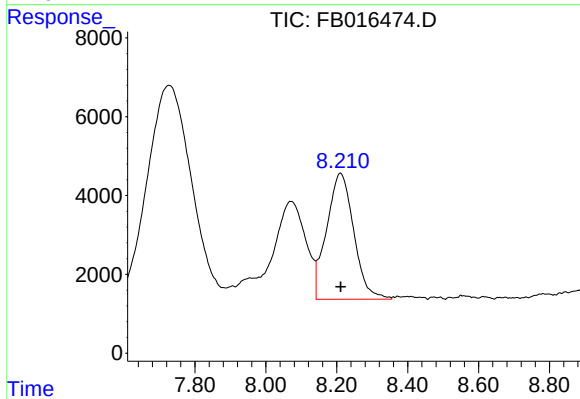

#4 Benzene


R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 169653
Conc: 11.43 ng/ml

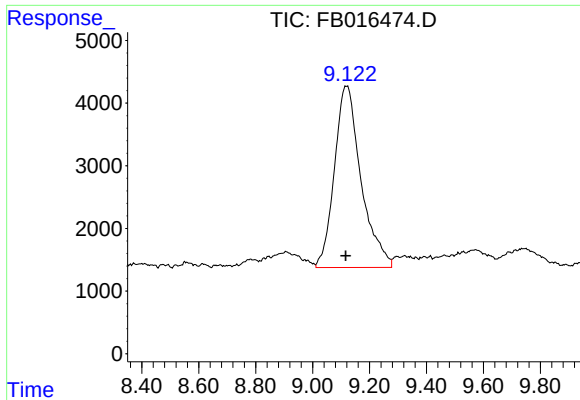

#5 AAA-TFT


R.T.: 9.120 min
Delta R.T.: 0.003 min
Response: 188005
Conc: 26.75 ng/ml

Instrument :
FID_B
ClientSampleId :
S83-0020MSD

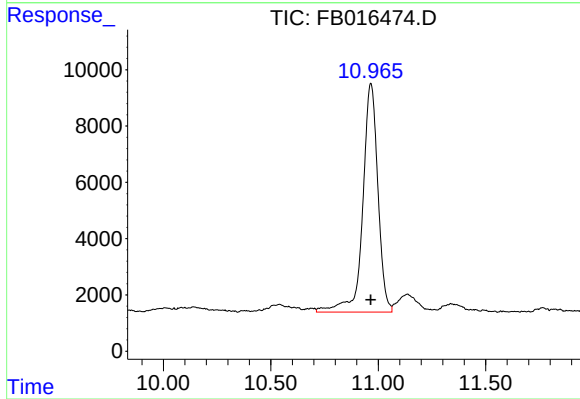


#6 Toluene

R.T.: 10.966 min
Delta R.T.: 0.000 min
Response: 399055
Conc: 32.15 ng/ml

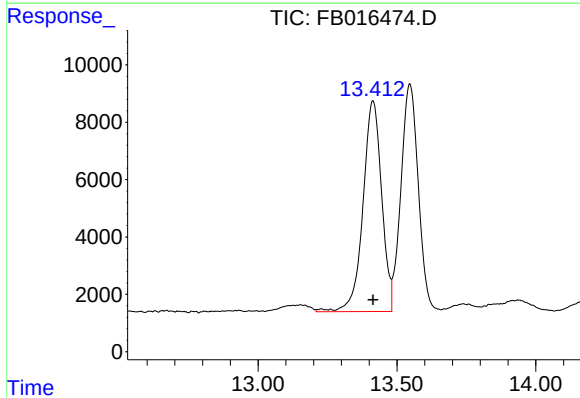


#7 Ethylbenzene

R.T.: 13.414 min
Delta R.T.: 0.000 min
Response: 342944
Conc: 24.50 ng/ml

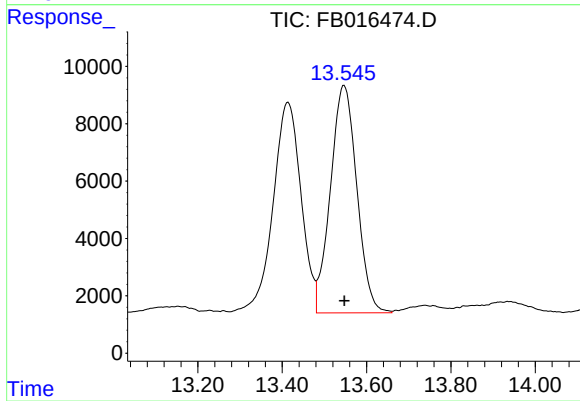

#8 m-Xylene


R.T.: 13.547 min
Delta R.T.: 0.000 min
Response: 344780
Conc: 22.65 ng/ml

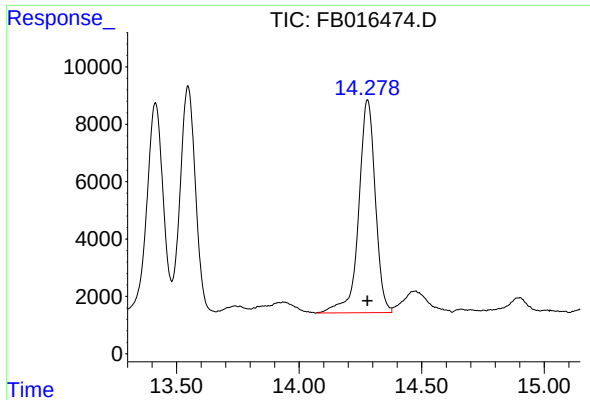

#9 O-Xylene

R.T.: 14.279 min
Delta R.T.: 0.000 min
Response: 349032
Conc: 22.37 ng/ml

Instrument :
FID_B
ClientSampleId :
S83-0020MSD

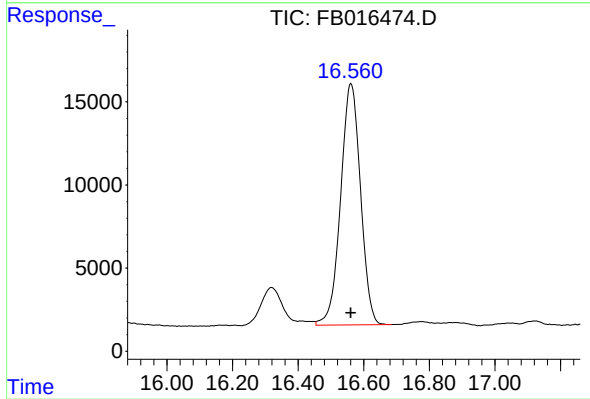

#10 1,2,4-Trimethylbenzene

R.T.: 16.562 min
Delta R.T.: 0.001 min
Response: 611071
Conc: 35.48 ng/ml