

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062921\
 Data File : FB025942.D
 Signal(s) : FID2B.CH
 Acq On : 29 Jun 2021 11:03
 Operator : AJ/MA
 Sample : BSF0629W1
 Misc : 5.02g/5.00 ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 30 01:10:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.218	450742	18.651 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.167	725523	27.569 ng/ml
2) t 2,2,4-Trimethylpentane	7.872	606301	30.097 ng/ml
3) t n-Heptane	8.191	339704	9.450 ng/ml
4) t Benzene	8.342	379896	9.100 ng/ml
6) t Toluene	11.039	1058119	25.713 ng/ml
7) t Ethylbenzene	13.446	317389	8.328 ng/ml
8) t m-Xylene	13.577	611256	15.549 ng/ml
9) t O-Xylene	14.299	543140	17.034 ng/ml
10) t 1,2,4-Trimethylbenzene	16.552	317251	16.118 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062921\
Data File : FB025942.D
Signal(s) : FID2B.CH
Acq On : 29 Jun 2021 11:03
Operator : AJ/MA
Sample : BSF0629W1
Misc : 5.02g/5.00 ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 30 01:10:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

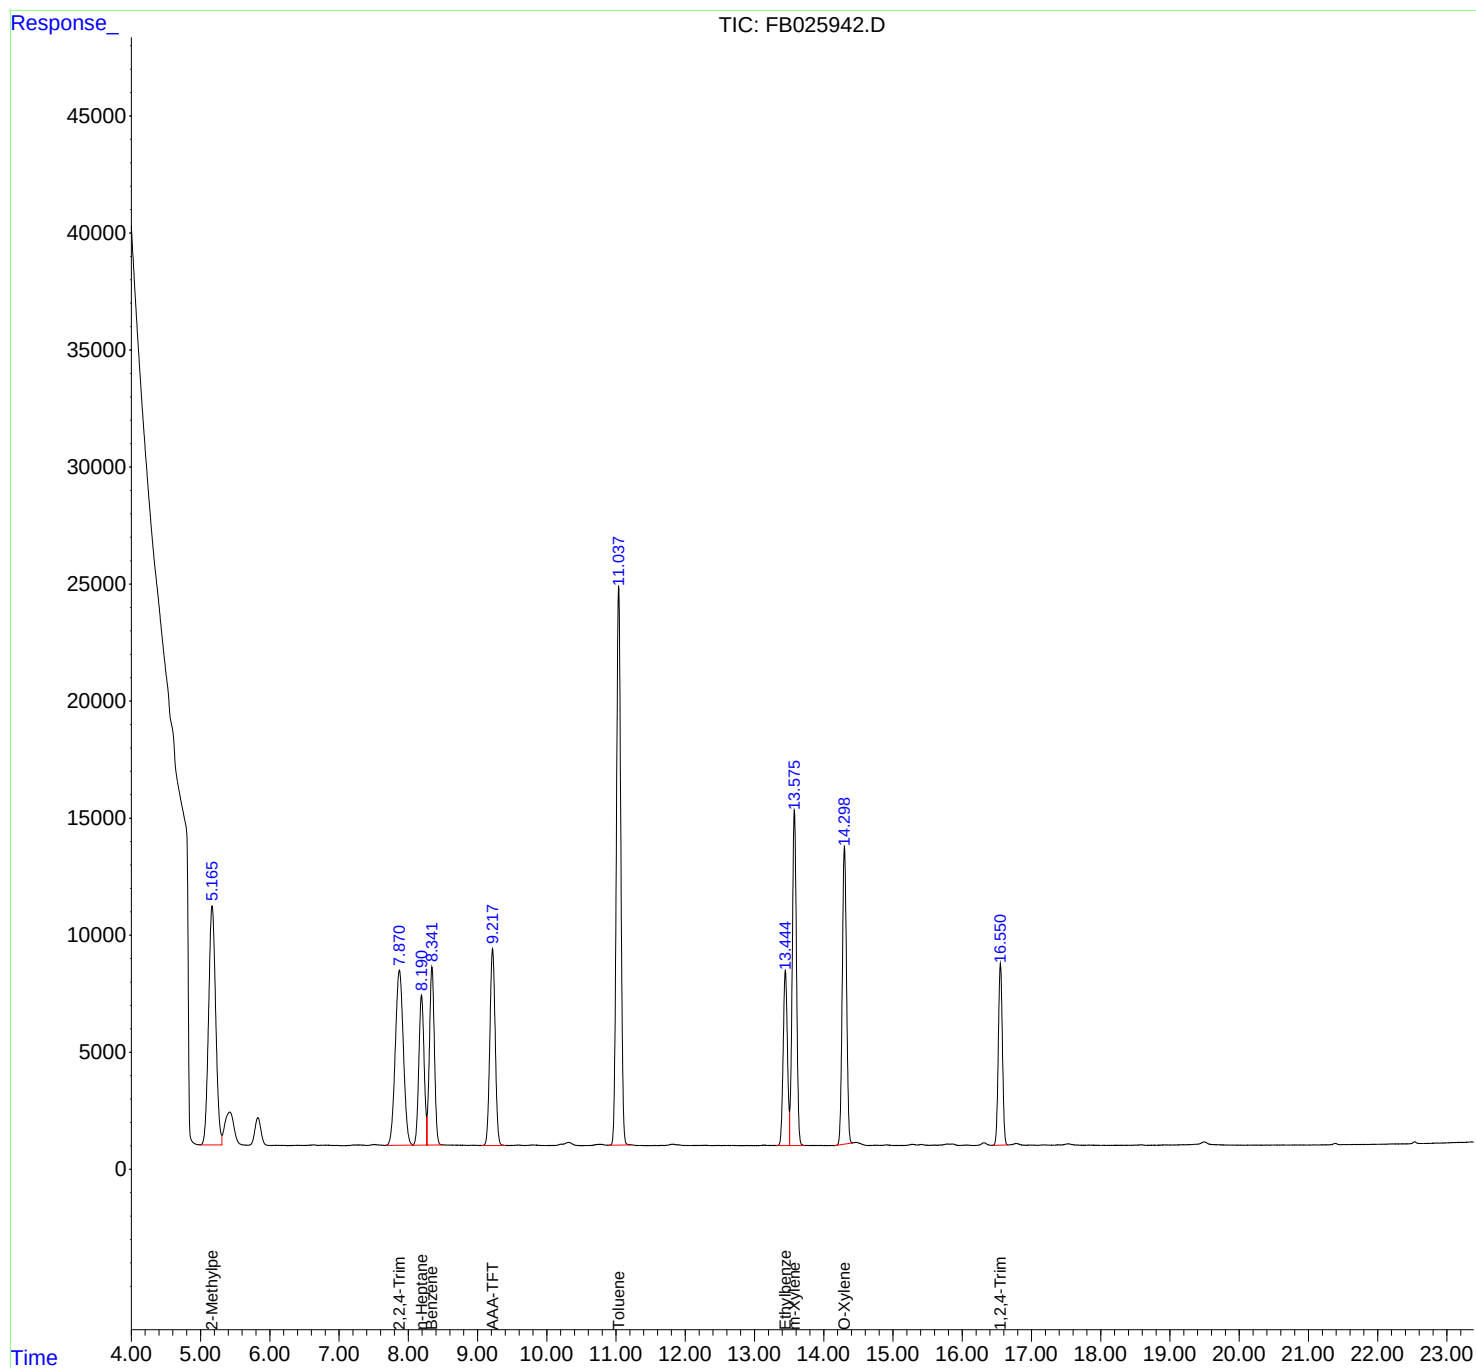

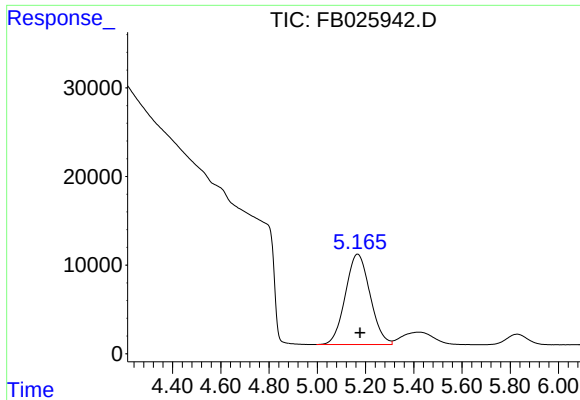


#1 2-Methylpentane

R.T.: 5.167 min
Delta R.T.: -0.010 min
Response: 725523
Conc: 27.57 ng/ml

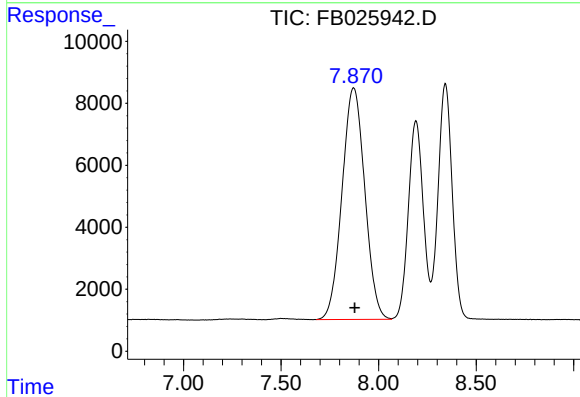


#2 2,2,4-Trimethylpentane

R.T.: 7.872 min
Delta R.T.: -0.006 min
Response: 606301
Conc: 30.10 ng/ml

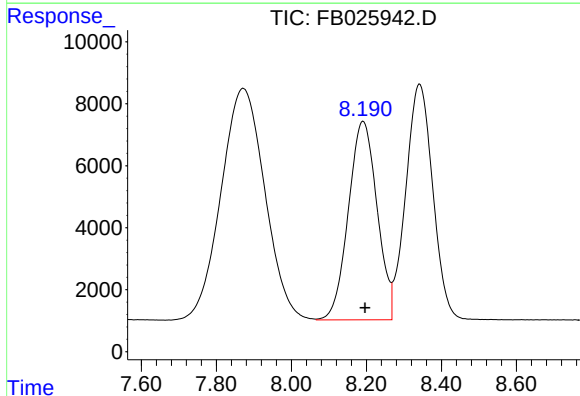


#3 n-Heptane

R.T.: 8.191 min
Delta R.T.: -0.004 min
Response: 339704
Conc: 9.45 ng/ml

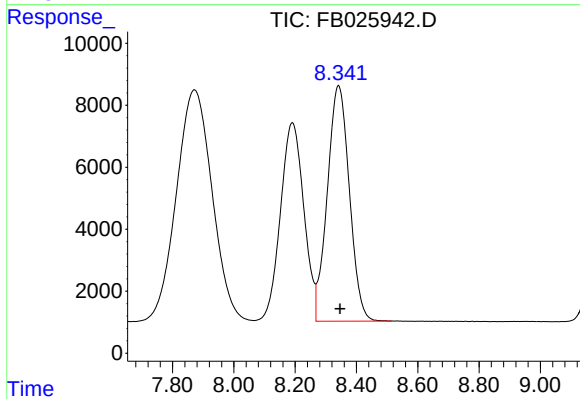


#4 Benzene

R.T.: 8.342 min
Delta R.T.: -0.005 min
Response: 379896
Conc: 9.10 ng/ml

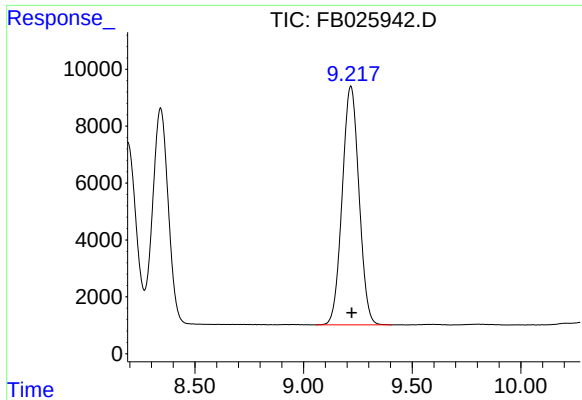


#5 AAA-TFT

R.T.: 9.218 min
Delta R.T.: -0.003 min
Response: 450742
Conc: 18.65 ng/ml

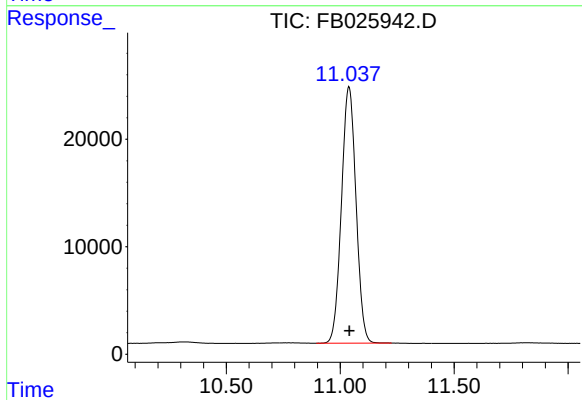


#6 Toluene

R.T.: 11.039 min
Delta R.T.: -0.003 min
Response: 1058119
Conc: 25.71 ng/ml

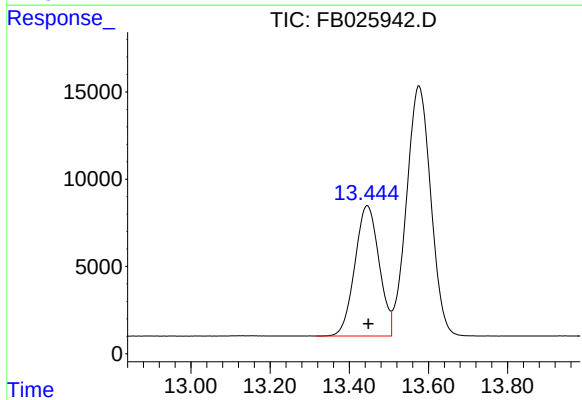


#7 Ethylbenzene

R.T.: 13.446 min
Delta R.T.: -0.002 min
Response: 317389
Conc: 8.33 ng/ml

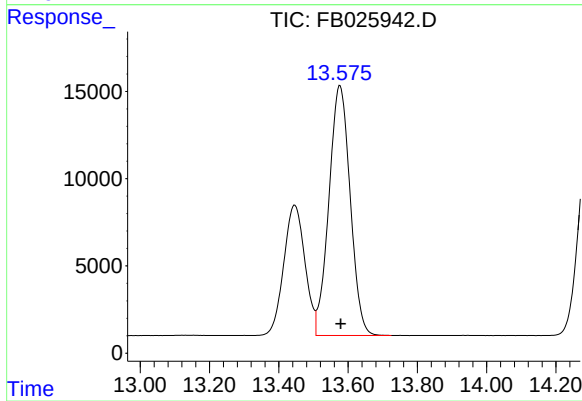


#8 m-Xylene

R.T.: 13.577 min
Delta R.T.: -0.002 min
Response: 611256
Conc: 15.55 ng/ml

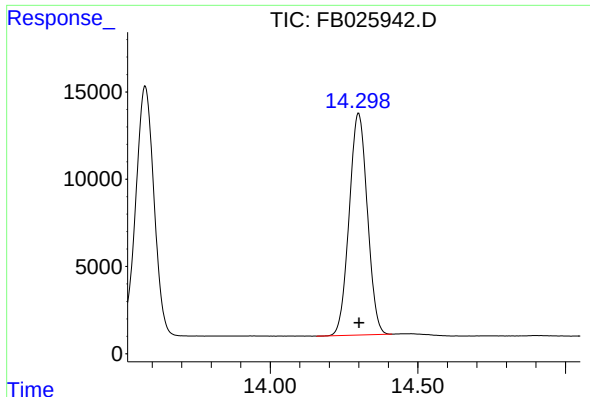

#9 O-Xylene

R.T.: 14.299 min
Delta R.T.: -0.002 min
Response: 543140
Conc: 17.03 ng/ml

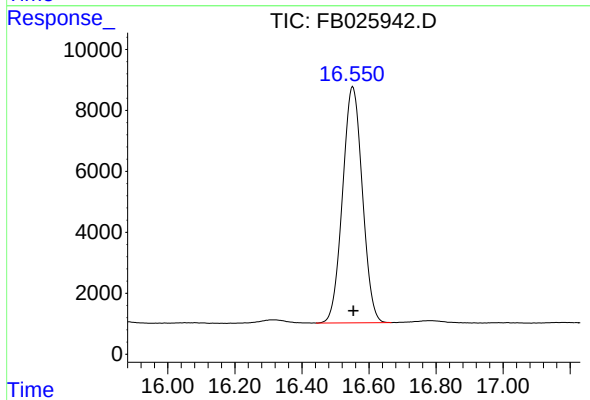

#10 1,2,4-Trimethylbenzene

R.T.: 16.552 min
Delta R.T.: -0.002 min
Response: 317251
Conc: 16.12 ng/ml