

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062921\
 Data File : FB025951.D
 Signal(s) : FID2B.CH
 Acq On : 29 Jun 2021 16:37
 Operator : AJ/MA
 Sample : M2857-04MSD
 Misc : 5.00g/5.00 ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 30 01:11:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.233	415286	17.184 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.203	586433	22.284 ng/ml
2) t 2,2,4-Trimethylpentane	7.897	474906	23.574 ng/ml
3) t n-Heptane	8.210	300086	8.348 ng/ml
4) t Benzene	8.362	321730	7.707 ng/ml
6) t Toluene	11.050	881105	21.412 ng/ml
7) t Ethylbenzene	13.454	260748	6.842 ng/ml
8) t m-Xylene	13.584	499121	12.696 ng/ml
9) t O-Xylene	14.307	441305	13.841 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	261659	13.294 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062921\
Data File : FB025951.D
Signal(s) : FID2B.CH
Acq On : 29 Jun 2021 16:37
Operator : AJ/MA
Sample : M2857-04MSD
Misc : 5.00g/5.00 ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 30 01:11:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

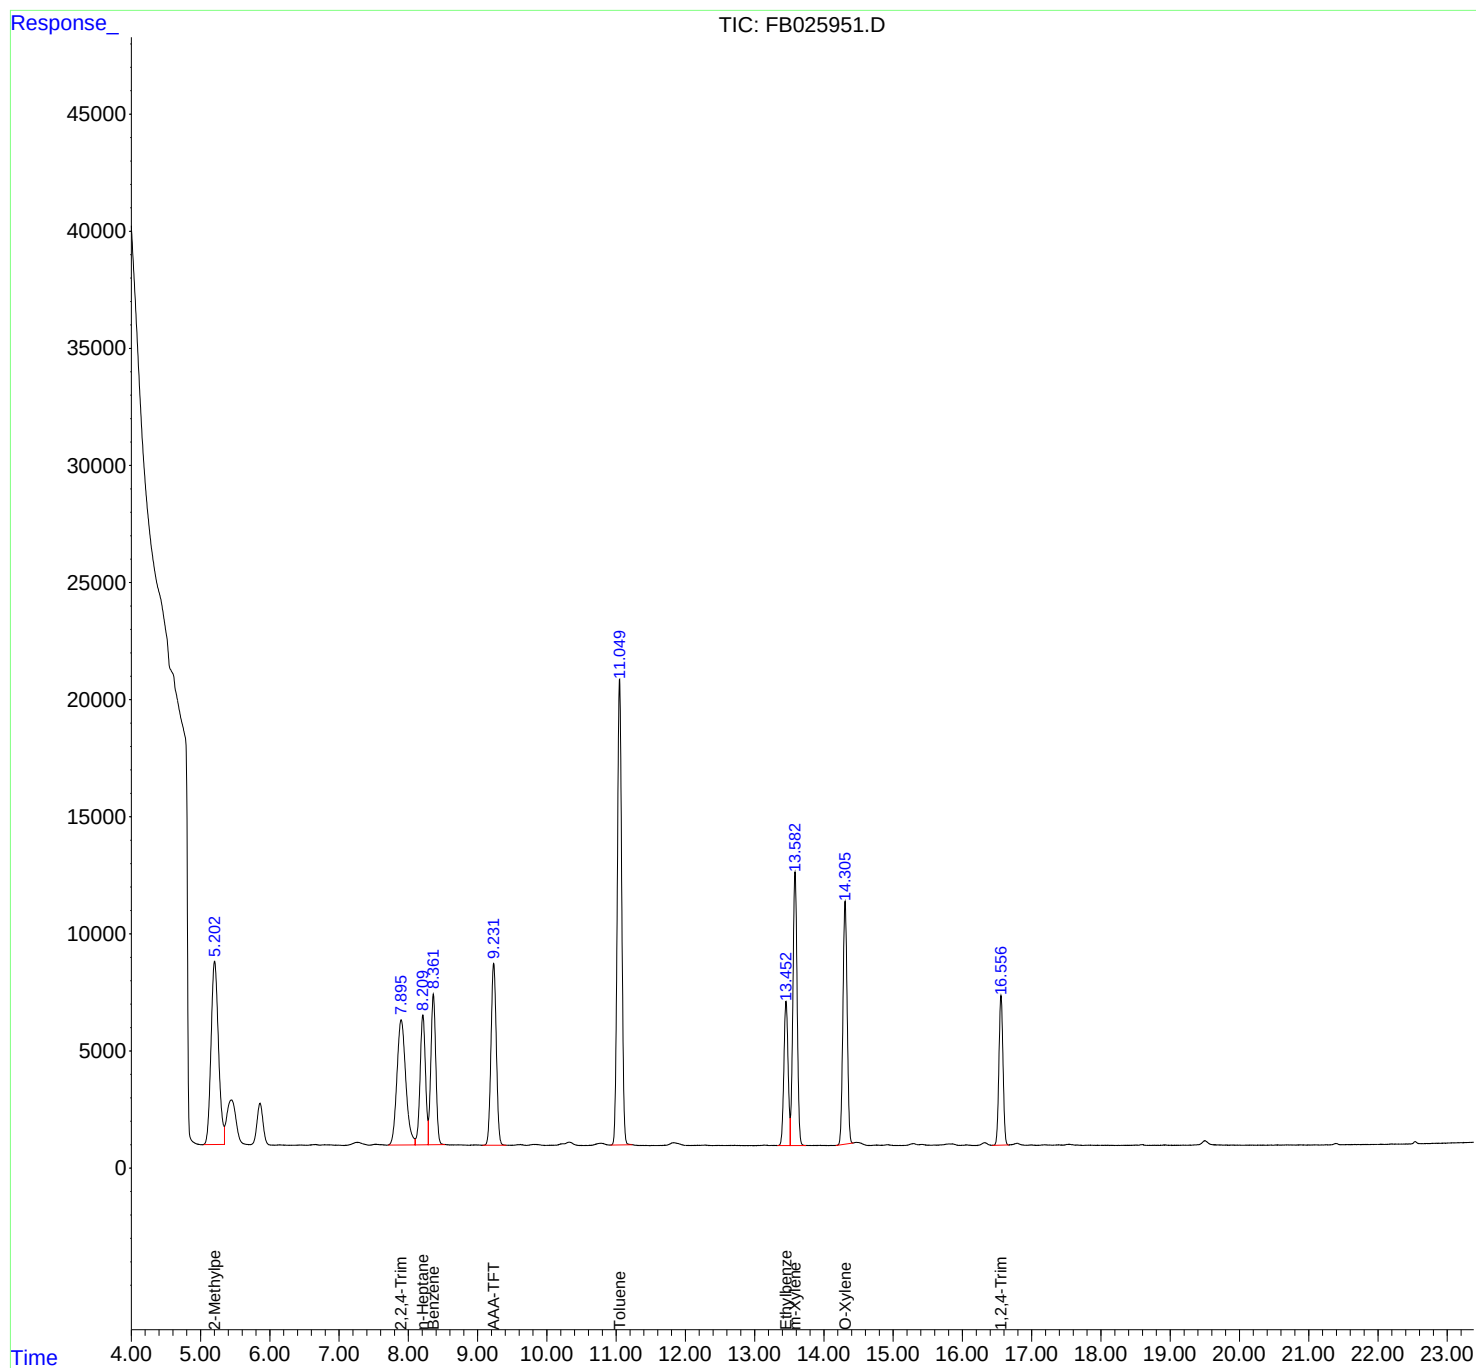

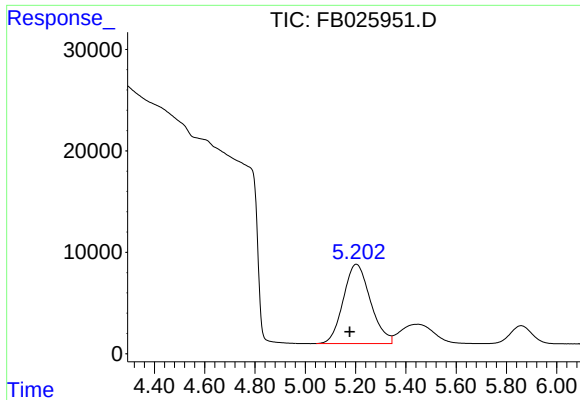


#1 2-Methylpentane

R.T.: 5.203 min
Delta R.T.: 0.026 min
Response: 586433
Conc: 22.28 ng/ml

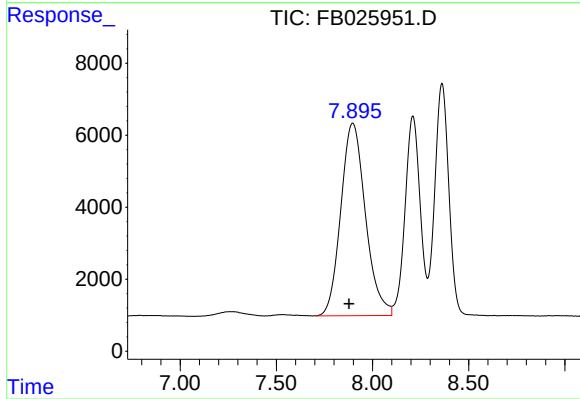


#2 2,2,4-Trimethylpentane

R.T.: 7.897 min
Delta R.T.: 0.019 min
Response: 474906
Conc: 23.57 ng/ml

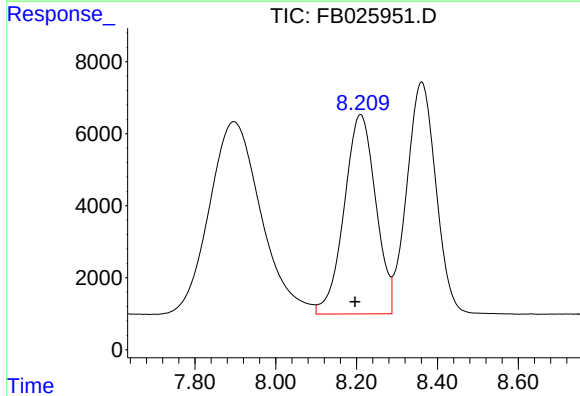


#3 n-Heptane

R.T.: 8.210 min
Delta R.T.: 0.014 min
Response: 300086
Conc: 8.35 ng/ml

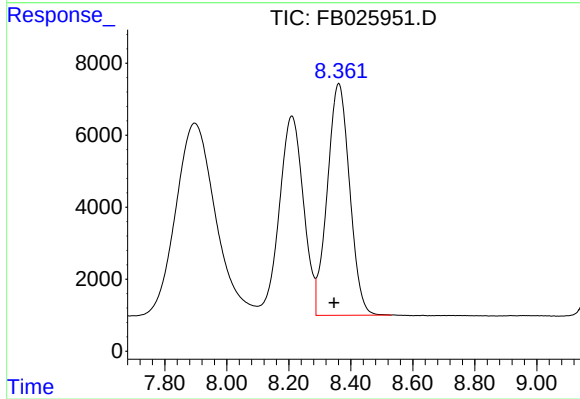


#4 Benzene

R.T.: 8.362 min
Delta R.T.: 0.015 min
Response: 321730
Conc: 7.71 ng/ml

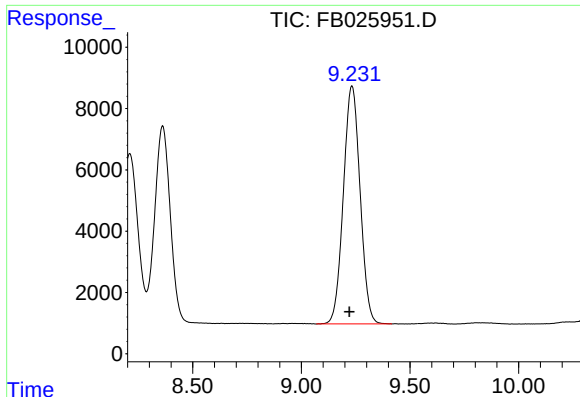


#5 AAA-TFT

R.T.: 9.233 min
Delta R.T.: 0.012 min
Response: 415286
Conc: 17.18 ng/ml

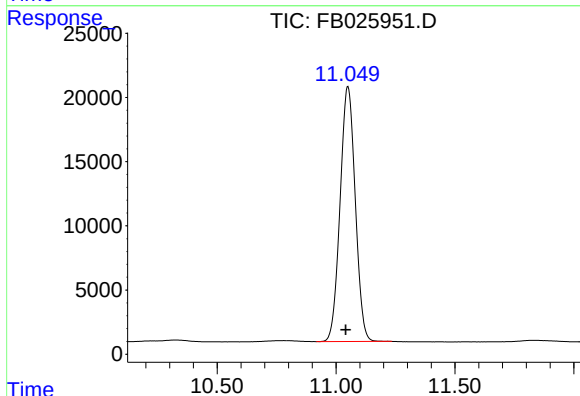


#6 Toluene

R.T.: 11.050 min
Delta R.T.: 0.009 min
Response: 881105
Conc: 21.41 ng/ml

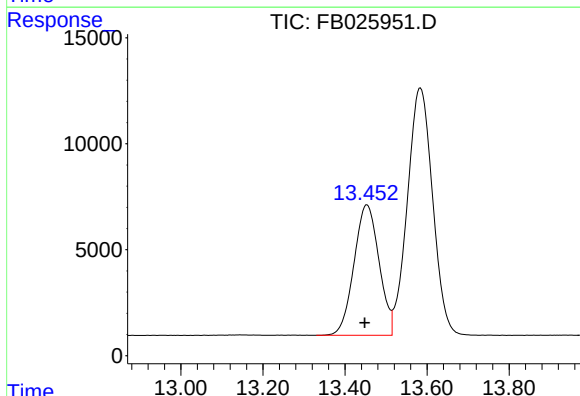


#7 Ethylbenzene

R.T.: 13.454 min
Delta R.T.: 0.006 min
Response: 260748
Conc: 6.84 ng/ml

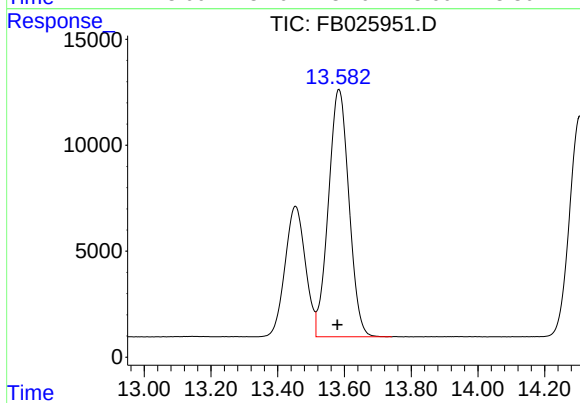


#8 m-Xylene

R.T.: 13.584 min
Delta R.T.: 0.005 min
Response: 499121
Conc: 12.70 ng/ml

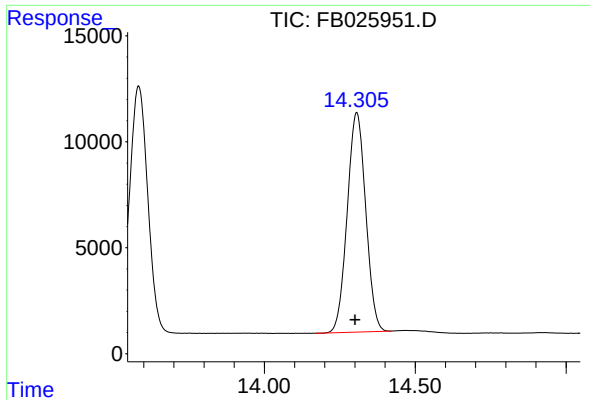

#9 O-Xylene

R.T.: 14.307 min
Delta R.T.: 0.005 min
Response: 441305
Conc: 13.84 ng/ml

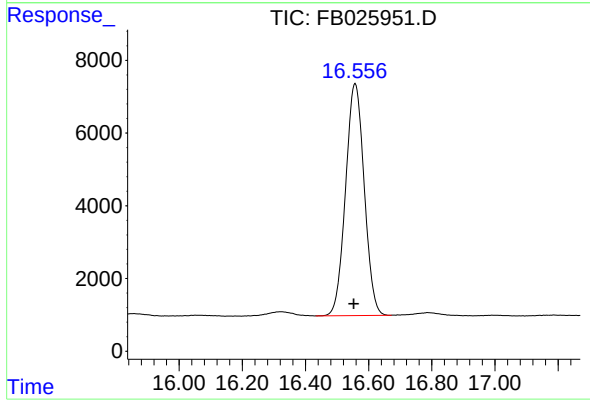

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.004 min
Response: 261659
Conc: 13.29 ng/ml