

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062921\
 Data File : FB025959.D
 Signal(s) : FID2B.CH
 Acq On : 29 Jun 2021 23:21
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc : 5.02g/5.00 ml DI WATER
 ALS Vial : 23 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 30 01:37:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.219	415118	17.177 ng/ml
Target Compounds				
1) t	2-Methylpentane	5.167	662513	25.174 ng/ml
2) t	2,2,4-Trimethylpentane	7.874	553164	27.459 ng/ml
3) t	n-Heptane	8.192	317886	8.844 ng/ml
4) t	Benzene	8.343	349156	8.364 ng/ml
6) t	Toluene	11.040	976235	23.723 ng/ml
7) t	Ethylbenzene	13.448	288300	7.565 ng/ml
8) t	m-Xylene	13.578	550979	14.016 ng/ml
9) t	O-Xylene	14.301	484395	15.192 ng/ml
10) t	1,2,4-Trimethylbenzene	16.554	290077	14.738 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062921\
Data File : FB025959.D
Signal(s) : FID2B.CH
Acq On : 29 Jun 2021 23:21
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc : 5.02g/5.00 ml DI WATER
ALS Vial : 23 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 30 01:37:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

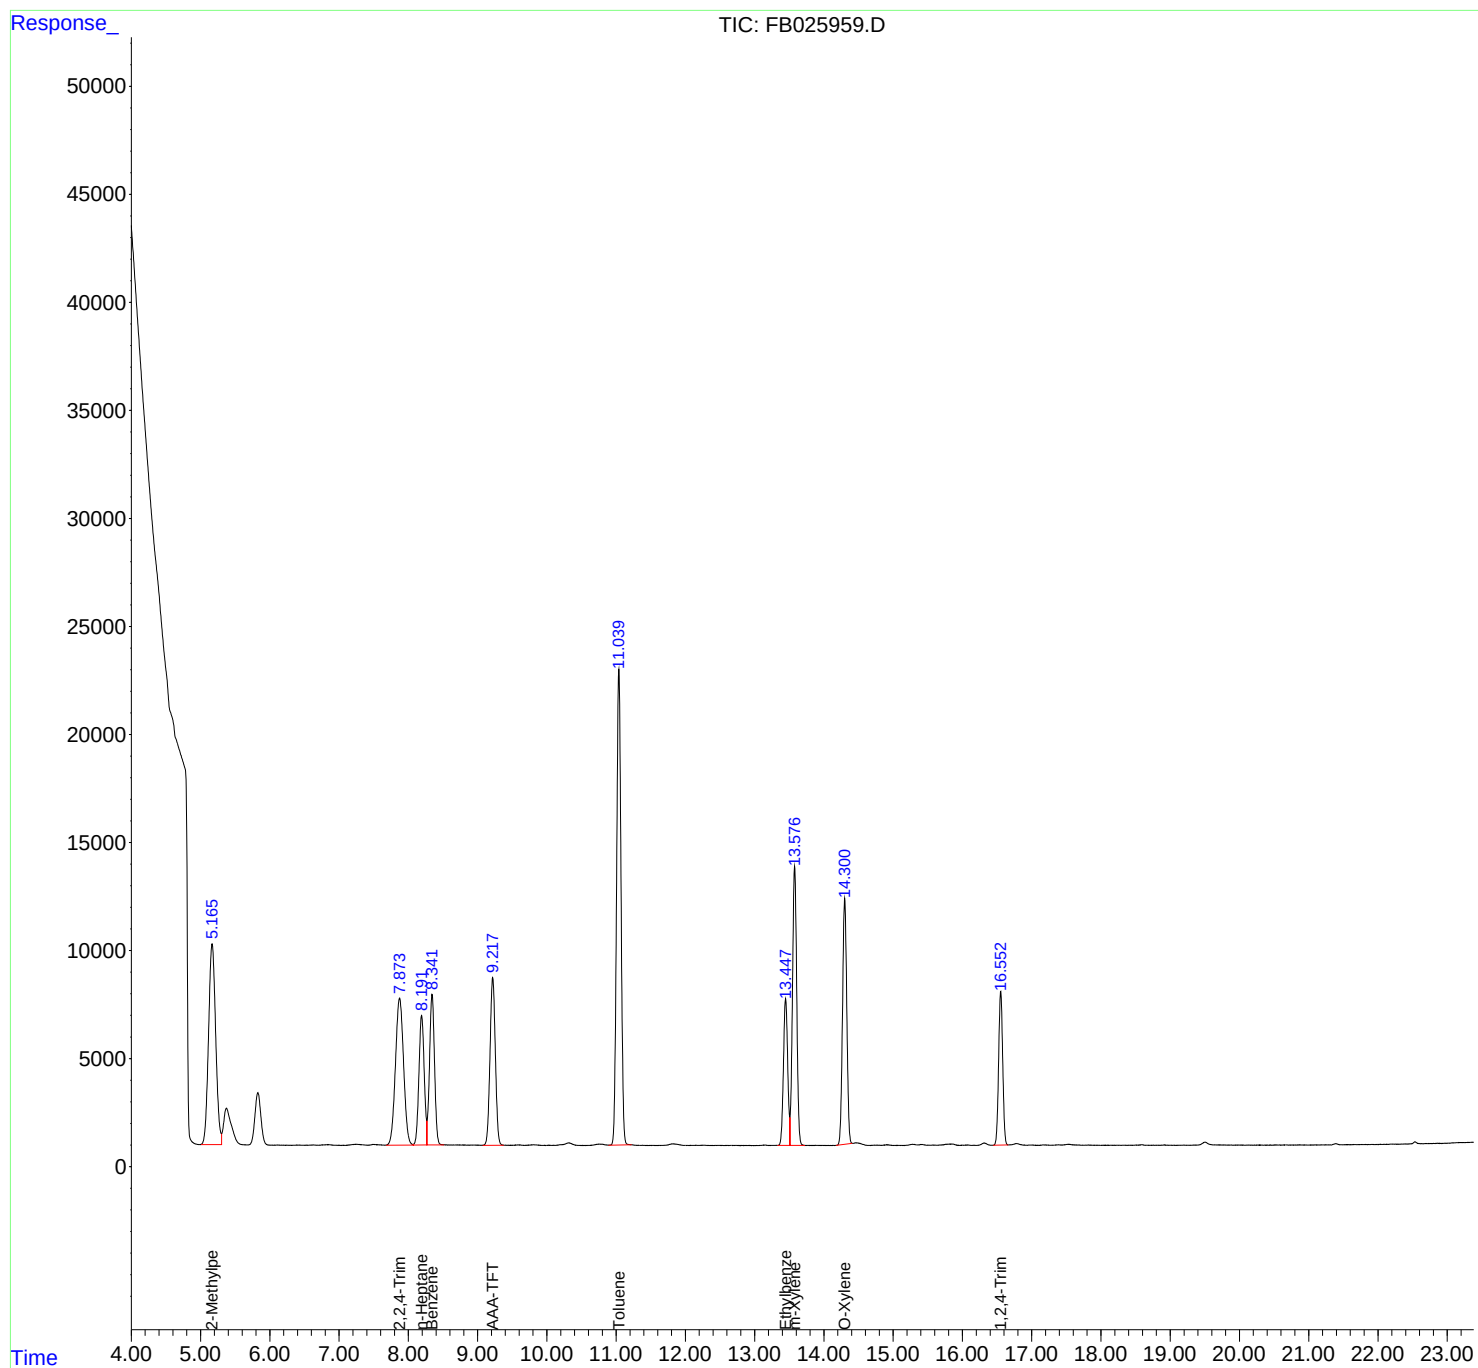

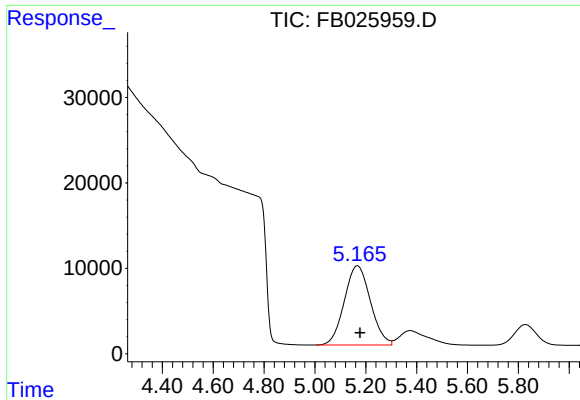


#1 2-Methylpentane

R.T.: 5.167 min
Delta R.T.: -0.010 min
Response: 662513
Conc: 25.17 ng/ml

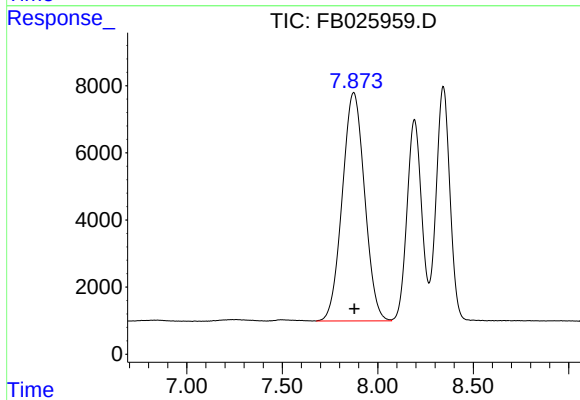


#2 2,2,4-Trimethylpentane

R.T.: 7.874 min
Delta R.T.: -0.004 min
Response: 553164
Conc: 27.46 ng/ml

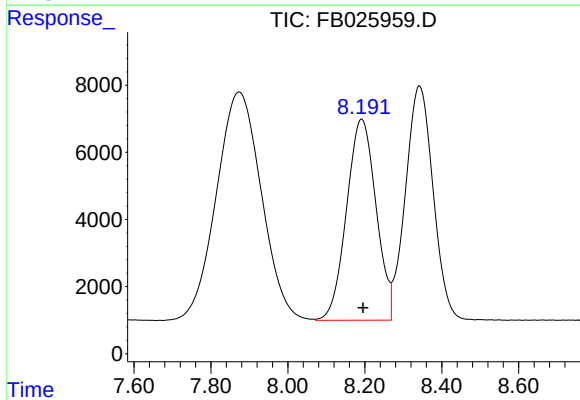


#3 n-Heptane

R.T.: 8.192 min
Delta R.T.: -0.004 min
Response: 317886
Conc: 8.84 ng/ml

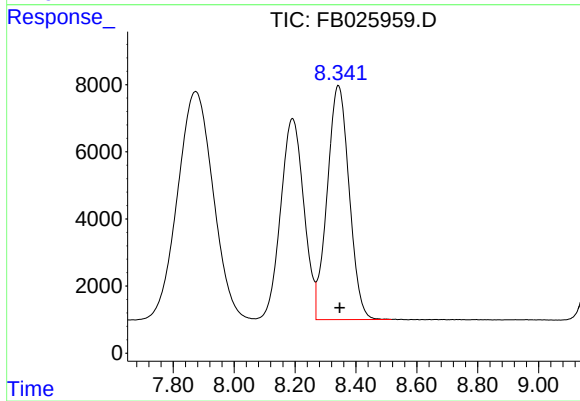


#4 Benzene

R.T.: 8.343 min
Delta R.T.: -0.004 min
Response: 349156
Conc: 8.36 ng/ml

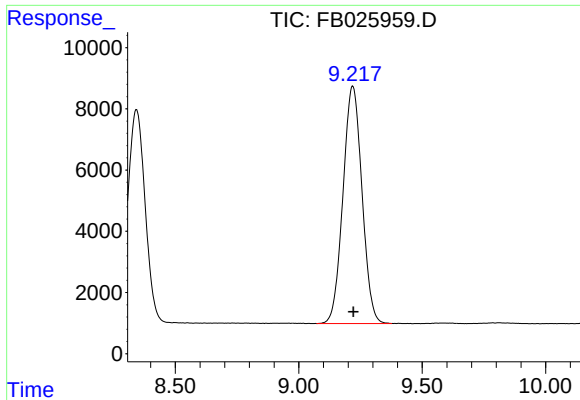


#5 AAA-TFT

R.T.: 9.219 min
Delta R.T.: -0.002 min
Response: 415118
Conc: 17.18 ng/ml

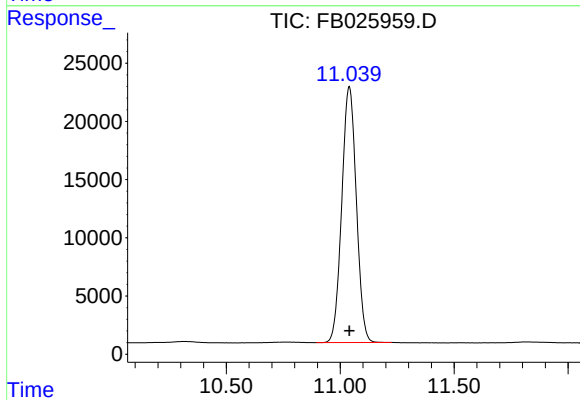


#6 Toluene

R.T.: 11.040 min
Delta R.T.: -0.001 min
Response: 976235
Conc: 23.72 ng/ml

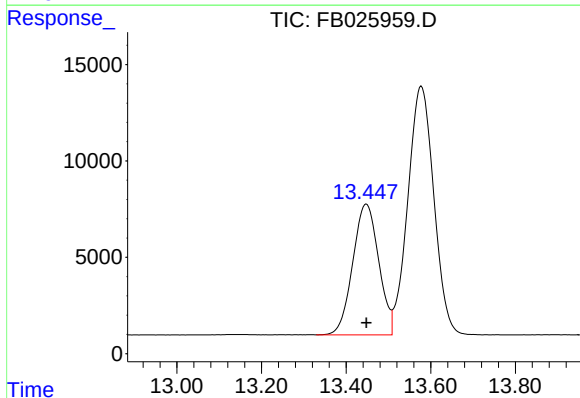


#7 Ethylbenzene

R.T.: 13.448 min
Delta R.T.: 0.000 min
Response: 288300
Conc: 7.56 ng/ml

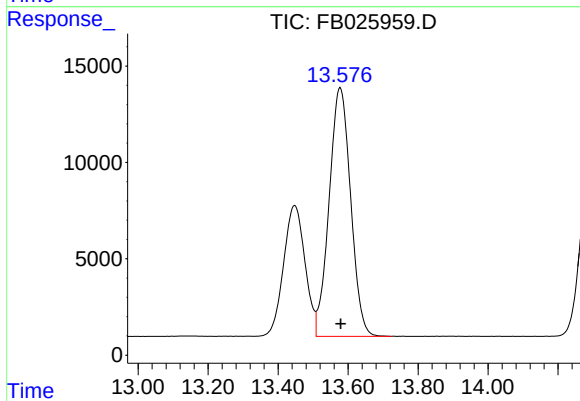


#8 m-Xylene

R.T.: 13.578 min
Delta R.T.: 0.000 min
Response: 550979
Conc: 14.02 ng/ml

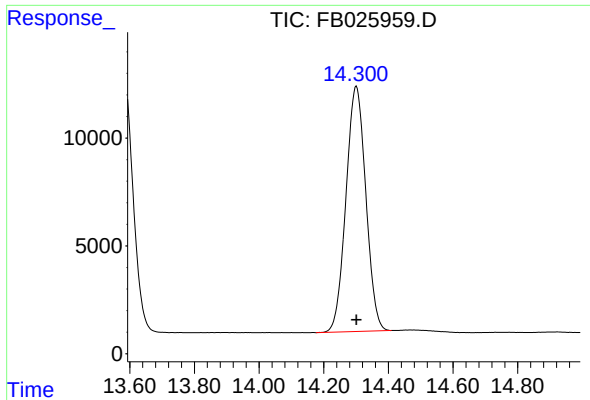

#9 O-Xylene

R.T.: 14.301 min
Delta R.T.: 0.000 min
Response: 484395
Conc: 15.19 ng/ml

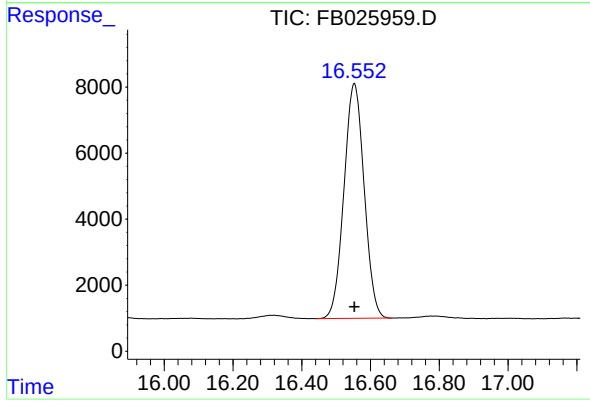

#10 1,2,4-Trimethylbenzene

R.T.: 16.554 min
Delta R.T.: 0.000 min
Response: 290077
Conc: 14.74 ng/ml