

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063020\
 Data File : FB024516.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jun 2020 11:42
 Operator : DD/AJ
 Sample : BSF0630S1
 Misc : 5.00gm/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 01 01:16:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	505350	20.887 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	974634	30.492 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	1065552	31.785 ng/ml
3) t n-Heptane	7.757	351585	10.397 ng/ml
4) t Benzene	7.891	415094	10.268 ng/ml
6) t Toluene	10.630	1183703	30.121 ng/ml
7) t Ethylbenzene	13.070	371705	10.593 ng/ml
8) t m-Xylene	13.203	724774	21.164 ng/ml
9) t O-Xylene	13.931	711209	21.213 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	598481	21.555 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063020\
Data File : FB024516.D
Signal(s) : FID2B.CH
Acq On : 30 Jun 2020 11:42
Operator : DD/AJ
Sample : BSF0630S1
Misc : 5.00gm/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 01 01:16:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

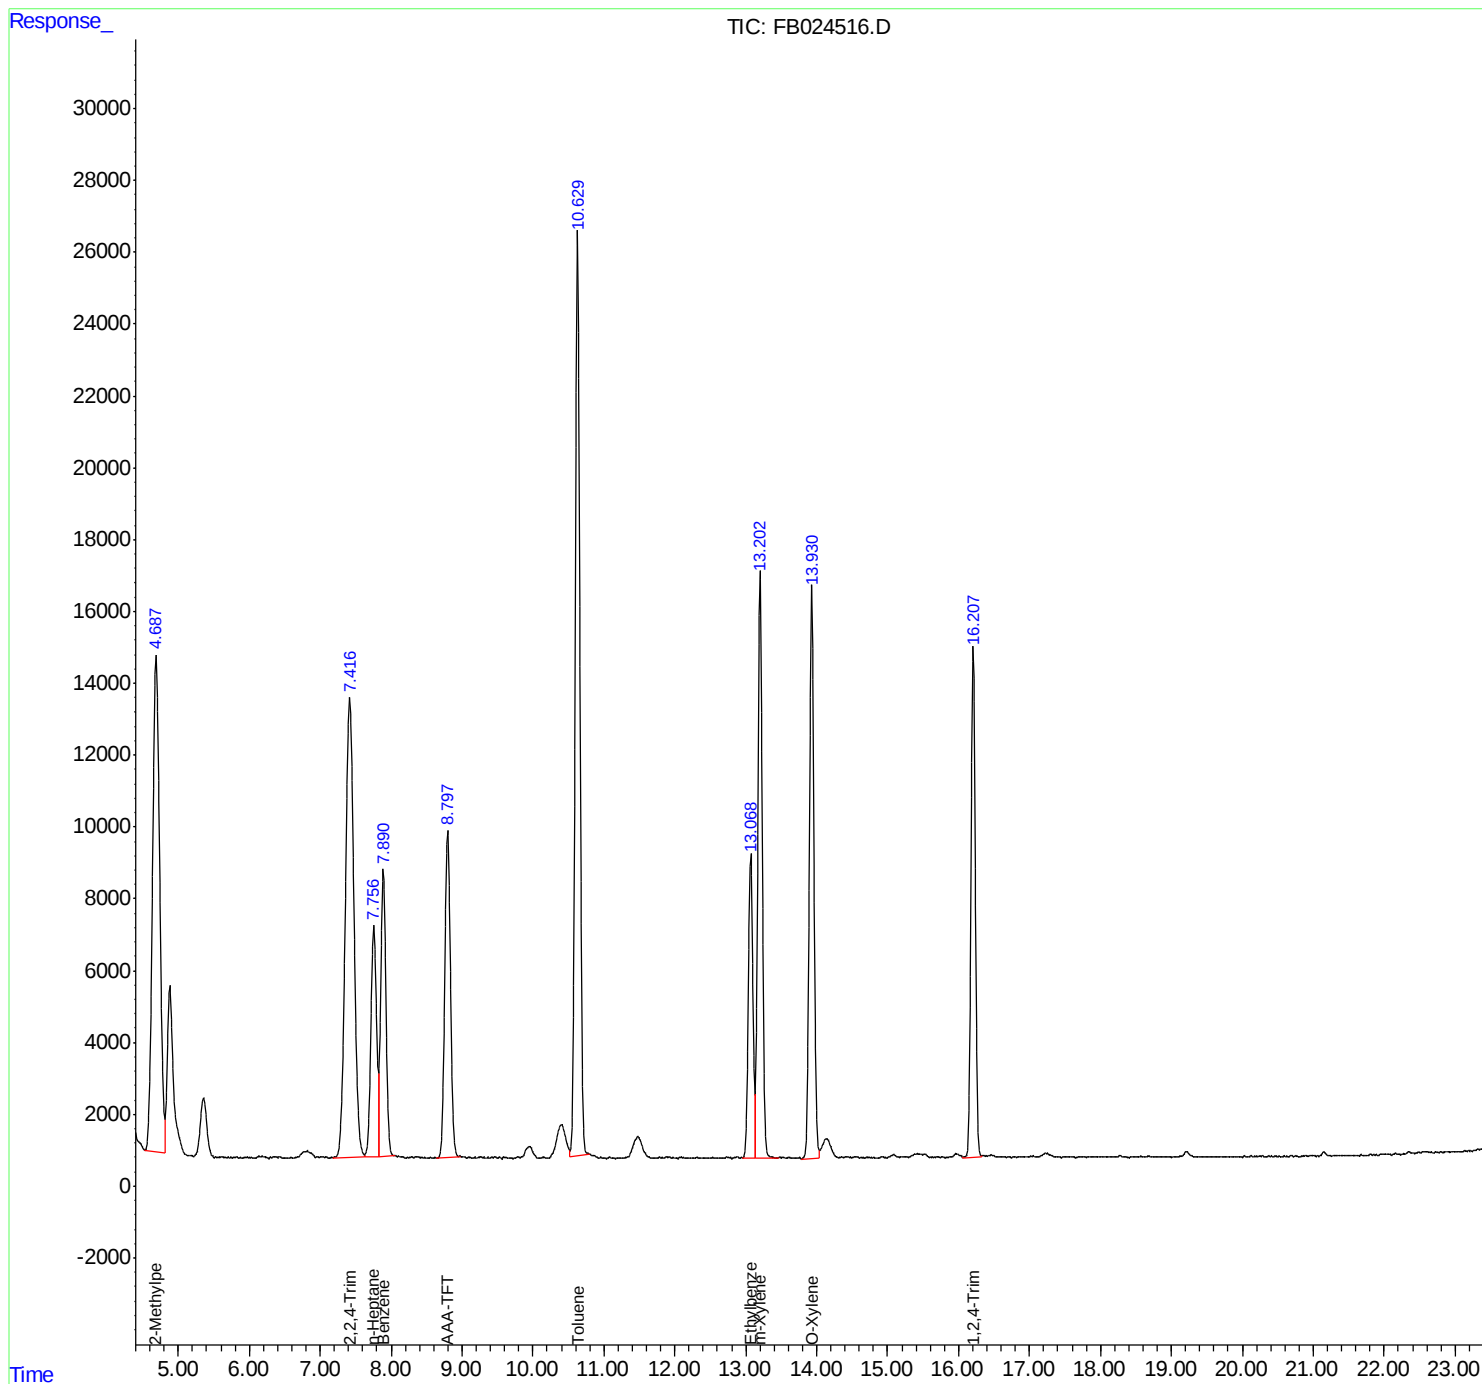

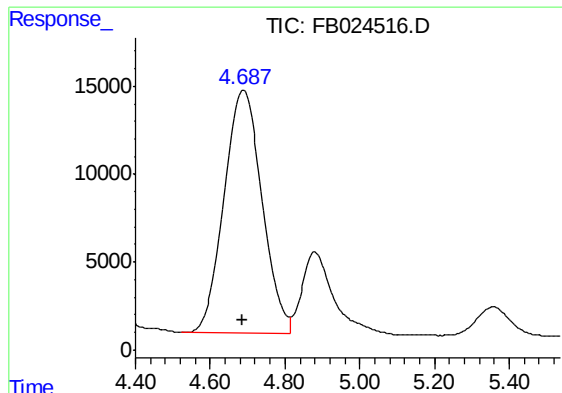


#1 2-Methylpentane

R.T.: 4.688 min
Delta R.T.: 0.001 min
Response: 974634
Conc: 30.49 ng/ml

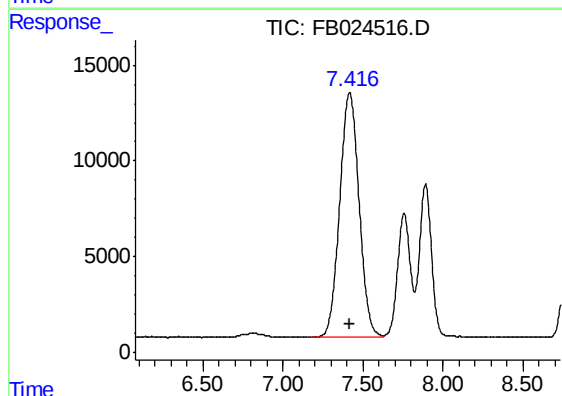


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.001 min
Response: 1065552
Conc: 31.78 ng/ml

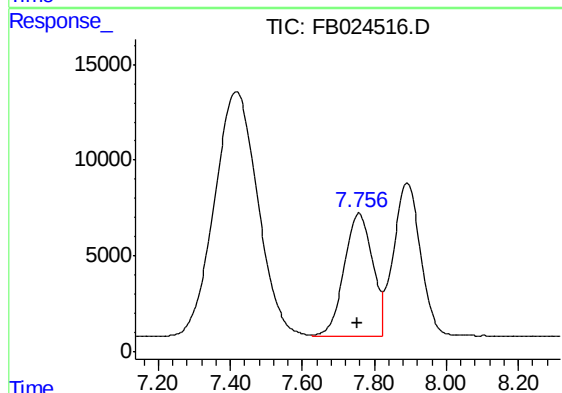


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.002 min
Response: 351585
Conc: 10.40 ng/ml

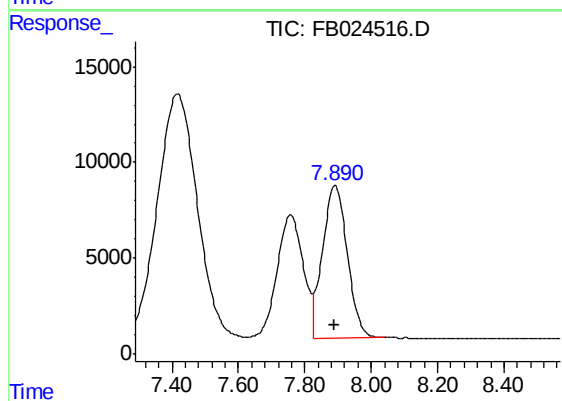


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.001 min
Response: 415094
Conc: 10.27 ng/ml

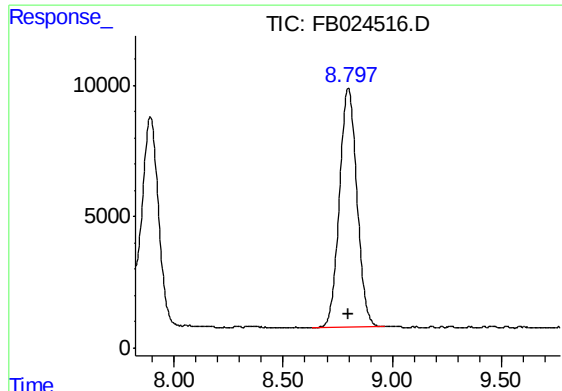


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.002 min
Response: 505350
Conc: 20.89 ng/ml

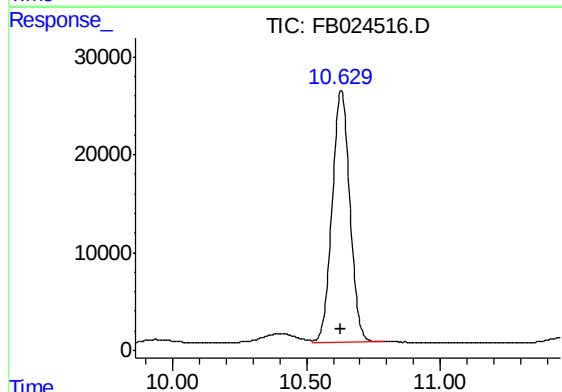


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.002 min
Response: 1183703
Conc: 30.12 ng/ml

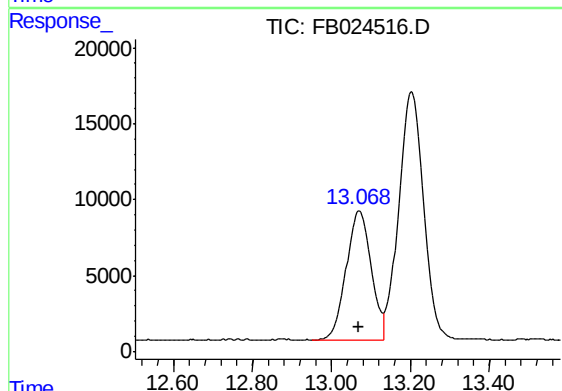


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.002 min
Response: 371705
Conc: 10.59 ng/ml

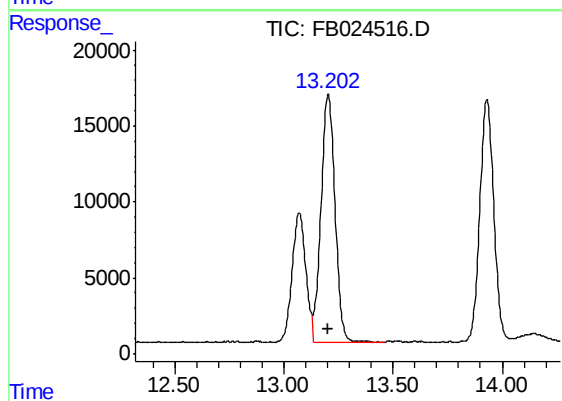


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.002 min
Response: 724774
Conc: 21.16 ng/ml

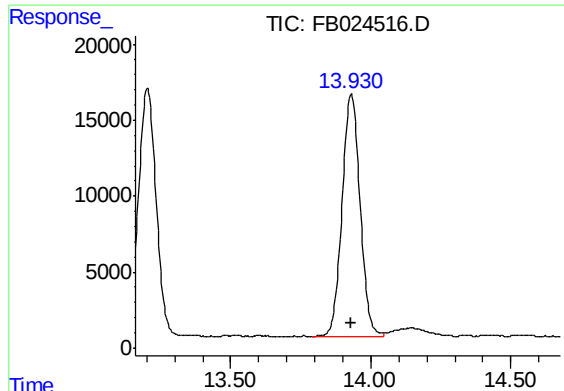

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.002 min
Response: 711209
Conc: 21.21 ng/ml

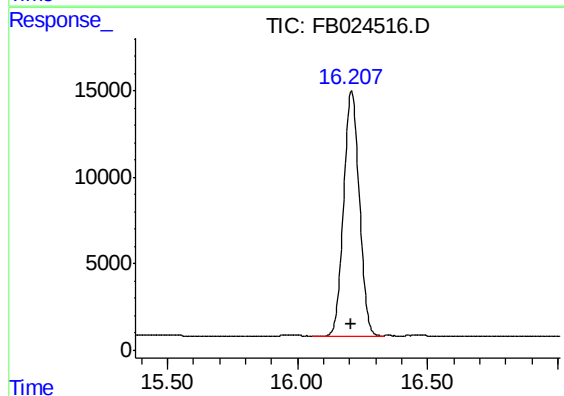

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.001 min
Response: 598481
Conc: 21.55 ng/ml