

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063020\
 Data File : FB024519.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jun 2020 13:14
 Operator : DD/AJ
 Sample : L2815-17MSD
 Misc : 5.01gm/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 01 01:16:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	507939	20.994 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	779557	24.389 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	721623	21.526 ng/ml
3) t n-Heptane	7.759	130253	3.852 ng/ml
4) t Benzene	7.892	397779	9.840 ng/ml
6) t Toluene	10.630	1083084	27.561 ng/ml
7) t Ethylbenzene	13.071	297355	8.474 ng/ml
8) t m-Xylene	13.204	447814	13.076 ng/ml
9) t O-Xylene	13.931	549811	16.399 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	169981	6.122 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063020\
Data File : FB024519.D
Signal(s) : FID2B.CH
Acq On : 30 Jun 2020 13:14
Operator : DD/AJ
Sample : L2815-17MSD
Misc : 5.01gm/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 01 01:16:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

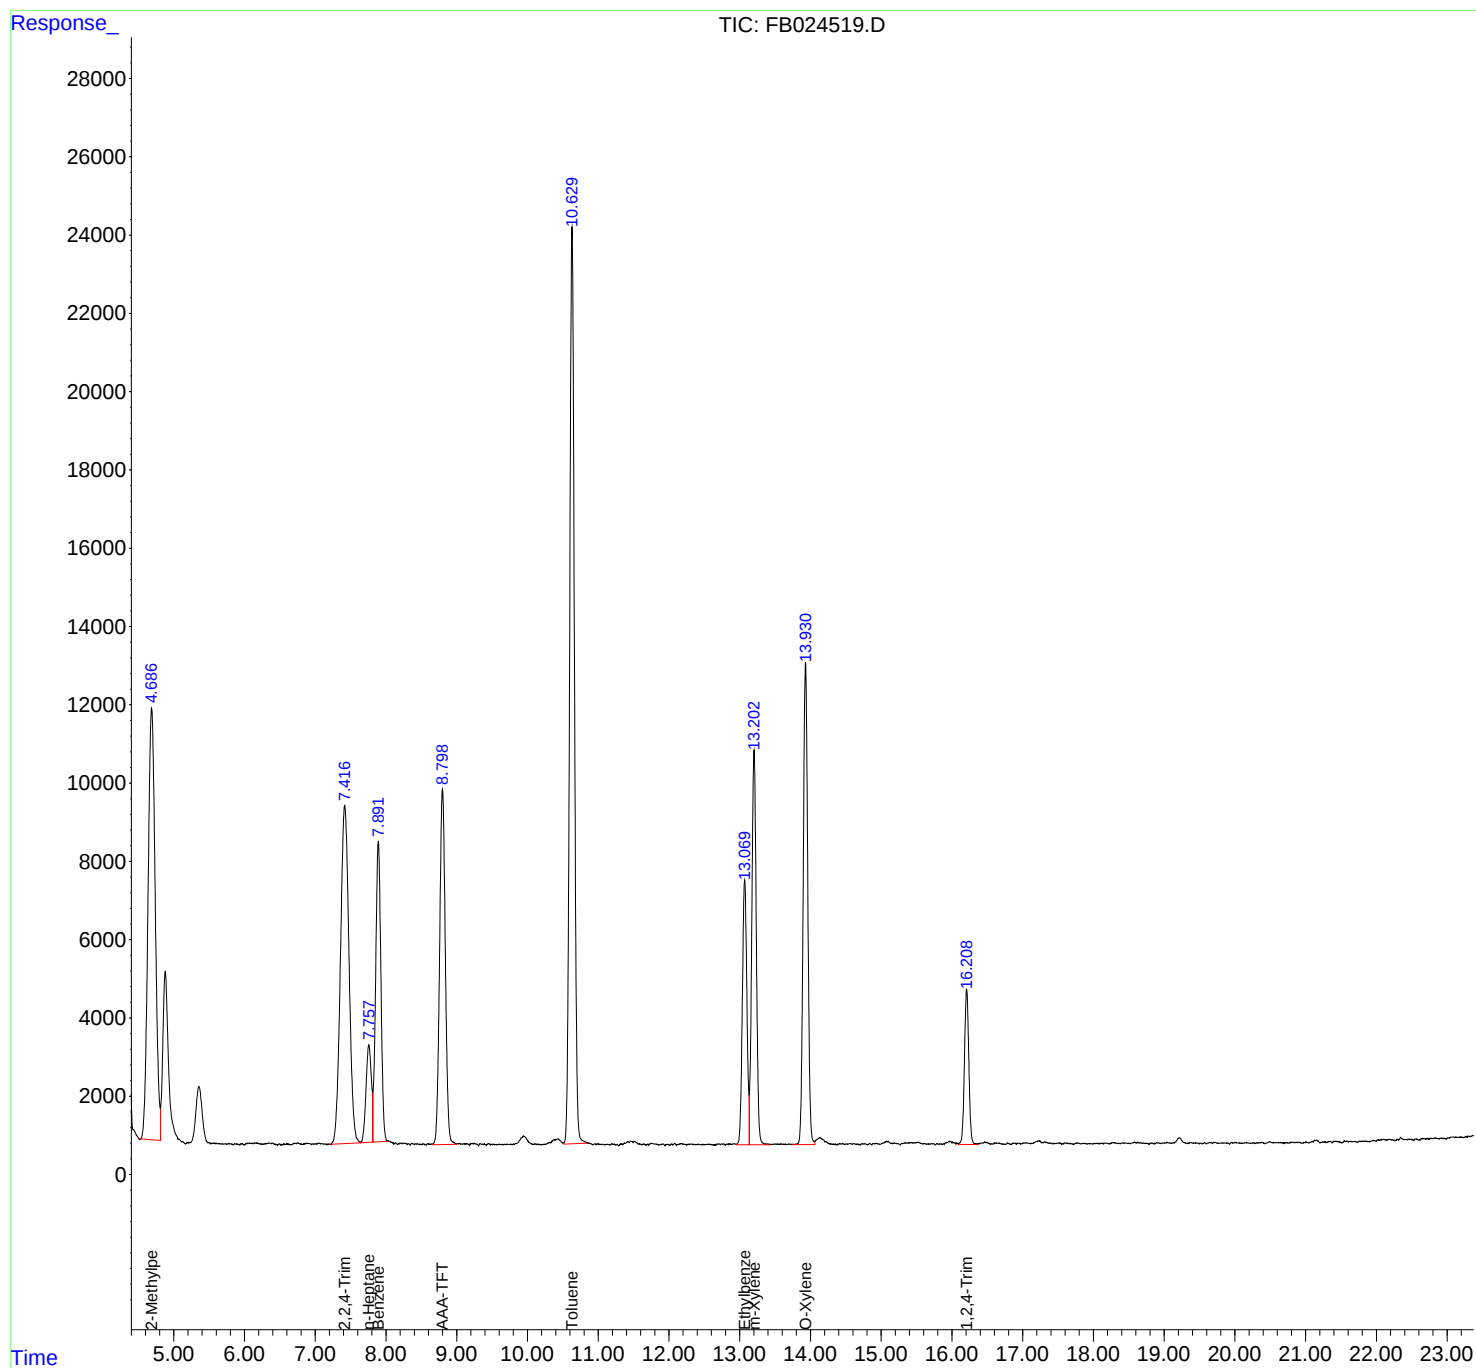

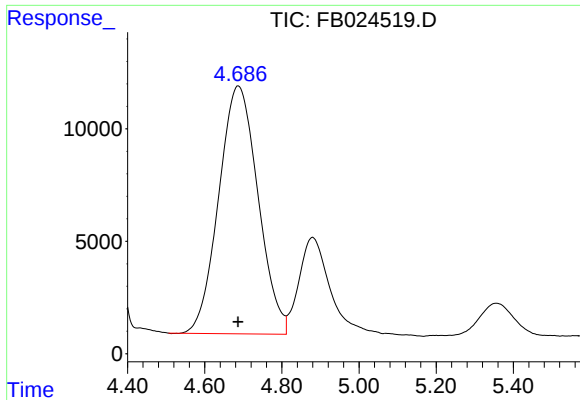


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 779557
Conc: 24.39 ng/ml

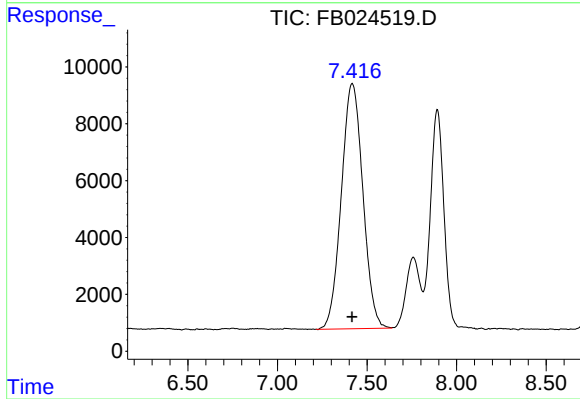


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.002 min
Response: 721623
Conc: 21.53 ng/ml

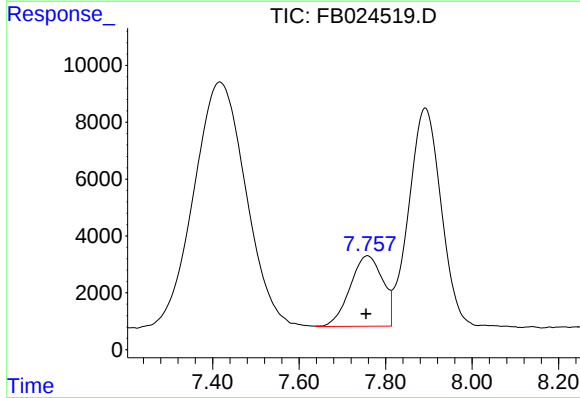


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.004 min
Response: 130253
Conc: 3.85 ng/ml

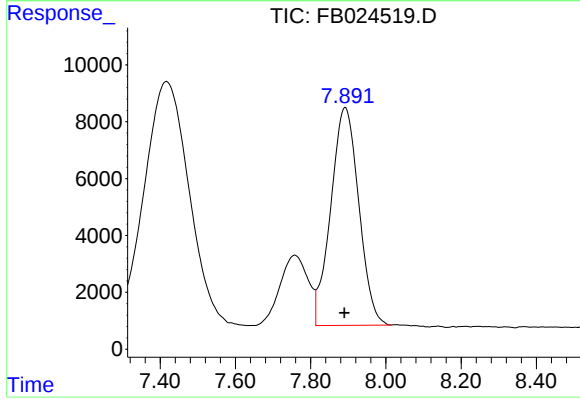


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.002 min
Response: 397779
Conc: 9.84 ng/ml

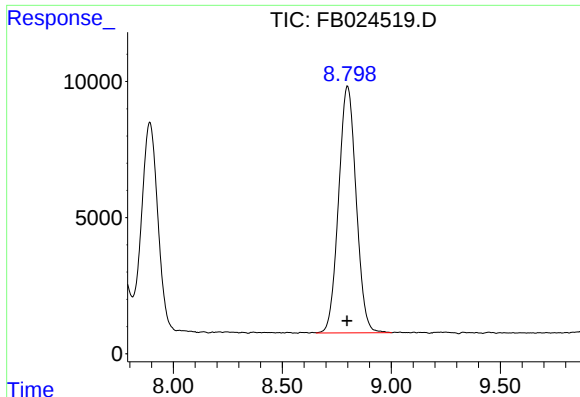


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: 0.002 min
Response: 507939
Conc: 20.99 ng/ml

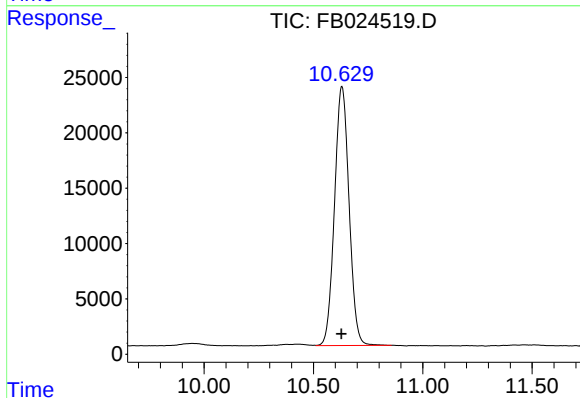


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.002 min
Response: 1083084
Conc: 27.56 ng/ml

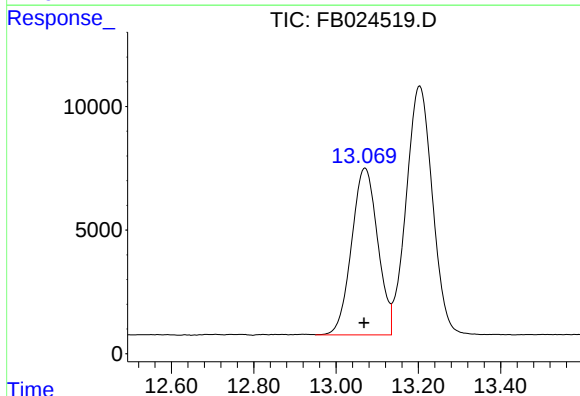


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.003 min
Response: 297355
Conc: 8.47 ng/ml

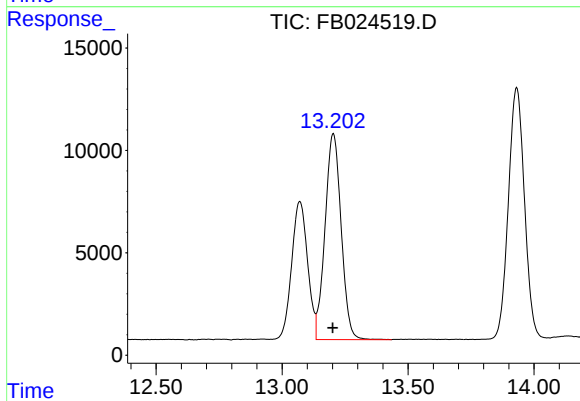


#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: 0.002 min
Response: 447814
Conc: 13.08 ng/ml

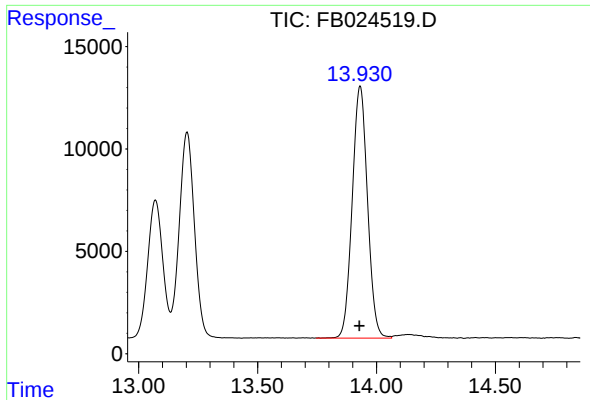

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.003 min
Response: 549811
Conc: 16.40 ng/ml

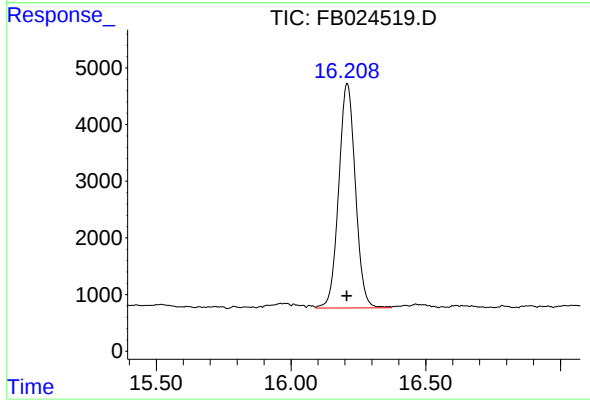

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.002 min
Response: 169981
Conc: 6.12 ng/ml