

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063021\
 Data File : FB025969.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jun 2021 18:35
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc : 5.02g/5.00 ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 01 08:51:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
 Quant Title :
 QLast Update : Wed Jun 09 13:39:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.227	490185	20.283 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.179	718461	27.300 ng/ml
2) t 2,2,4-Trimethylpentane	7.883	617218	30.639 ng/ml
3) t n-Heptane	8.201	356760	9.925 ng/ml
4) t Benzene	8.352	391723	9.384 ng/ml
6) t Toluene	11.047	1095021	26.610 ng/ml
7) t Ethylbenzene	13.455	320629	8.413 ng/ml
8) t m-Xylene	13.585	608596	15.481 ng/ml
9) t O-Xylene	14.308	524326	16.444 ng/ml
10) t 1,2,4-Trimethylbenzene	16.561	319346	16.225 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063021\
Data File : FB025969.D
Signal(s) : FID2B.CH
Acq On : 30 Jun 2021 18:35
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc : 5.02g/5.00 ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 01 08:51:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

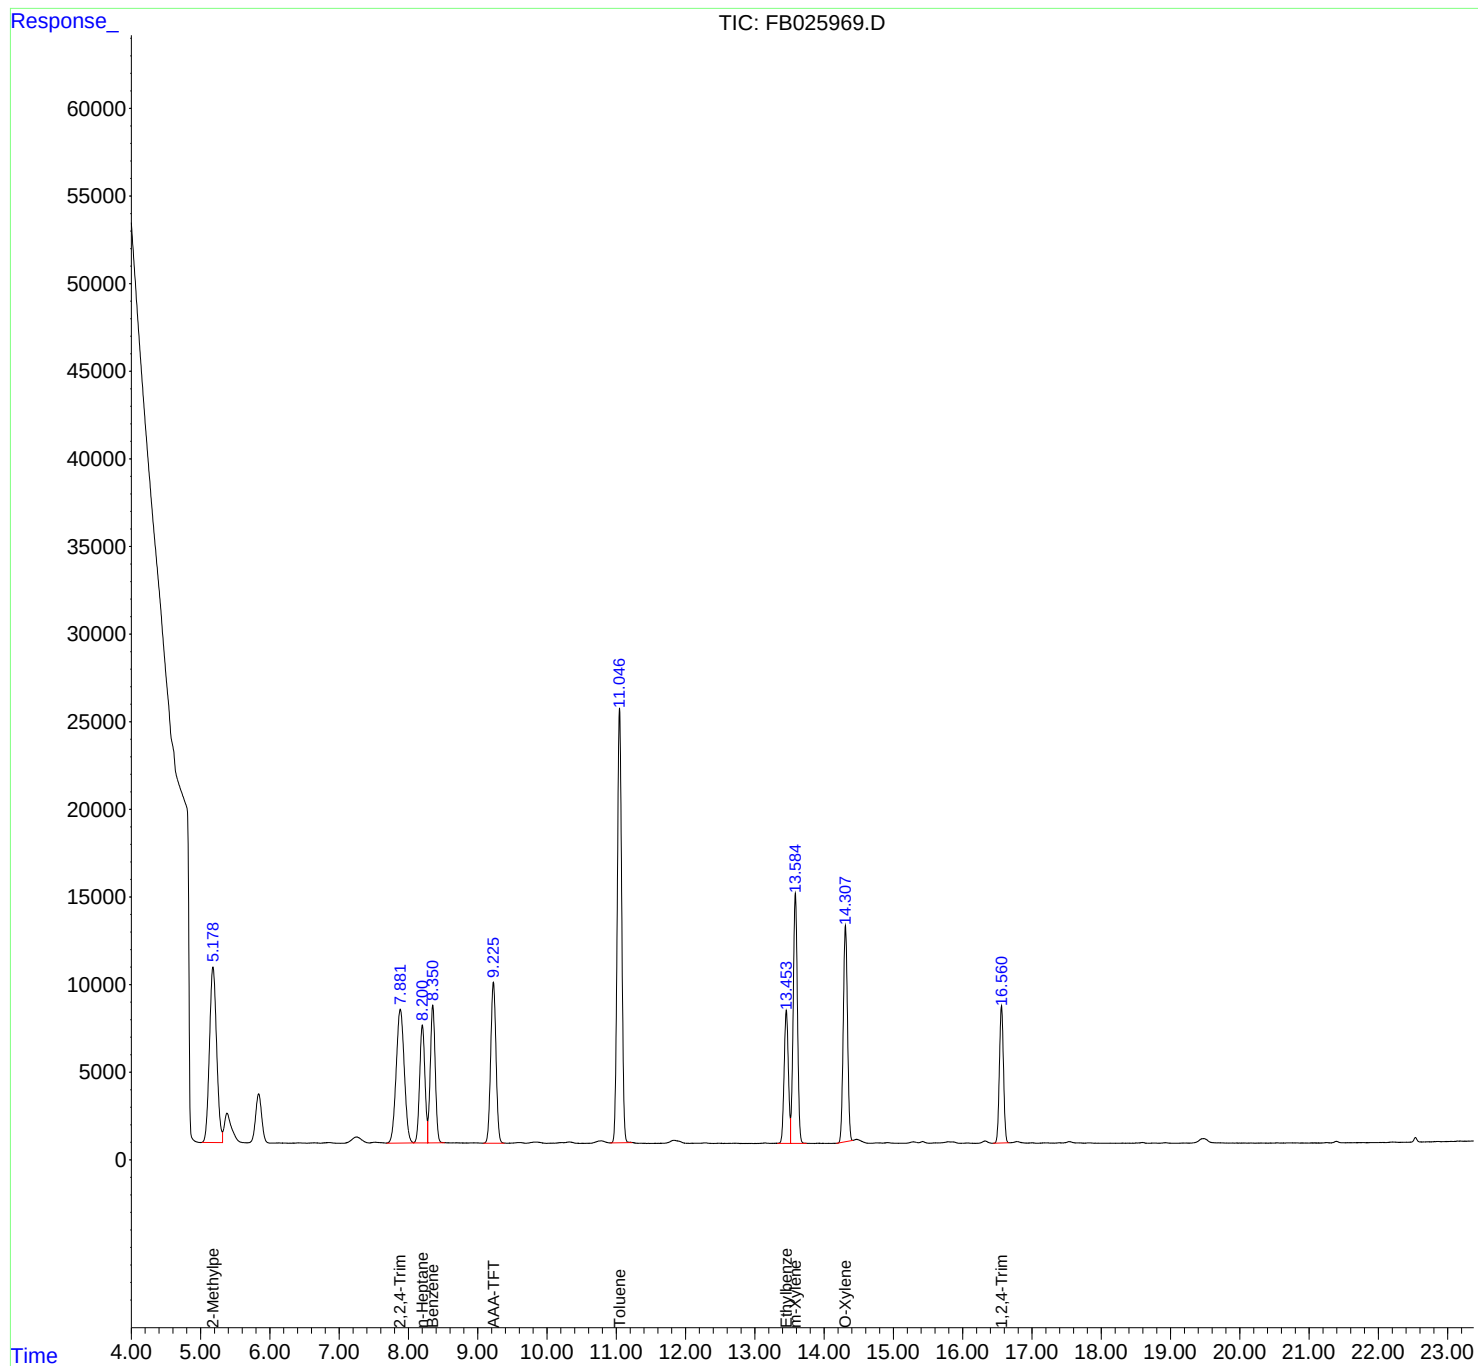

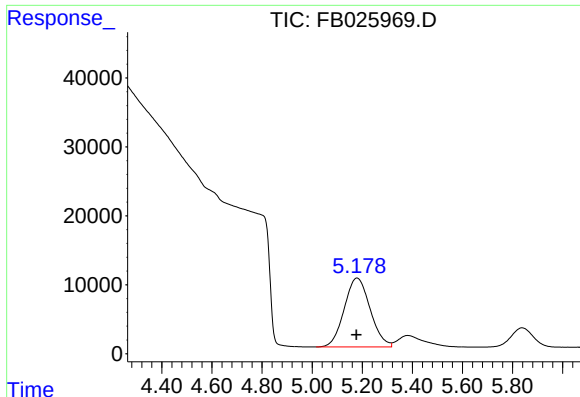


#1 2-Methylpentane

R.T.: 5.179 min
Delta R.T.: 0.002 min
Response: 718461
Conc: 27.30 ng/ml

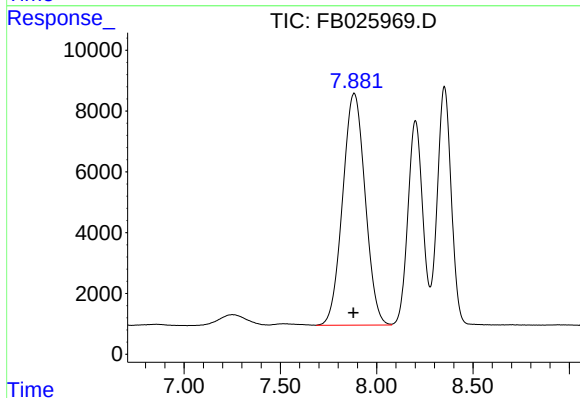


#2 2,2,4-Trimethylpentane

R.T.: 7.883 min
Delta R.T.: 0.005 min
Response: 617218
Conc: 30.64 ng/ml

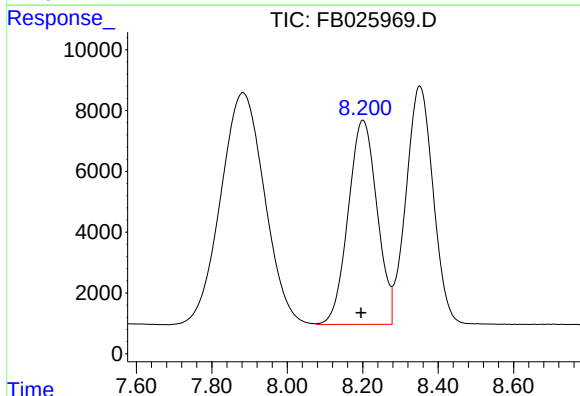


#3 n-Heptane

R.T.: 8.201 min
Delta R.T.: 0.005 min
Response: 356760
Conc: 9.92 ng/ml

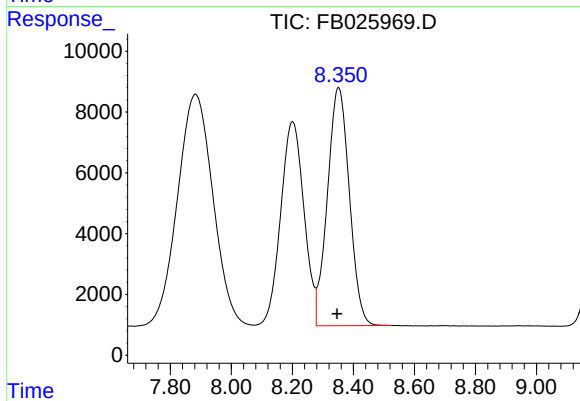


#4 Benzene

R.T.: 8.352 min
Delta R.T.: 0.005 min
Response: 391723
Conc: 9.38 ng/ml

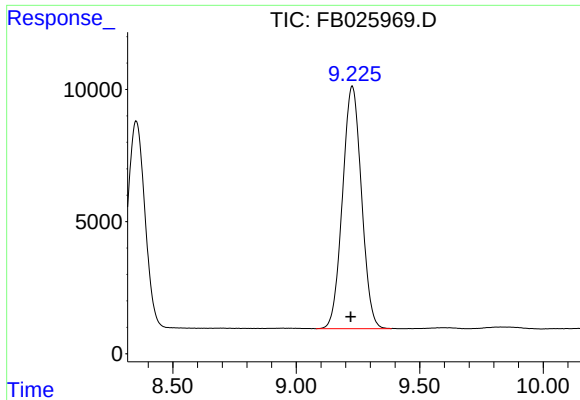


#5 AAA-TFT

R.T.: 9.227 min
Delta R.T.: 0.006 min
Response: 490185
Conc: 20.28 ng/ml

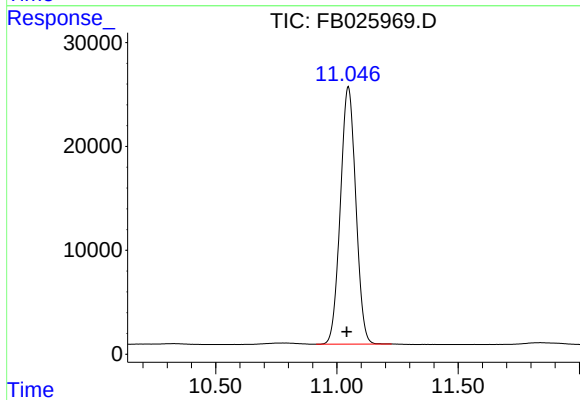


#6 Toluene

R.T.: 11.047 min
Delta R.T.: 0.006 min
Response: 1095021
Conc: 26.61 ng/ml

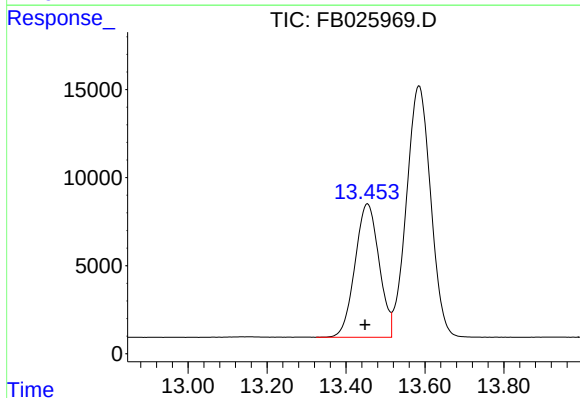


#7 Ethylbenzene

R.T.: 13.455 min
Delta R.T.: 0.007 min
Response: 320629
Conc: 8.41 ng/ml

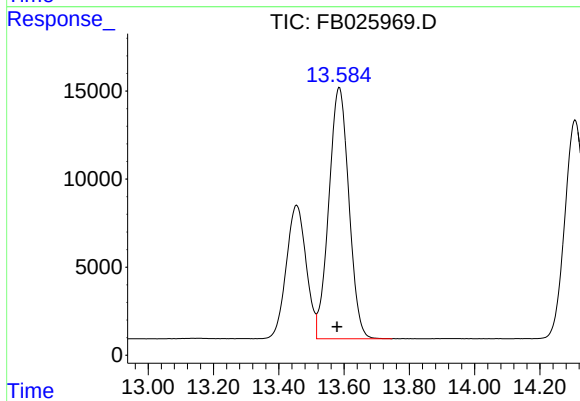


#8 m-Xylene

R.T.: 13.585 min
Delta R.T.: 0.007 min
Response: 608596
Conc: 15.48 ng/ml

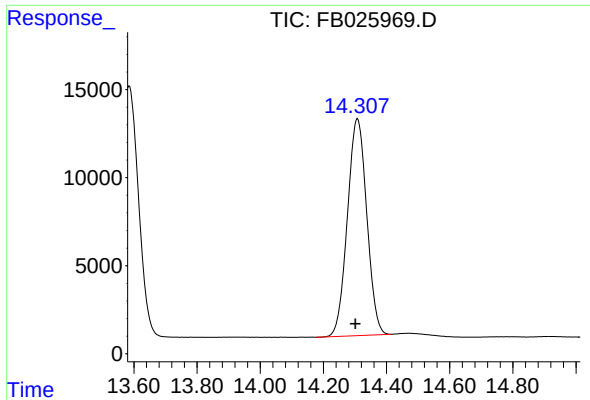

#9 O-Xylene

R.T.: 14.308 min
Delta R.T.: 0.007 min
Response: 524326
Conc: 16.44 ng/ml

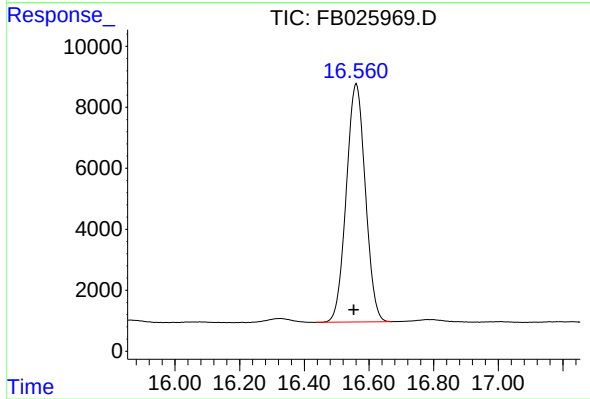

#10 1,2,4-Trimethylbenzene

R.T.: 16.561 min
Delta R.T.: 0.007 min
Response: 319346
Conc: 16.22 ng/ml