

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063022\
 Data File : FB027576.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jun 2022 14:51
 Operator : AJ/MA
 Sample : N3214-07
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 01 04:32:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	231620	20.650 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.718	126465	7.507 ng/ml
2) t 2,2,4-Trimethylpentane	7.431	119082	6.782 ng/ml
3) t n-Heptane	7.755	37855	2.161 ng/ml
4) t Benzene	7.890	43701	2.143 ng/ml
6) t Toluene	10.623	125505	6.482 ng/ml
7) t Ethylbenzene	13.060	42114	2.326 ng/ml
8) t m-Xylene	13.193	82310	4.617 ng/ml
9) t O-Xylene	13.920	80065	4.608 ng/ml
10) t 1,2,4-Trimethylbenzene	16.195	84209	4.902 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063022\
Data File : FB027576.D
Signal(s) : FID2B.CH
Acq On : 30 Jun 2022 14:51
Operator : AJ/MA
Sample : N3214-07
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 01 04:32:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

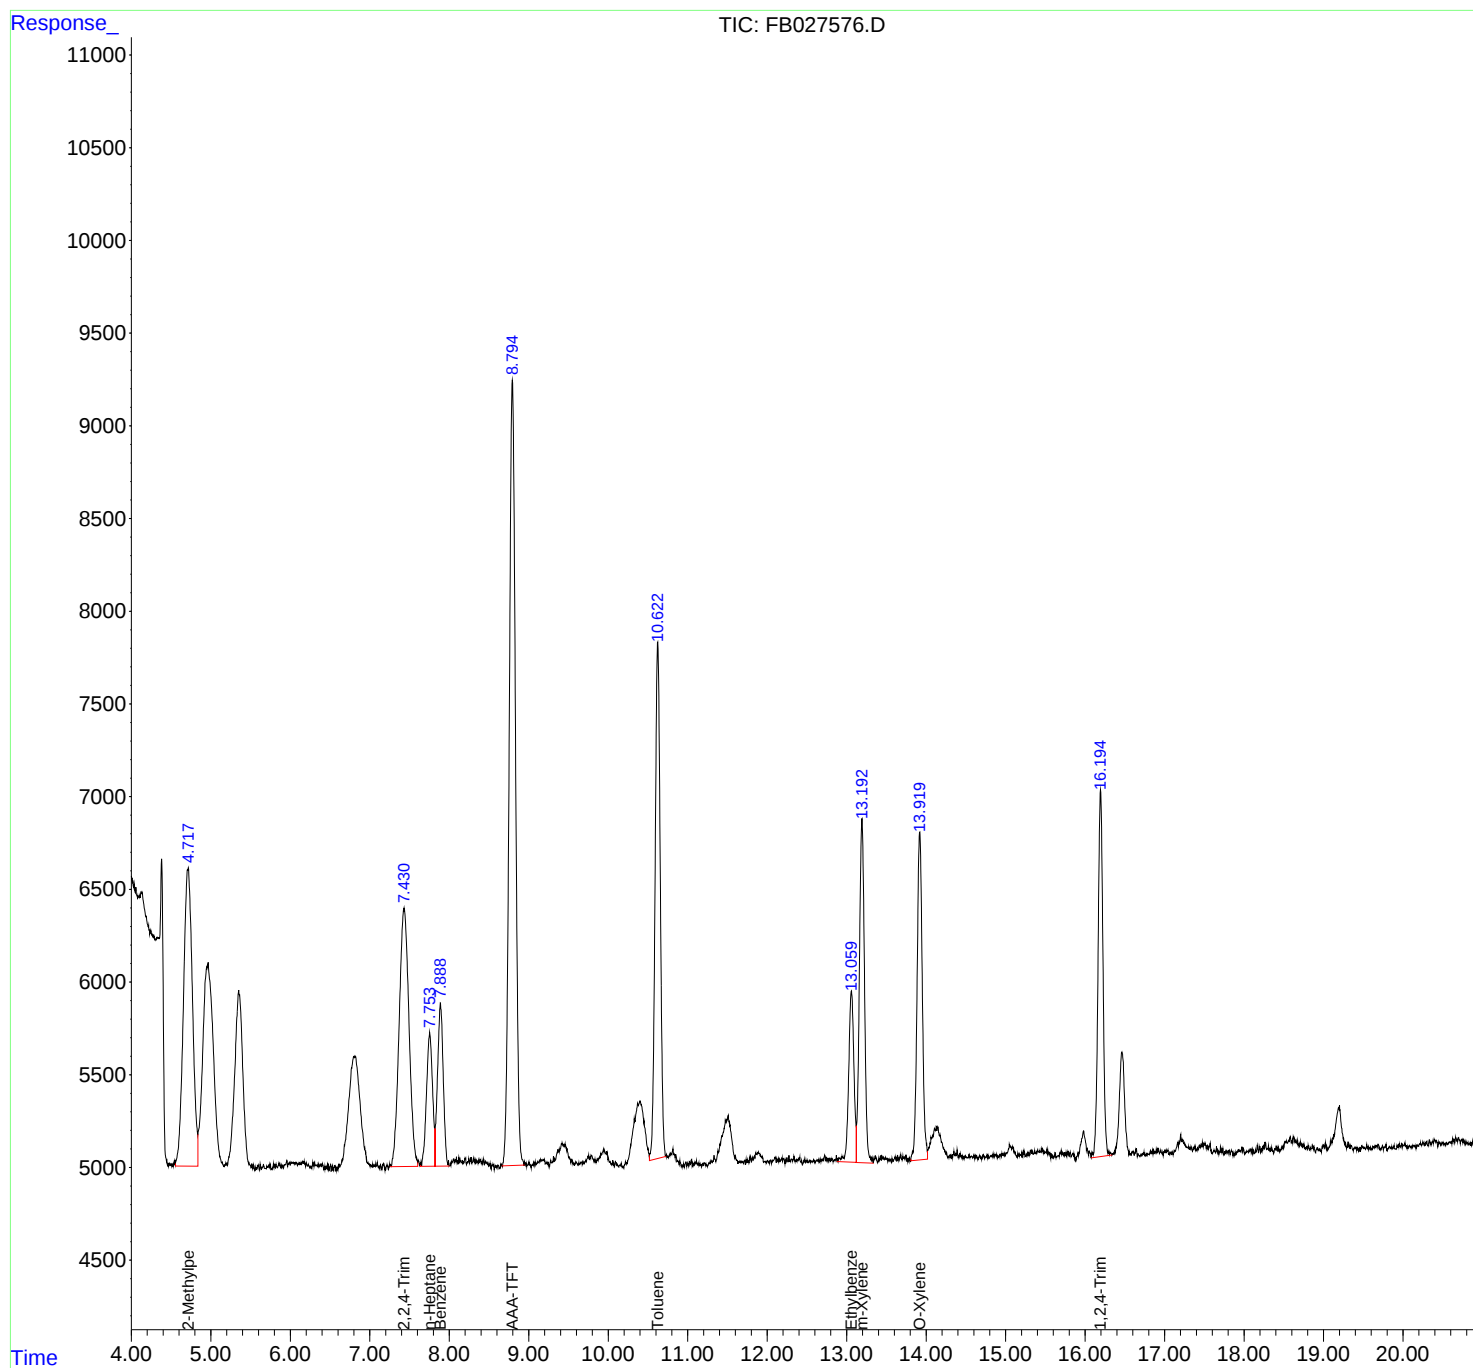

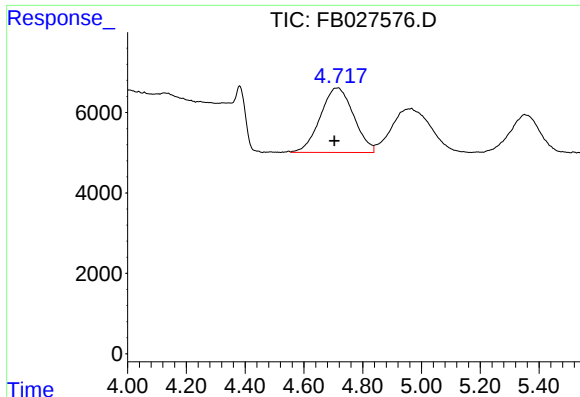


#1 2-Methylpentane

R.T.: 4.718 min
Delta R.T.: 0.014 min
Response: 126465
Conc: 7.51 ng/ml

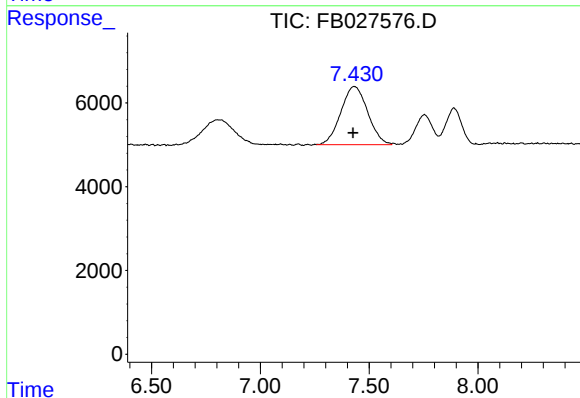


#2 2,2,4-Trimethylpentane

R.T.: 7.431 min
Delta R.T.: 0.005 min
Response: 119082
Conc: 6.78 ng/ml

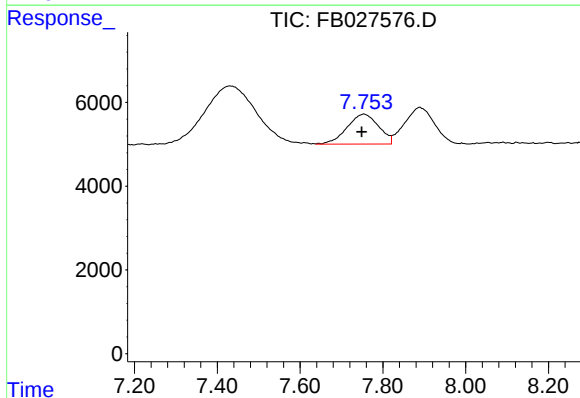


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.005 min
Response: 37855
Conc: 2.16 ng/ml

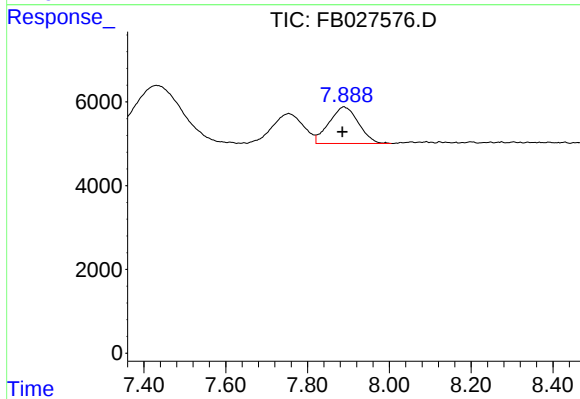


#4 Benzene

R.T.: 7.890 min
Delta R.T.: 0.004 min
Response: 43701
Conc: 2.14 ng/ml

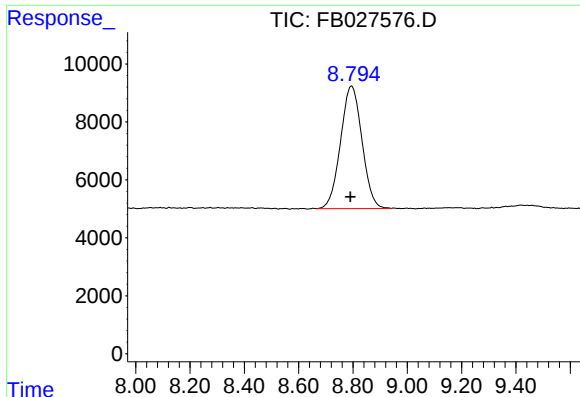


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: 0.004 min
Response: 231620
Conc: 20.65 ng/ml

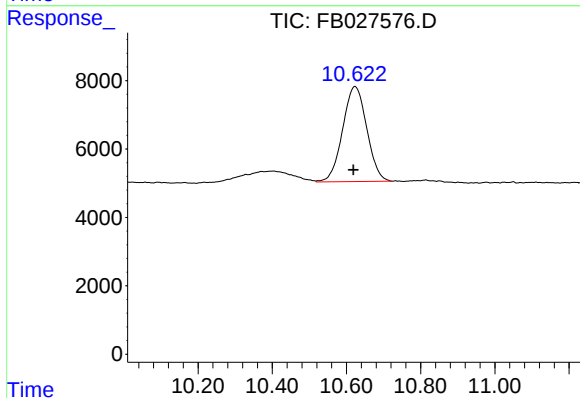


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.004 min
Response: 125505
Conc: 6.48 ng/ml

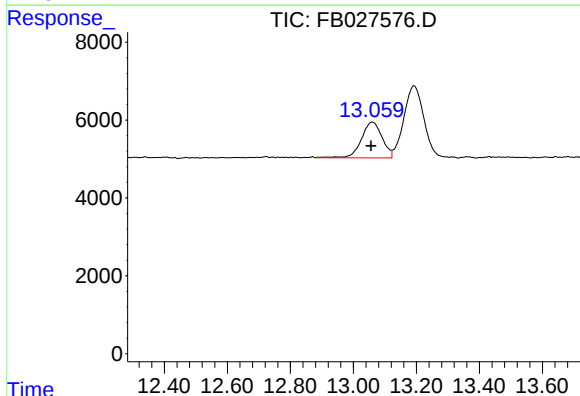


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.004 min
Response: 42114
Conc: 2.33 ng/ml

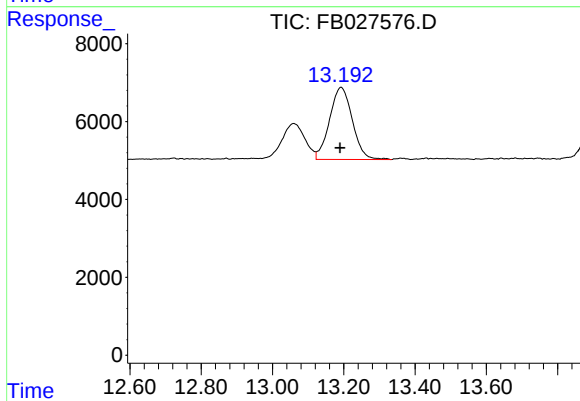


#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: 0.004 min
Response: 82310
Conc: 4.62 ng/ml

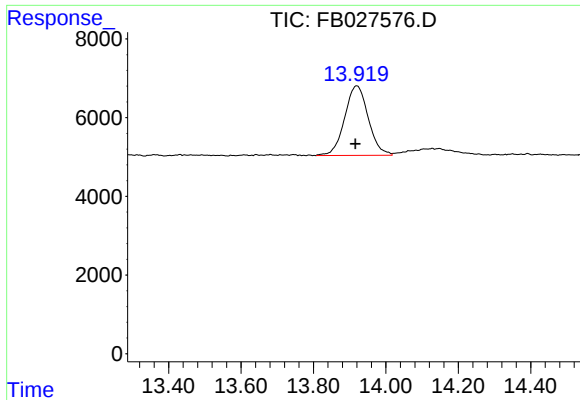

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.004 min
Response: 80065
Conc: 4.61 ng/ml

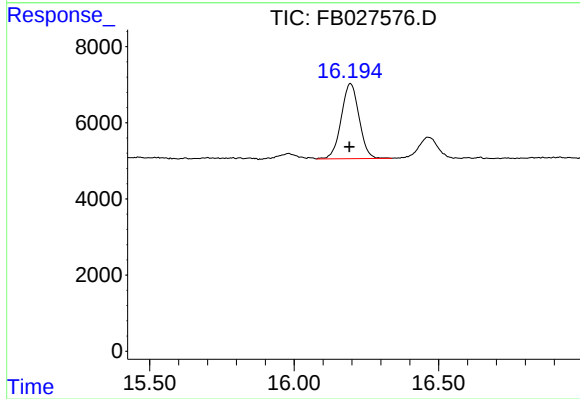

#10 1,2,4-Trimethylbenzene

R.T.: 16.195 min
Delta R.T.: 0.004 min
Response: 84209
Conc: 4.90 ng/ml