

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063022\
 Data File : FB027574.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jun 2022 13:30
 Operator : AJ/MA
 Sample : BSF0630S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 01 04:32:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	233872	20.850 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	518206	30.759 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	535907	30.521 ng/ml
3) t n-Heptane	7.753	182462	10.415 ng/ml
4) t Benzene	7.890	210747	10.335 ng/ml
6) t Toluene	10.624	592182	30.585 ng/ml
7) t Ethylbenzene	13.059	183433	10.129 ng/ml
8) t m-Xylene	13.193	362589	20.340 ng/ml
9) t O-Xylene	13.919	349460	20.112 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	339429	19.759 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063022\
Data File : FB027574.D
Signal(s) : FID2B.CH
Acq On : 30 Jun 2022 13:30
Operator : AJ/MA
Sample : BSF0630S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 01 04:32:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

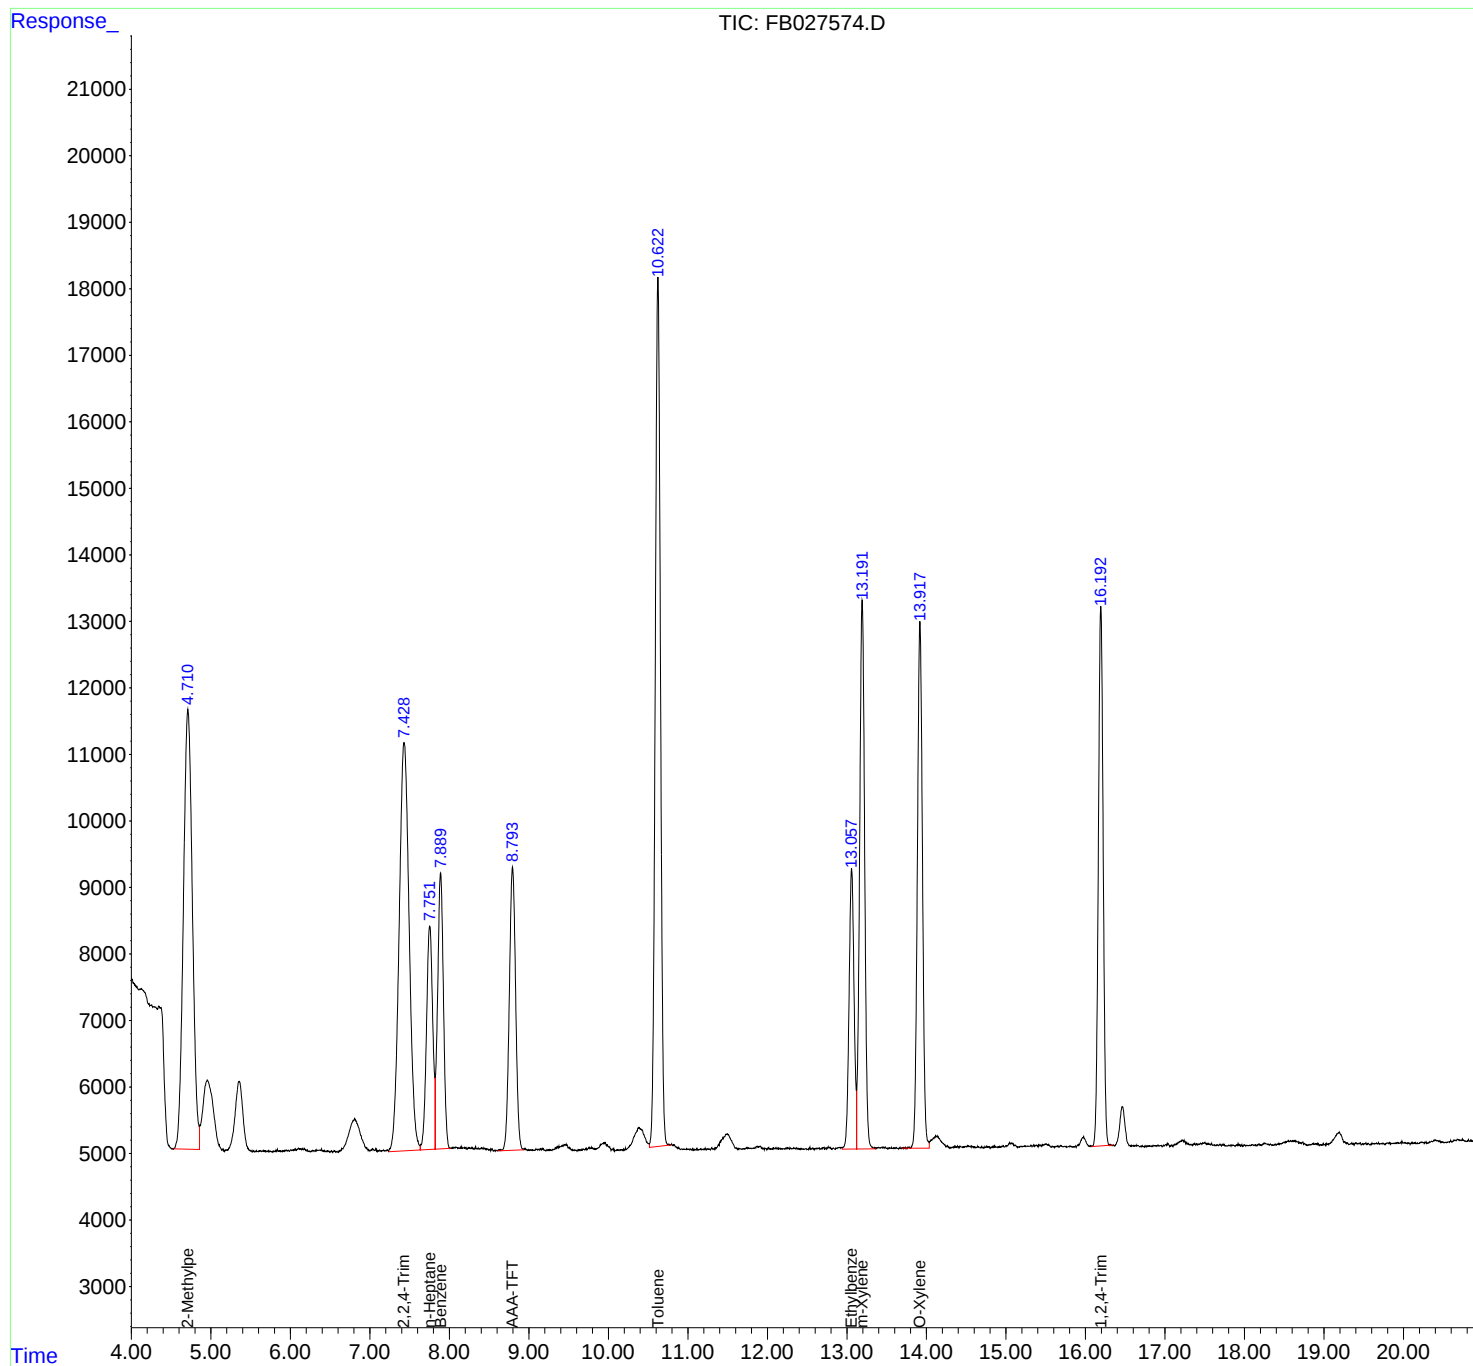

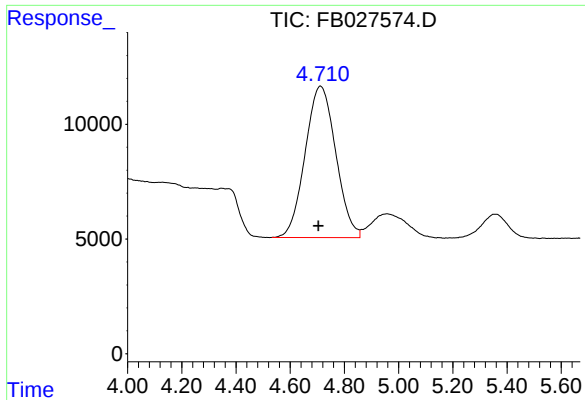


#1 2-Methylpentane

R.T.: 4.712 min
Delta R.T.: 0.008 min
Response: 518206
Conc: 30.76 ng/ml

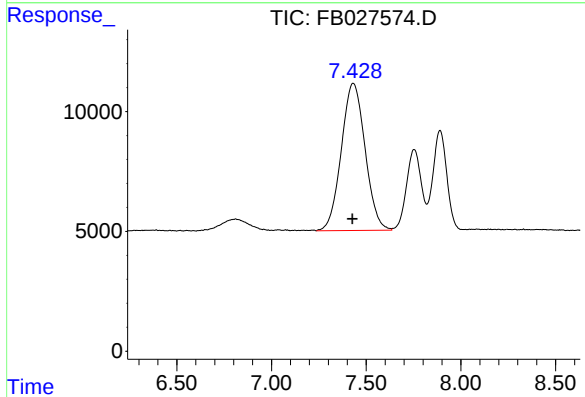


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: 0.004 min
Response: 535907
Conc: 30.52 ng/ml

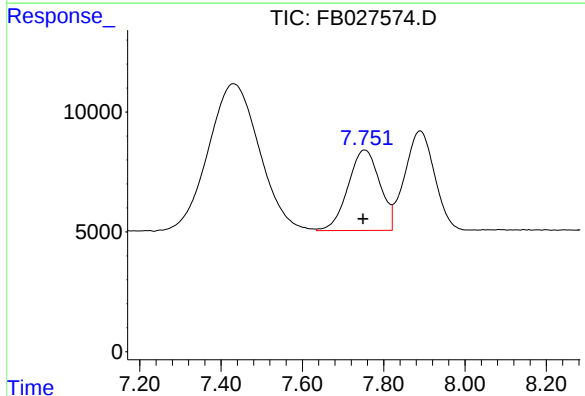


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.004 min
Response: 182462
Conc: 10.42 ng/ml

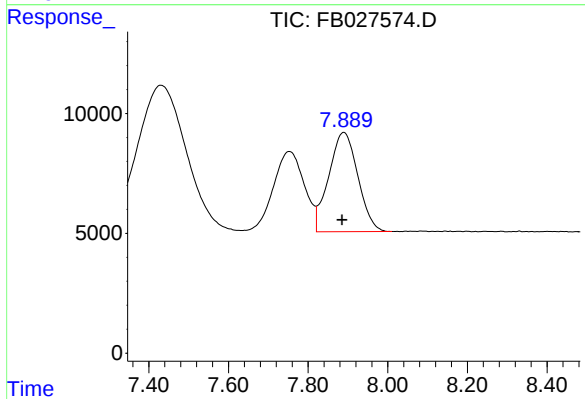


#4 Benzene

R.T.: 7.890 min
Delta R.T.: 0.005 min
Response: 210747
Conc: 10.33 ng/ml

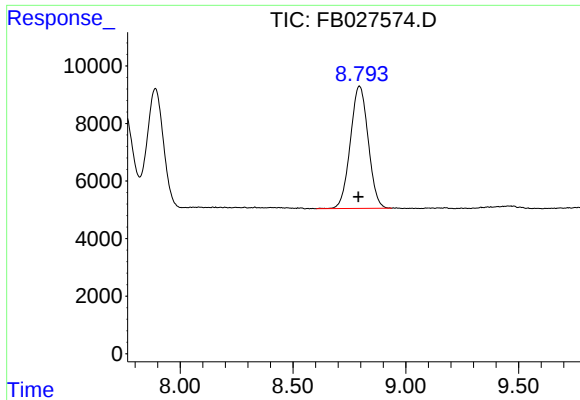


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: 0.004 min
Response: 233872
Conc: 20.85 ng/ml

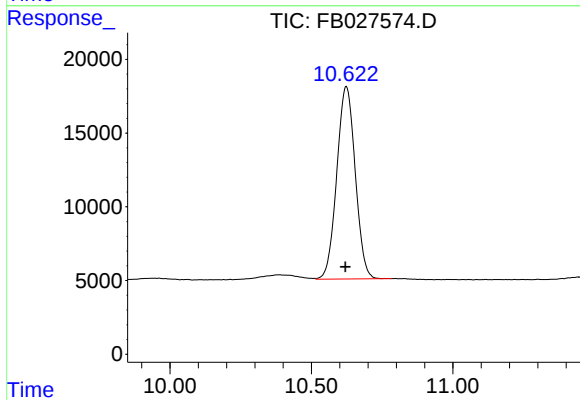


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.004 min
Response: 592182
Conc: 30.58 ng/ml

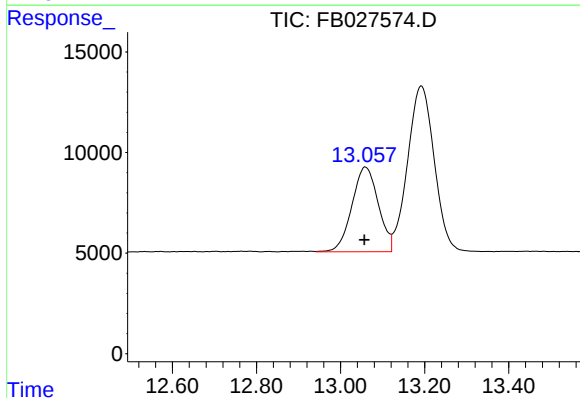


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.003 min
Response: 183433
Conc: 10.13 ng/ml

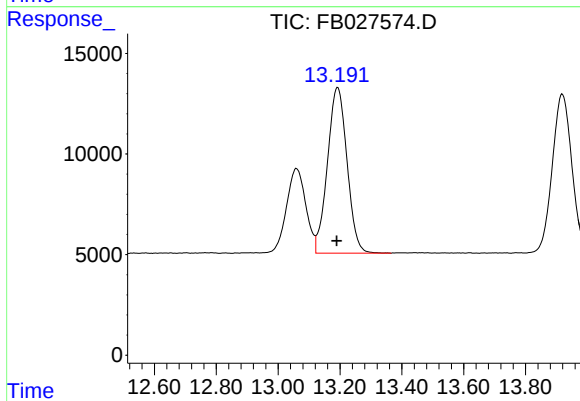

#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: 0.003 min
Response: 362589
Conc: 20.34 ng/ml

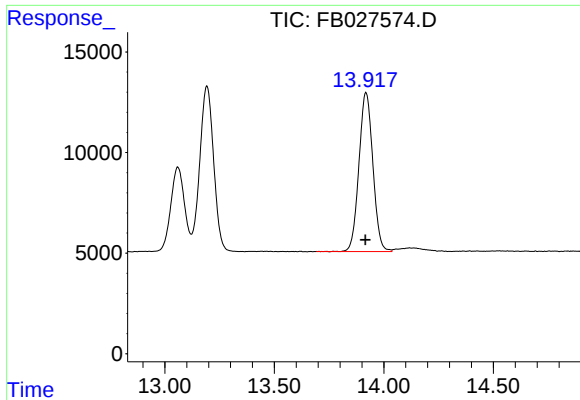


#9 O-Xylene

R.T.: 13.919 min

Delta R.T.: 0.003 min

Response: 349460

Conc: 20.11 ng/ml

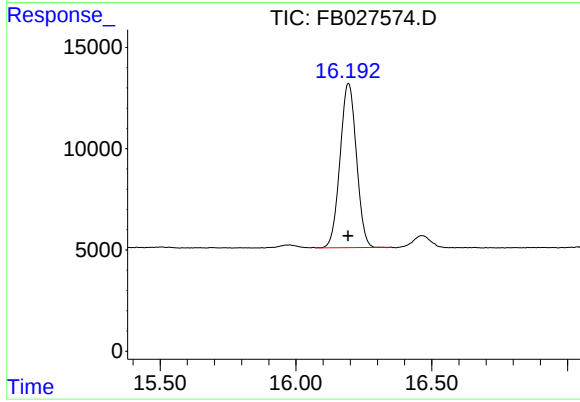

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min

Delta R.T.: 0.002 min

Response: 339429

Conc: 19.76 ng/ml