

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063022\
 Data File : FB027575.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jun 2022 14:14
 Operator : AJ/MA
 Sample : BSF0630S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 01 04:32:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	223602	19.935 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	546243	32.423 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	567316	32.310 ng/ml
3) t n-Heptane	7.754	183403	10.469 ng/ml
4) t Benzene	7.889	210667	10.331 ng/ml
6) t Toluene	10.623	610499	31.531 ng/ml
7) t Ethylbenzene	13.059	192066	10.606 ng/ml
8) t m-Xylene	13.192	378461	21.231 ng/ml
9) t O-Xylene	13.919	365501	21.035 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	367898	21.416 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063022\
Data File : FB027575.D
Signal(s) : FID2B.CH
Acq On : 30 Jun 2022 14:14
Operator : AJ/MA
Sample : BSF0630S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 01 04:32:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

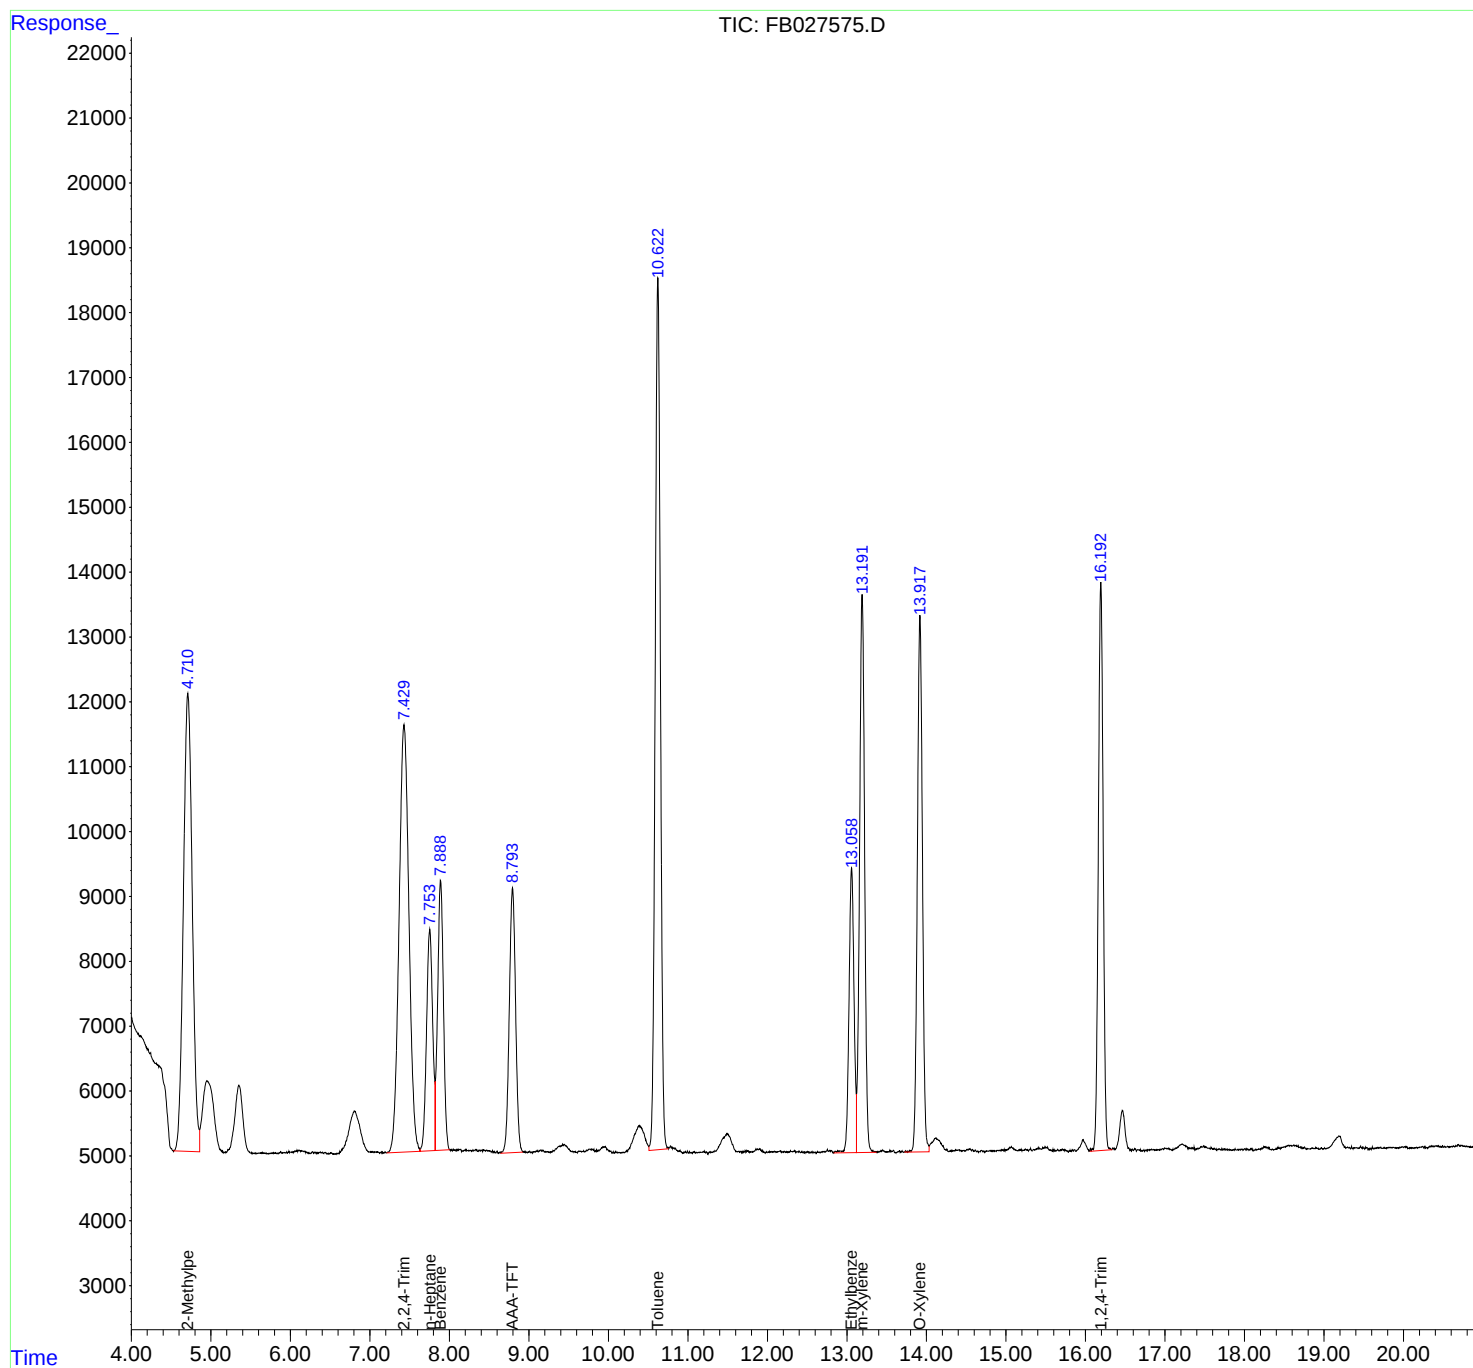

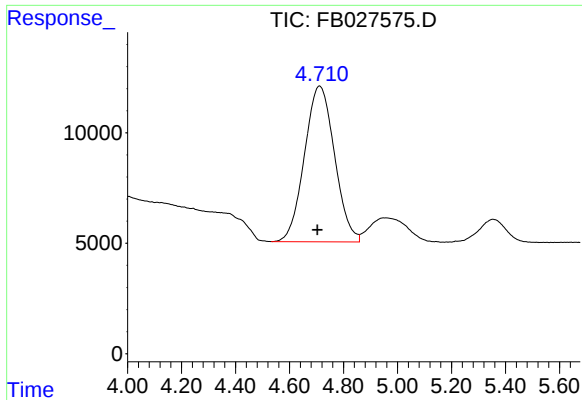


#1 2-Methylpentane

R.T.: 4.711 min
Delta R.T.: 0.007 min
Response: 546243
Conc: 32.42 ng/ml

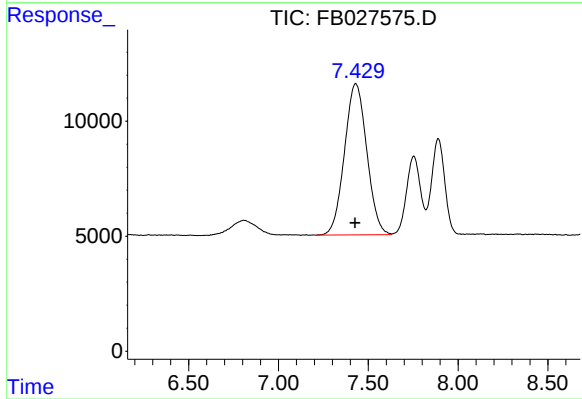


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: 0.004 min
Response: 567316
Conc: 32.31 ng/ml

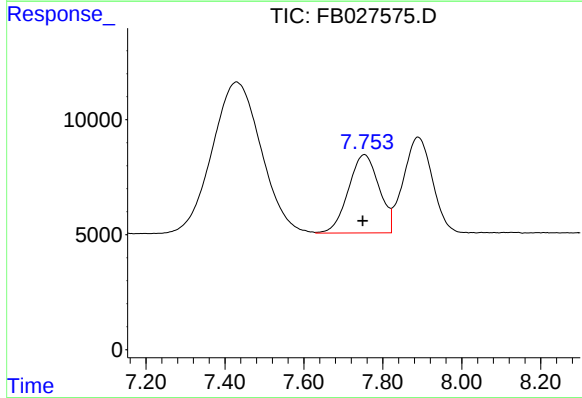


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.005 min
Response: 183403
Conc: 10.47 ng/ml

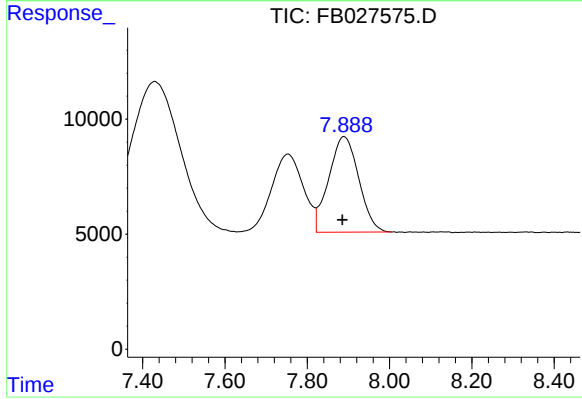


#4 Benzene

R.T.: 7.889 min
Delta R.T.: 0.004 min
Response: 210667
Conc: 10.33 ng/ml

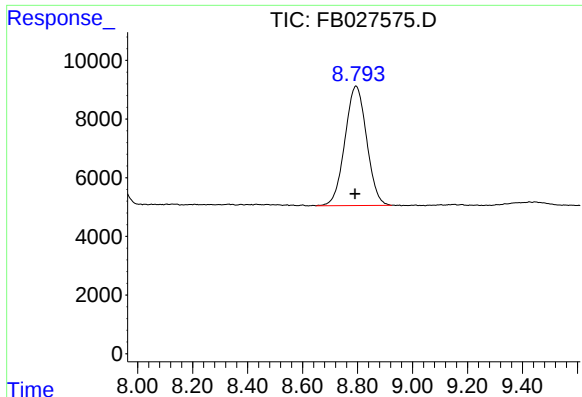


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: 0.004 min
Response: 223602
Conc: 19.93 ng/ml

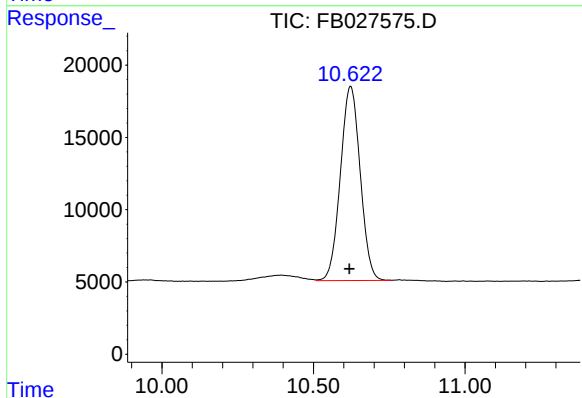


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.004 min
Response: 610499
Conc: 31.53 ng/ml

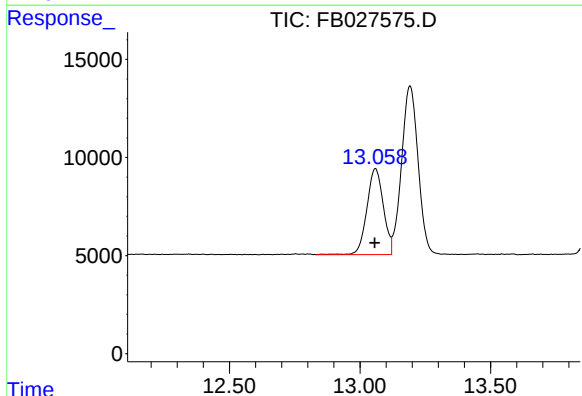


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.003 min
Response: 192066
Conc: 10.61 ng/ml

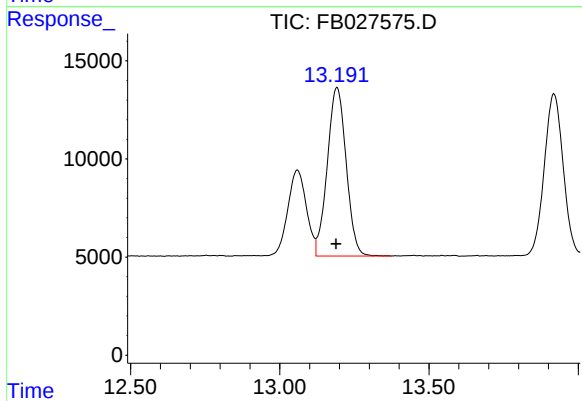


#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: 0.003 min
Response: 378461
Conc: 21.23 ng/ml

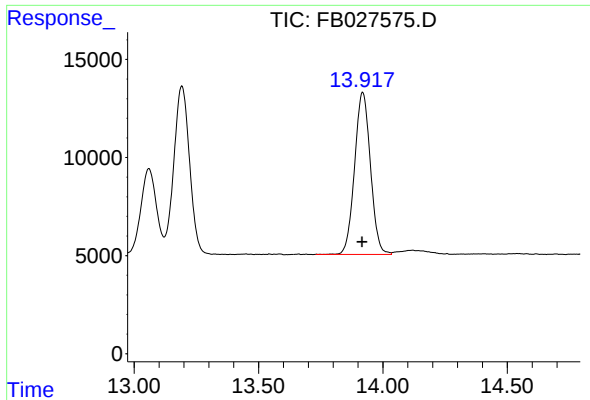

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.003 min
Response: 365501
Conc: 21.03 ng/ml

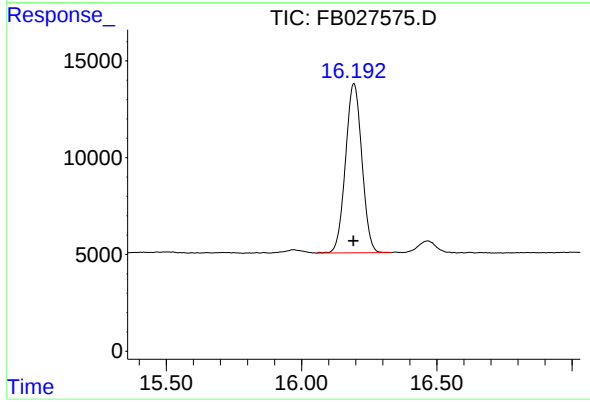

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.002 min
Response: 367898
Conc: 21.42 ng/ml