

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063022\
 Data File : FB027577.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jun 2022 15:29
 Operator : AJ/MA
 Sample : N3214-08
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 01 04:32:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	223454	19.922 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	174297	10.346 ng/ml
2) t 2,2,4-Trimethylpentane	7.434	164384	9.362 ng/ml
3) t n-Heptane	7.758	54065	3.086 ng/ml
4) t Benzene	7.892	58872	2.887 ng/ml
6) t Toluene	10.625	173704	8.971 ng/ml
7) t Ethylbenzene	13.062	55228	3.050 ng/ml
8) t m-Xylene	13.194	109321	6.133 ng/ml
9) t O-Xylene	13.921	105550	6.074 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	107747	6.272 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063022\
Data File : FB027577.D
Signal(s) : FID2B.CH
Acq On : 30 Jun 2022 15:29
Operator : AJ/MA
Sample : N3214-08
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 01 04:32:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

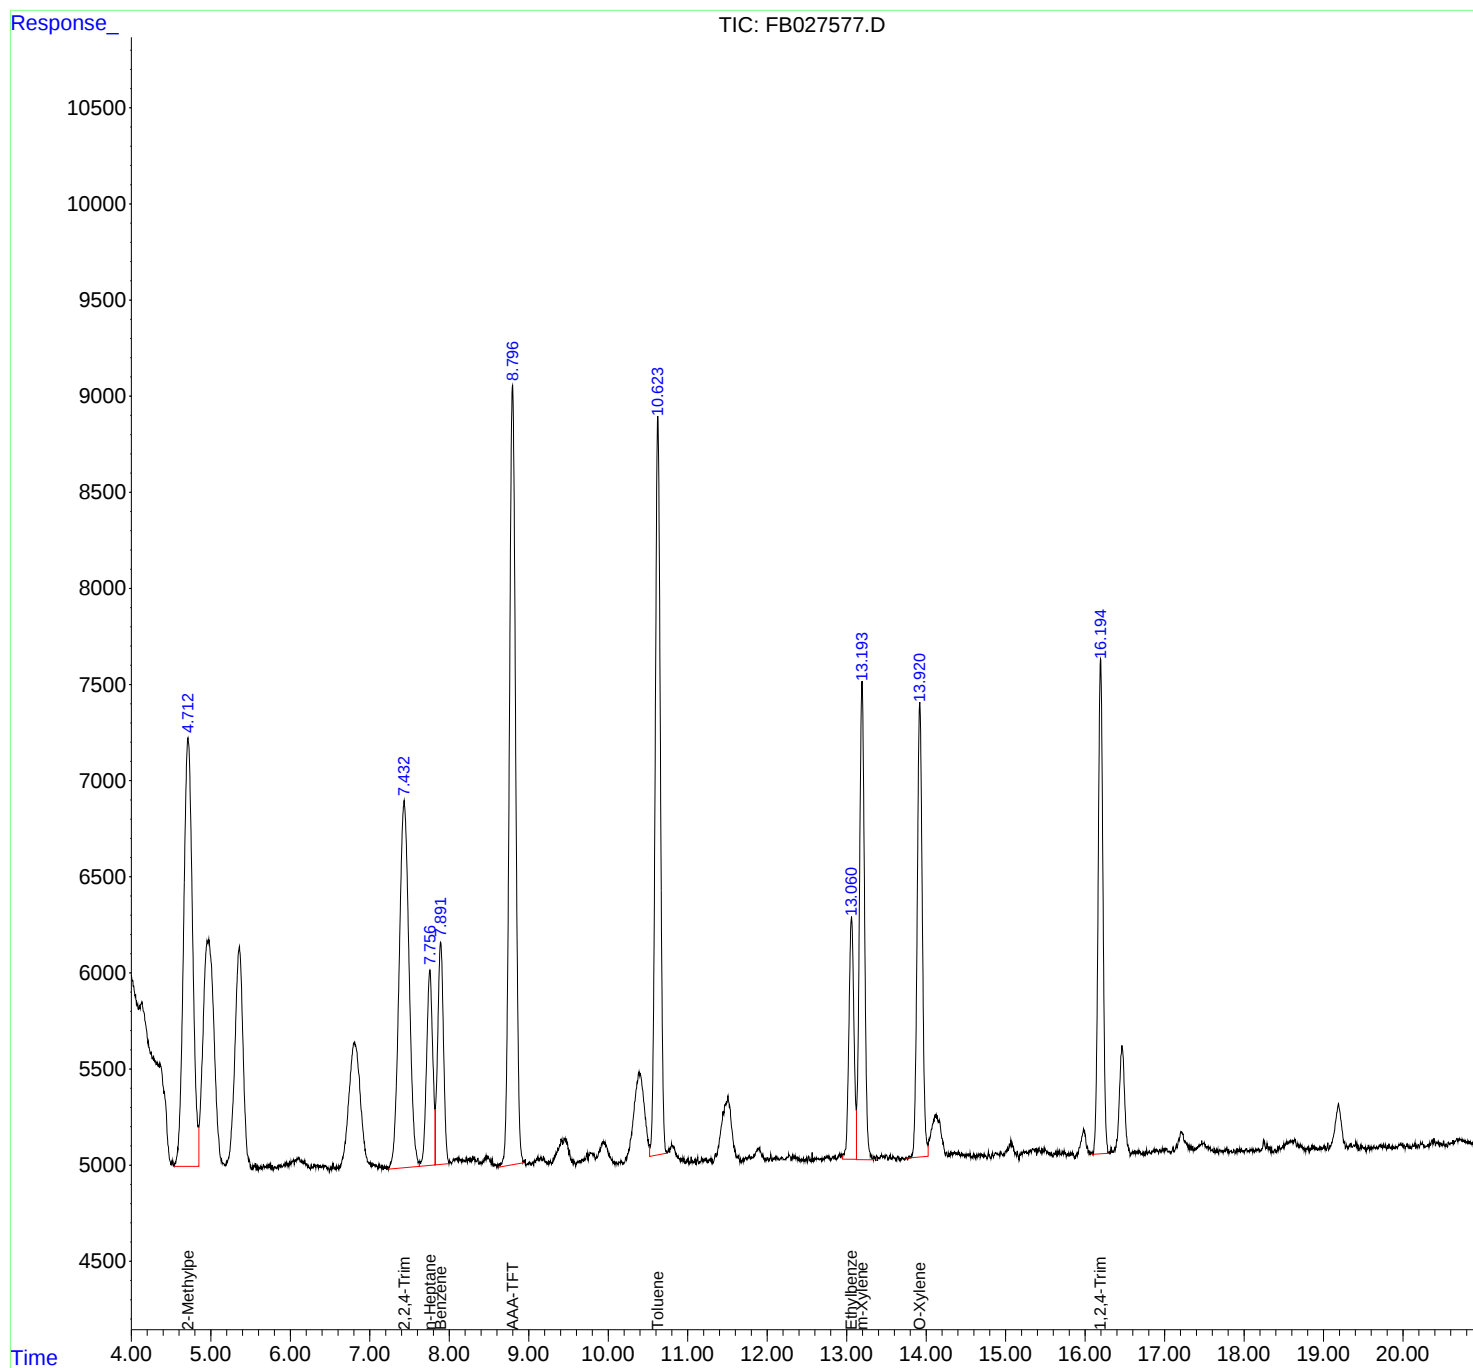

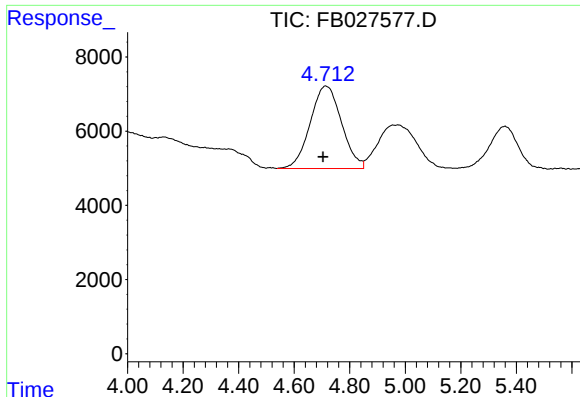


#1 2-Methylpentane

R.T.: 4.713 min
Delta R.T.: 0.009 min
Response: 174297
Conc: 10.35 ng/ml

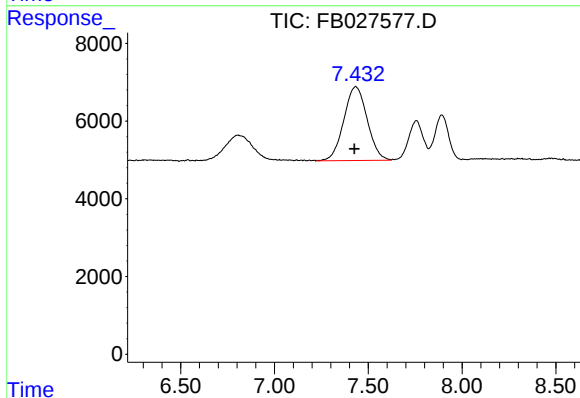


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: 0.007 min
Response: 164384
Conc: 9.36 ng/ml

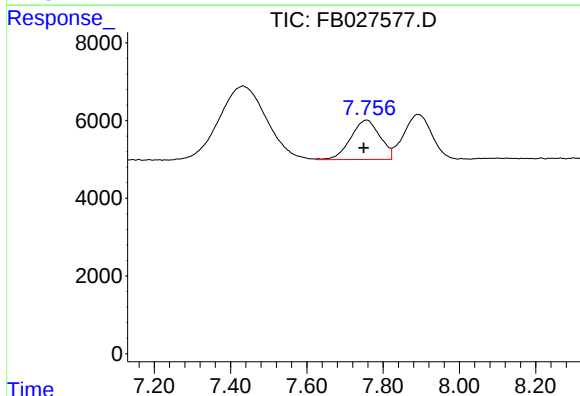


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.008 min
Response: 54065
Conc: 3.09 ng/ml

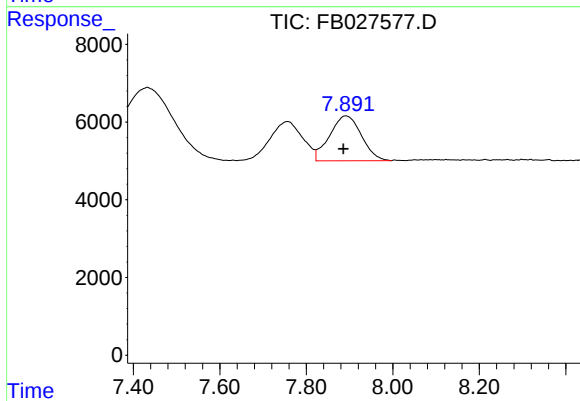


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.007 min
Response: 58872
Conc: 2.89 ng/ml

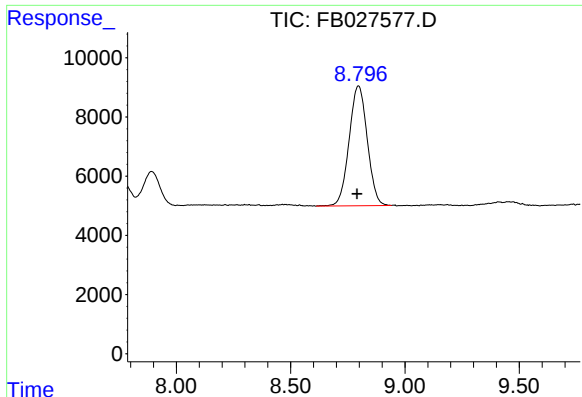


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.006 min
Response: 223454
Conc: 19.92 ng/ml

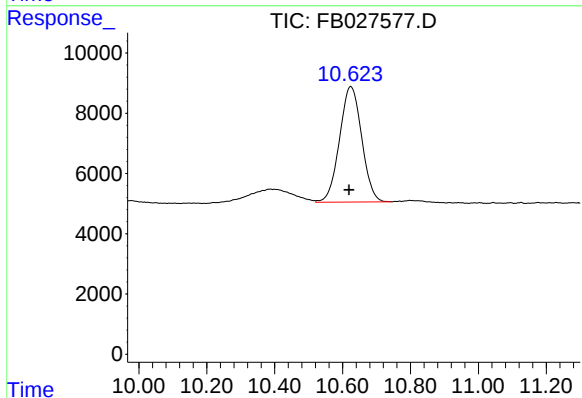


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.005 min
Response: 173704
Conc: 8.97 ng/ml

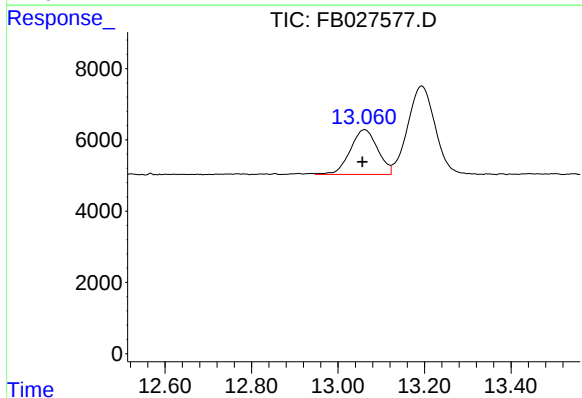


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: 0.006 min
Response: 55228
Conc: 3.05 ng/ml

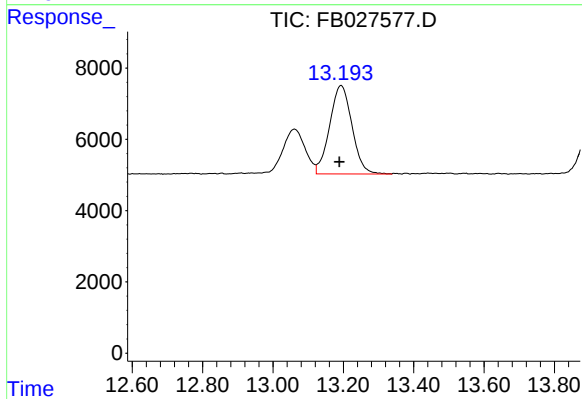


#8 m-Xylene

R.T.: 13.194 min
Delta R.T.: 0.005 min
Response: 109321
Conc: 6.13 ng/ml

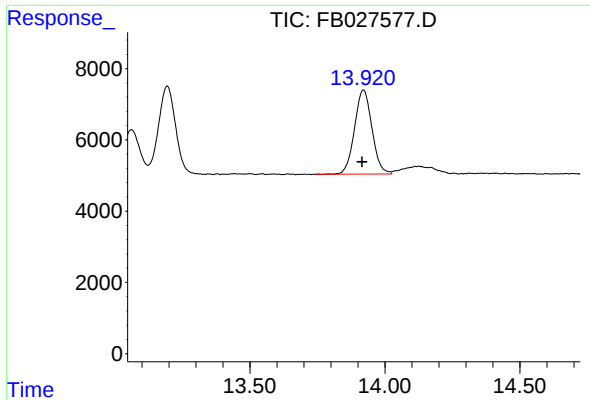

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: 0.005 min
Response: 105550
Conc: 6.07 ng/ml

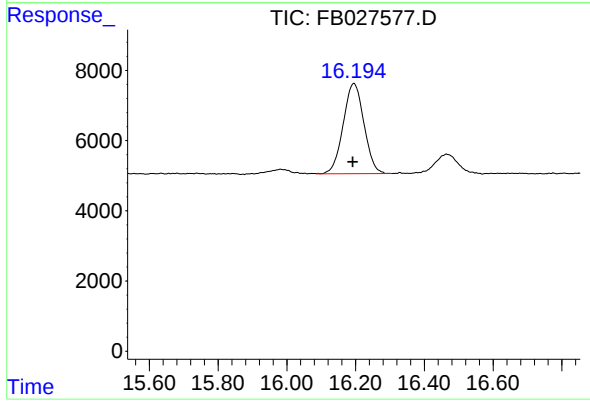

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.004 min
Response: 107747
Conc: 6.27 ng/ml