

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063022\
 Data File : FB027578.D
 Signal(s) : FID2B.CH
 Acq On : 30 Jun 2022 16:17
 Operator : AJ/MA
 Sample : N3214-07
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jul 01 04:32:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	221038	19.706 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	44301	2.630 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	28711	1.635 ng/ml
3) t n-Heptane	7.756	8649	0.494 ng/ml
4) t Benzene	7.892	9346	0.458 ng/ml
6) t Toluene	10.624	31675	1.636 ng/ml
7) t Ethylbenzene	13.067	9963	0.550 ng/ml
8) t m-Xylene	13.194	20109	1.128 ng/ml
9) t O-Xylene	13.925	17670	1.017 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	21534	1.254 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063022\
Data File : FB027578.D
Signal(s) : FID2B.CH
Acq On : 30 Jun 2022 16:17
Operator : AJ/MA
Sample : N3214-07
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 01 04:32:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

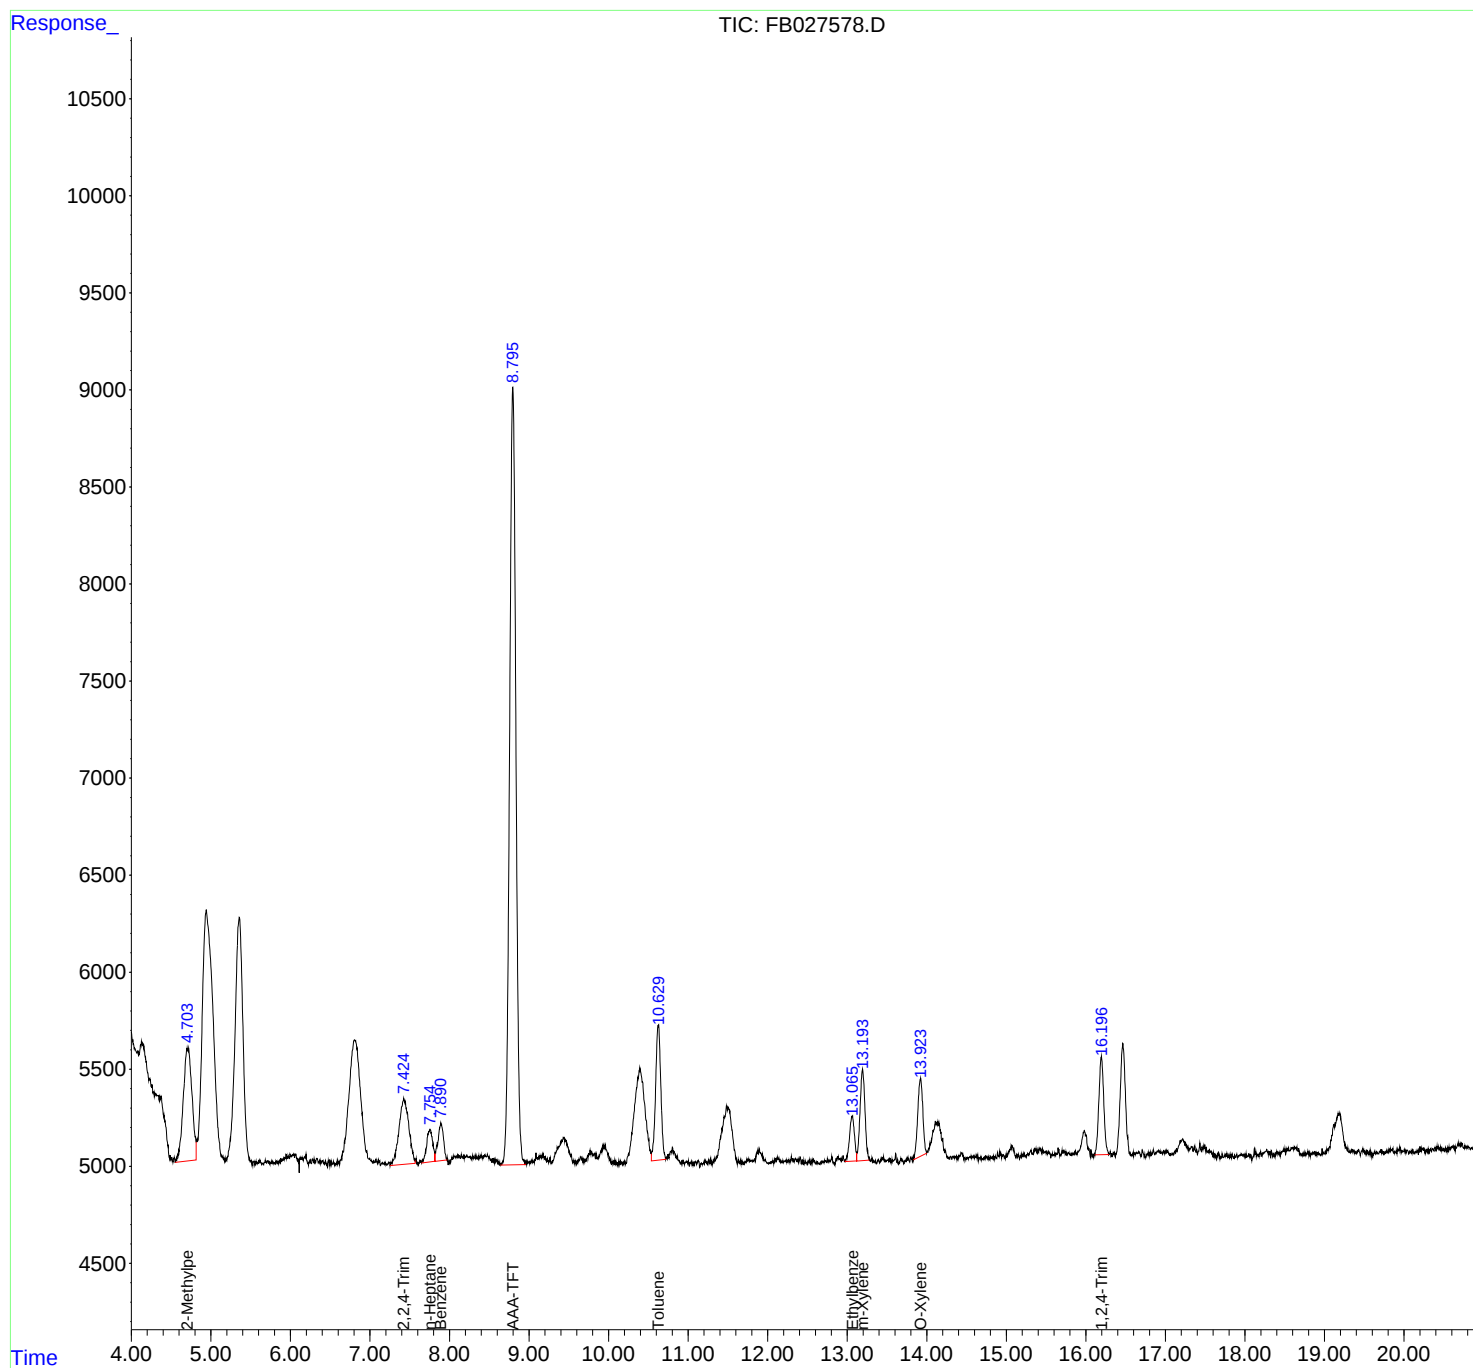

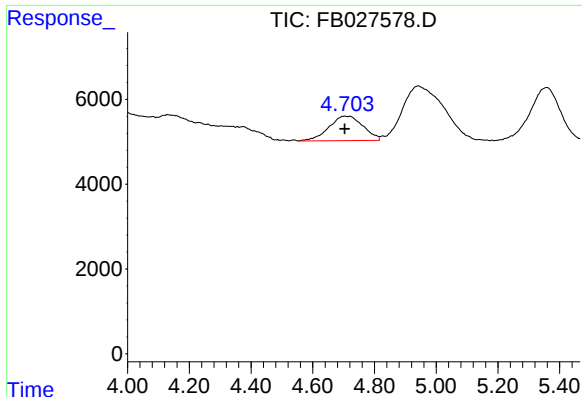


#1 2-Methylpentane

R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 44301
Conc: 2.63 ng/ml

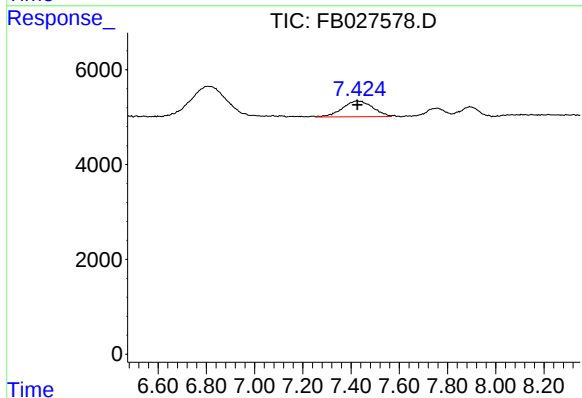


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: 0.000 min
Response: 28711
Conc: 1.64 ng/ml

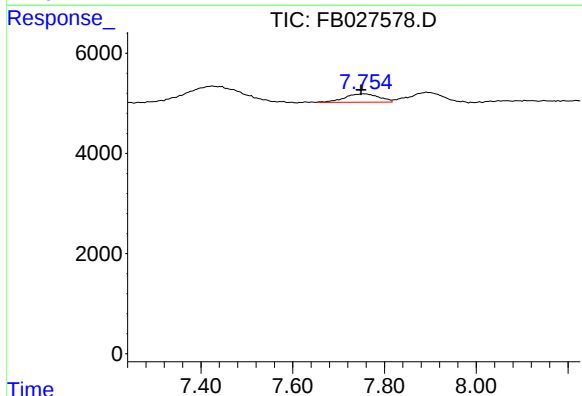


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.006 min
Response: 8649
Conc: 0.49 ng/ml

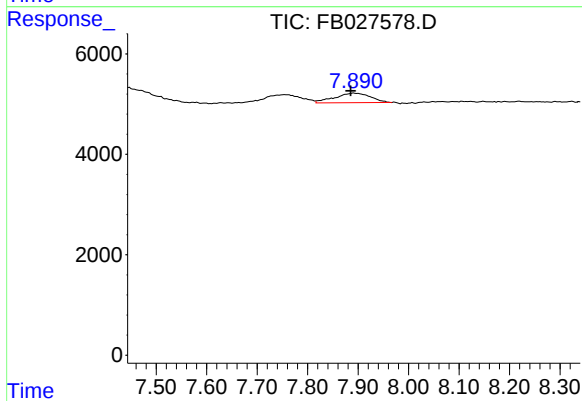


#4 Benzene

R.T.: 7.892 min
Delta R.T.: 0.006 min
Response: 9346
Conc: 0.46 ng/ml

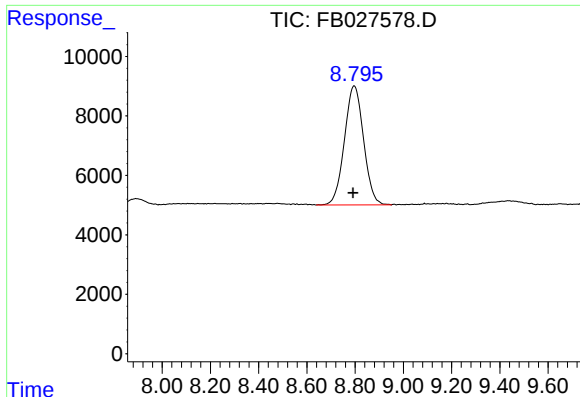


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.006 min
Response: 221038
Conc: 19.71 ng/ml

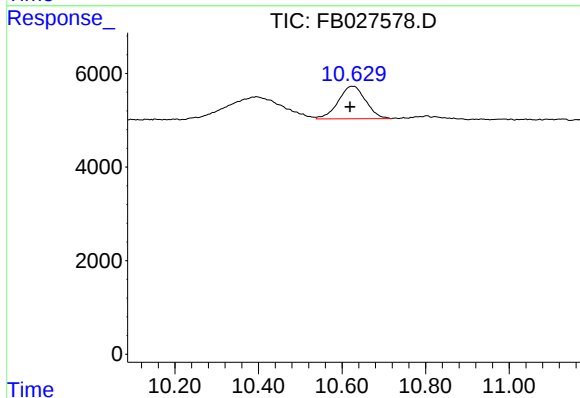


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.005 min
Response: 31675
Conc: 1.64 ng/ml

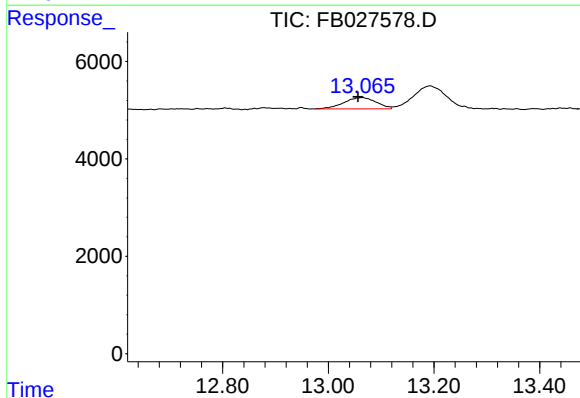


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.010 min
Response: 9963
Conc: 0.55 ng/ml

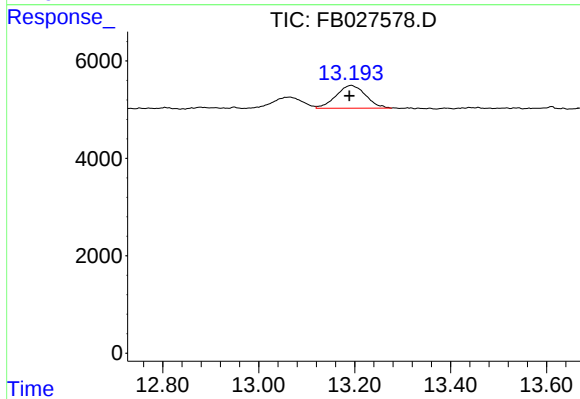


#8 m-Xylene

R.T.: 13.194 min
Delta R.T.: 0.005 min
Response: 20109
Conc: 1.13 ng/ml

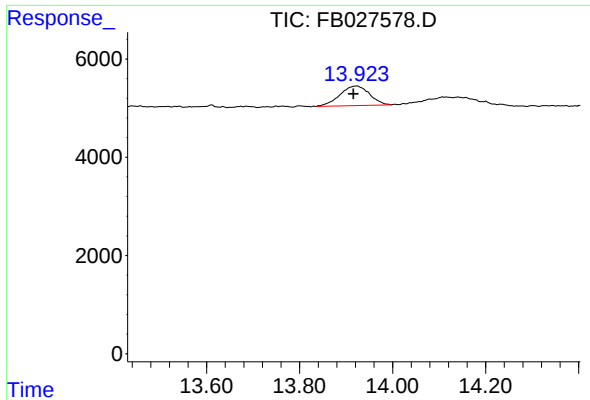

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.009 min
Response: 17670
Conc: 1.02 ng/ml

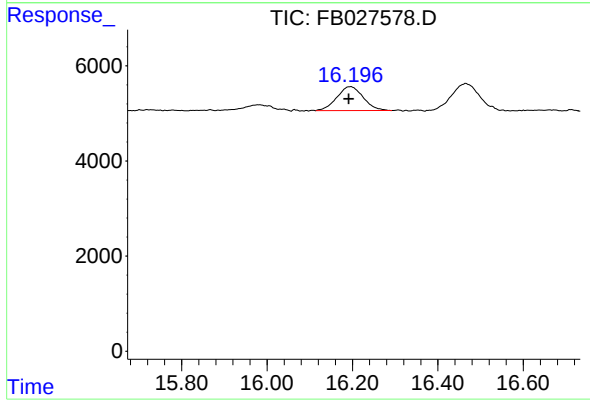

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.005 min
Response: 21534
Conc: 1.25 ng/ml