

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063025\
Data File : FB031971.D
Signal(s) : FID2B.CH
Acq On : 30 Jun 2025 12:59
Operator : YP/AJ
Sample : Q2436-04
Misc : 4.08G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-86

Integration File: Calibration.e
Quant Time: Jul 01 01:07:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	381071	24.700 ng/ml
Target Compounds			
8) t m-Xylene	13.187	2579	0.079 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB063025\
Data File : FB031971.D
Signal(s) : FID2B.CH
Acq On : 30 Jun 2025 12:59
Operator : YP/AJ
Sample : Q2436-04
Misc : 4.08G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-86

Integration File: Calibration.e
Quant Time: Jul 01 01:07:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

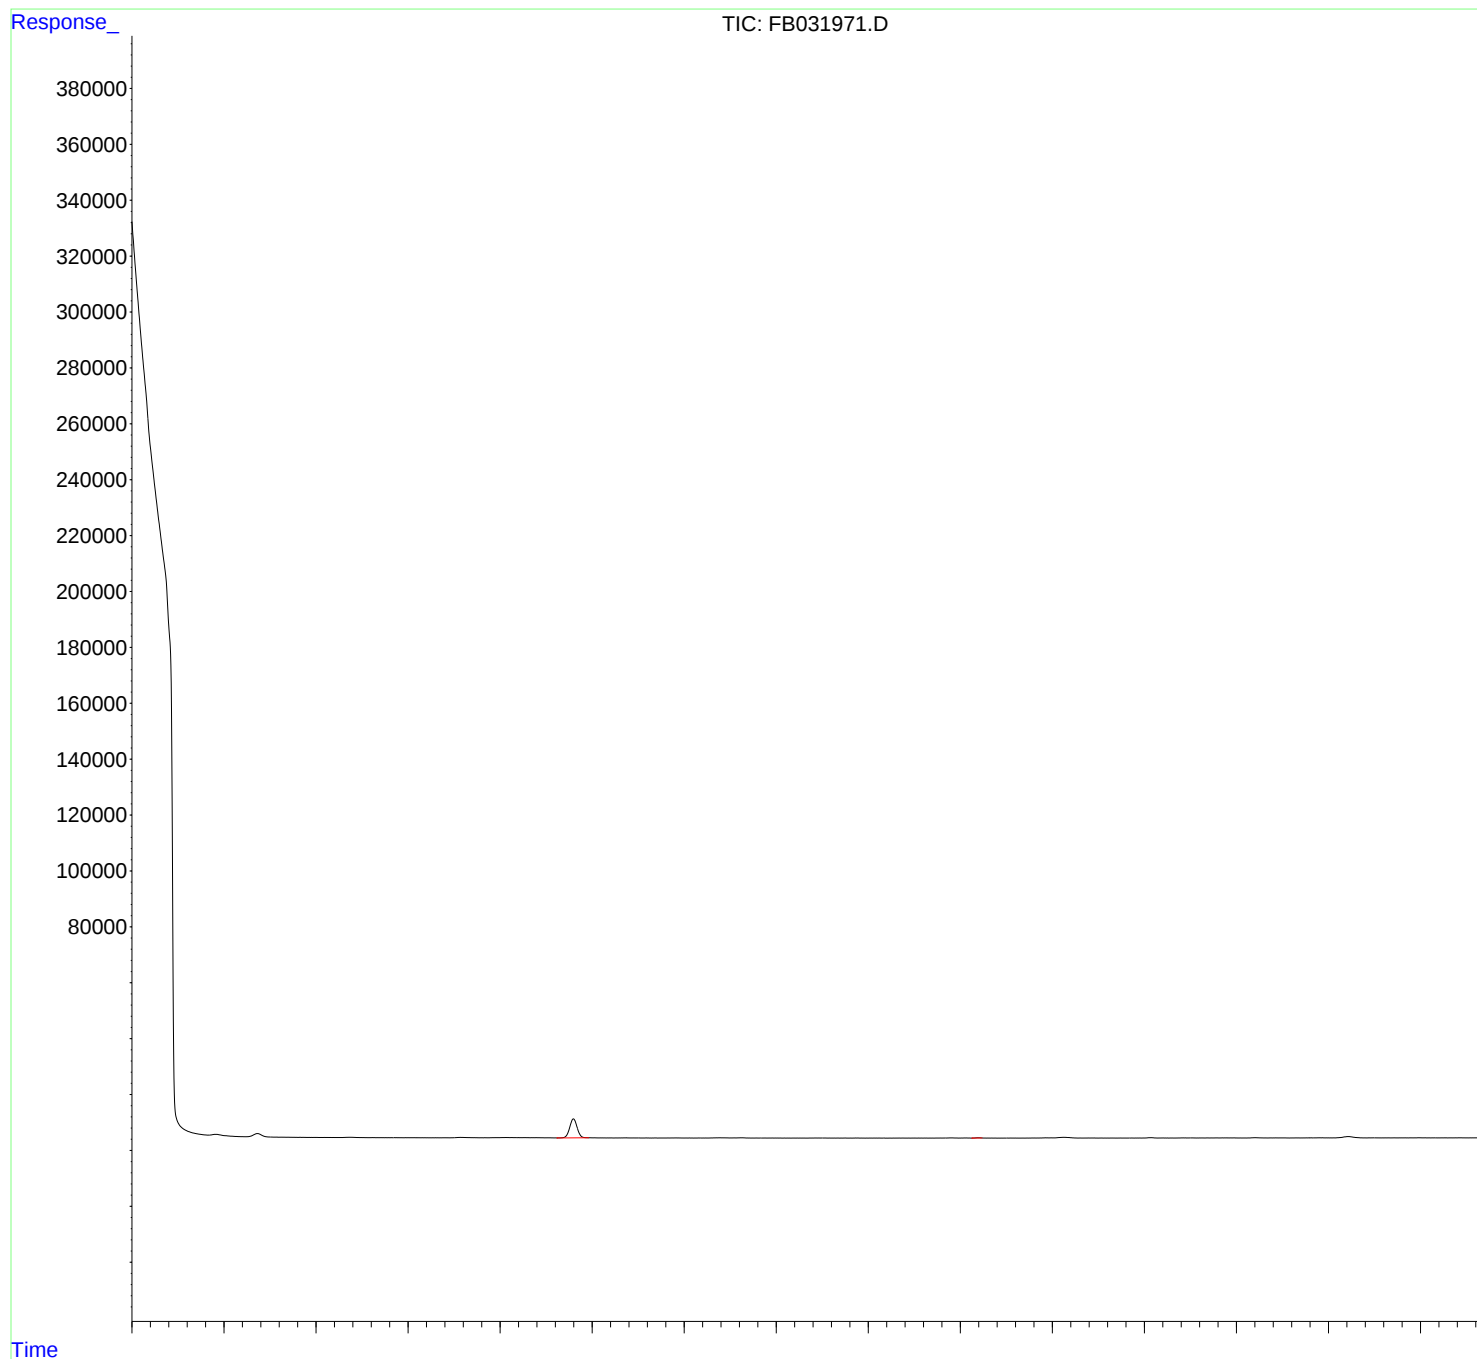


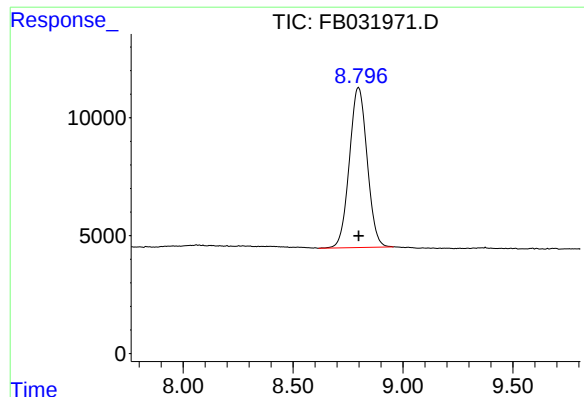

#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.000 min
Response: 381071
Conc: 24.70 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-86

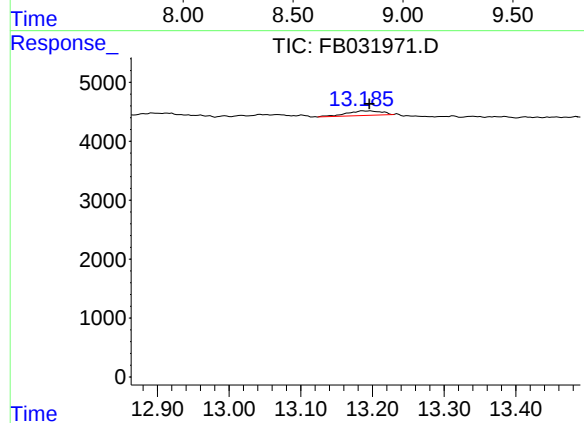

#8 m-Xylene

R.T.: 13.187 min
Delta R.T.: -0.009 min
Response: 2579
Conc: 0.08 ng/ml