

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB063025\  
Data File : FB031974.D  
Signal(s) : FID2B.CH  
Acq On : 30 Jun 2025 14:40  
Operator : YP/AJ  
Sample : Q2458-01  
Misc : 4.12G/5.00 ML DI WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
TP-76

Integration File: Calibration.e  
Quant Time: Jul 01 01:07:42 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB062325.M  
Quant Title :  
QLast Update : Mon Jun 23 13:56:54 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.802  | 252071   | 16.339 ng/ml |
| Target Compounds             |        |          |              |
| 6) t Toluene                 | 10.625 | 5641     | 0.158 ng/ml  |
| 8) t m-Xylene                | 13.199 | 5045     | 0.154 ng/ml  |
| 9) t O-Xylene                | 13.933 | 4111     | 0.132 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.205 | 11486    | 0.434 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB063025\  
Data File : FB031974.D  
Signal(s) : FID2B.CH  
Acq On : 30 Jun 2025 14:40  
Operator : YP/AJ  
Sample : Q2458-01  
Misc : 4.12G/5.00 ML DI WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
TP-76

Integration File: Calibration.e  
Quant Time: Jul 01 01:07:42 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB062325.M  
Quant Title :  
QLast Update : Mon Jun 23 13:56:54 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

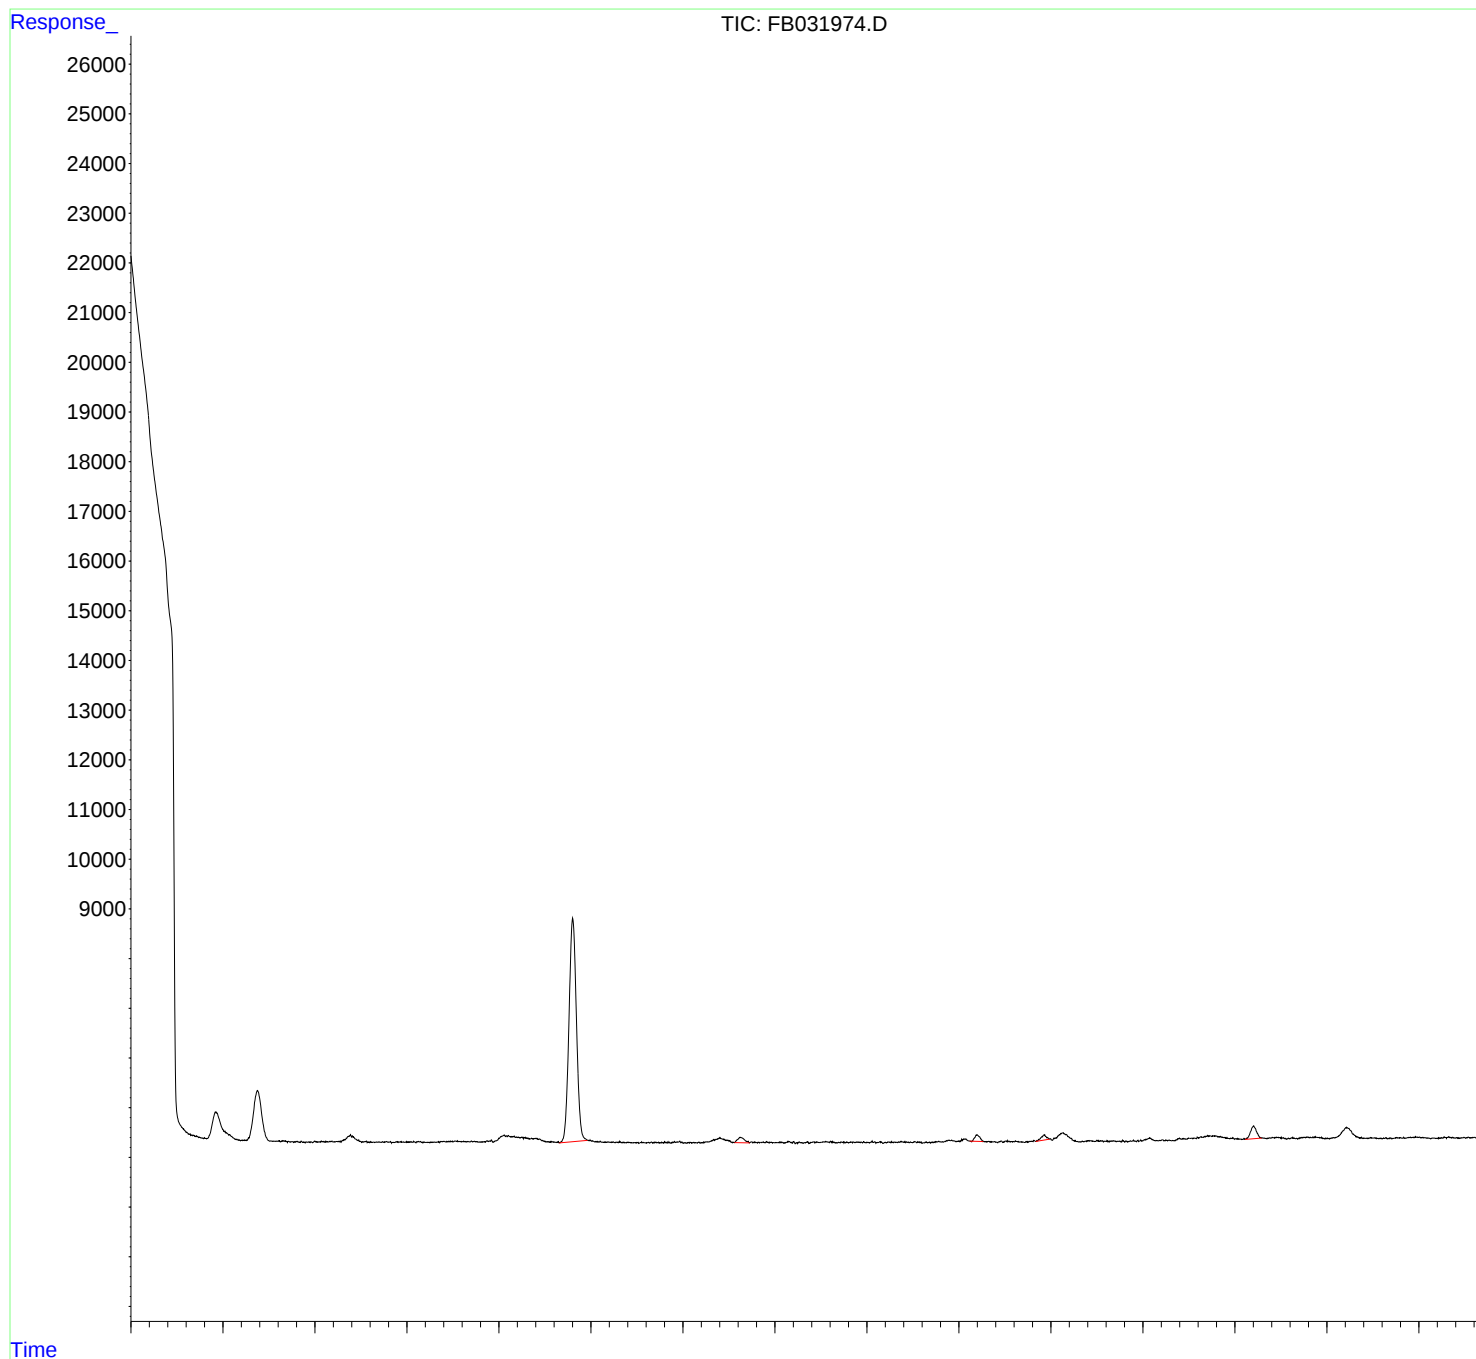


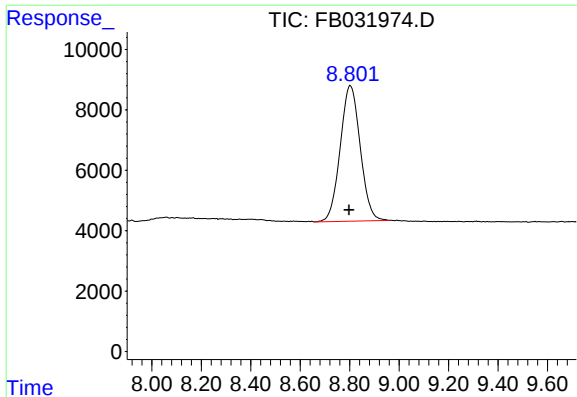

#5 AAA-TFT


R.T.: 8.802 min  
Delta R.T.: 0.004 min  
Response: 252071  
Conc: 16.34 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
TP-76

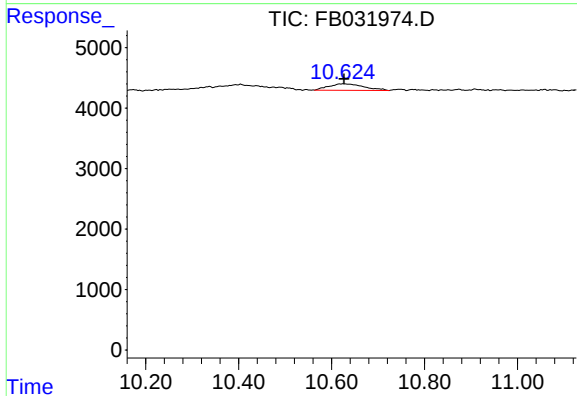


#6 Toluene

R.T.: 10.625 min  
Delta R.T.: -0.001 min  
Response: 5641  
Conc: 0.16 ng/ml

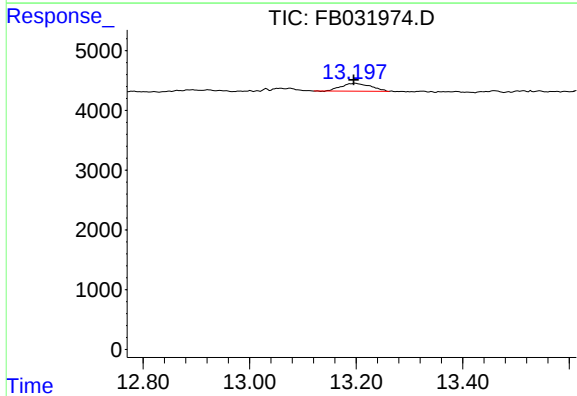


#8 m-Xylene

R.T.: 13.199 min  
Delta R.T.: 0.003 min  
Response: 5045  
Conc: 0.15 ng/ml

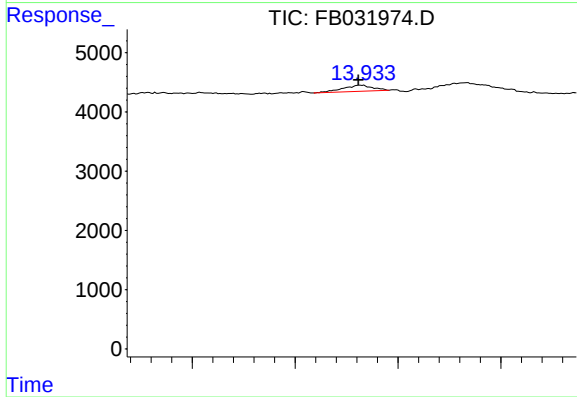

#9 O-Xylene

R.T.: 13.933 min  
Delta R.T.: 0.011 min  
Response: 4111  
Conc: 0.13 ng/ml

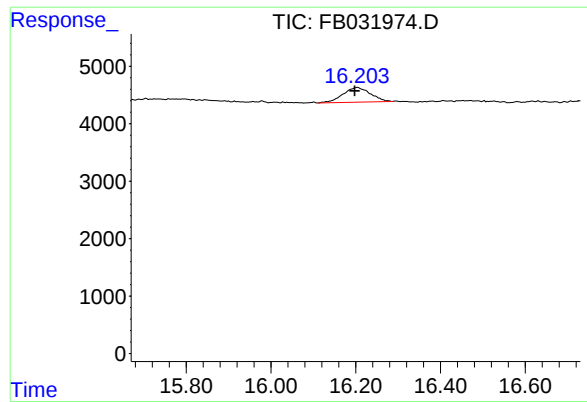

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min  
Delta R.T.: 0.007 min  
Response: 11486  
Conc: 0.43 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
TP-76