

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070119\
 Data File : FB021603.D
 Signal(s) : FID2B.CH
 Acq On : 1 Jul 2019 14:12
 Operator : MJ/SJ
 Sample : K3158-09MS
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OK-01-062819MS

Integration File: Calibration.e
 Quant Time: Jul 02 00:43:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.990	279481	20.213 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.862	933994	27.360 ng/ml
2) t 2,2,4-Trimethylpentane	7.610	881631	28.529 ng/ml
3) t n-Heptane	7.949	276595	9.450 ng/ml
4) t Benzene	8.084	324116	9.657 ng/ml
6) t Toluene	10.831	668668	29.273 ng/ml
7) t Ethylbenzene	13.277	235047	9.929 ng/ml
8) t m-Xylene	13.409	504812	19.917 ng/ml
9) t O-Xylene	14.139	523292	19.952 ng/ml
10) t 1,2,4-Trimethylbenzene	16.418	526739	20.048 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070119\
Data File : FB021603.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2019 14:12
Operator : MJ/SJ
Sample : K3158-09MS
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OK-01-062819MS

Integration File: Calibration.e
Quant Time: Jul 02 00:43:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

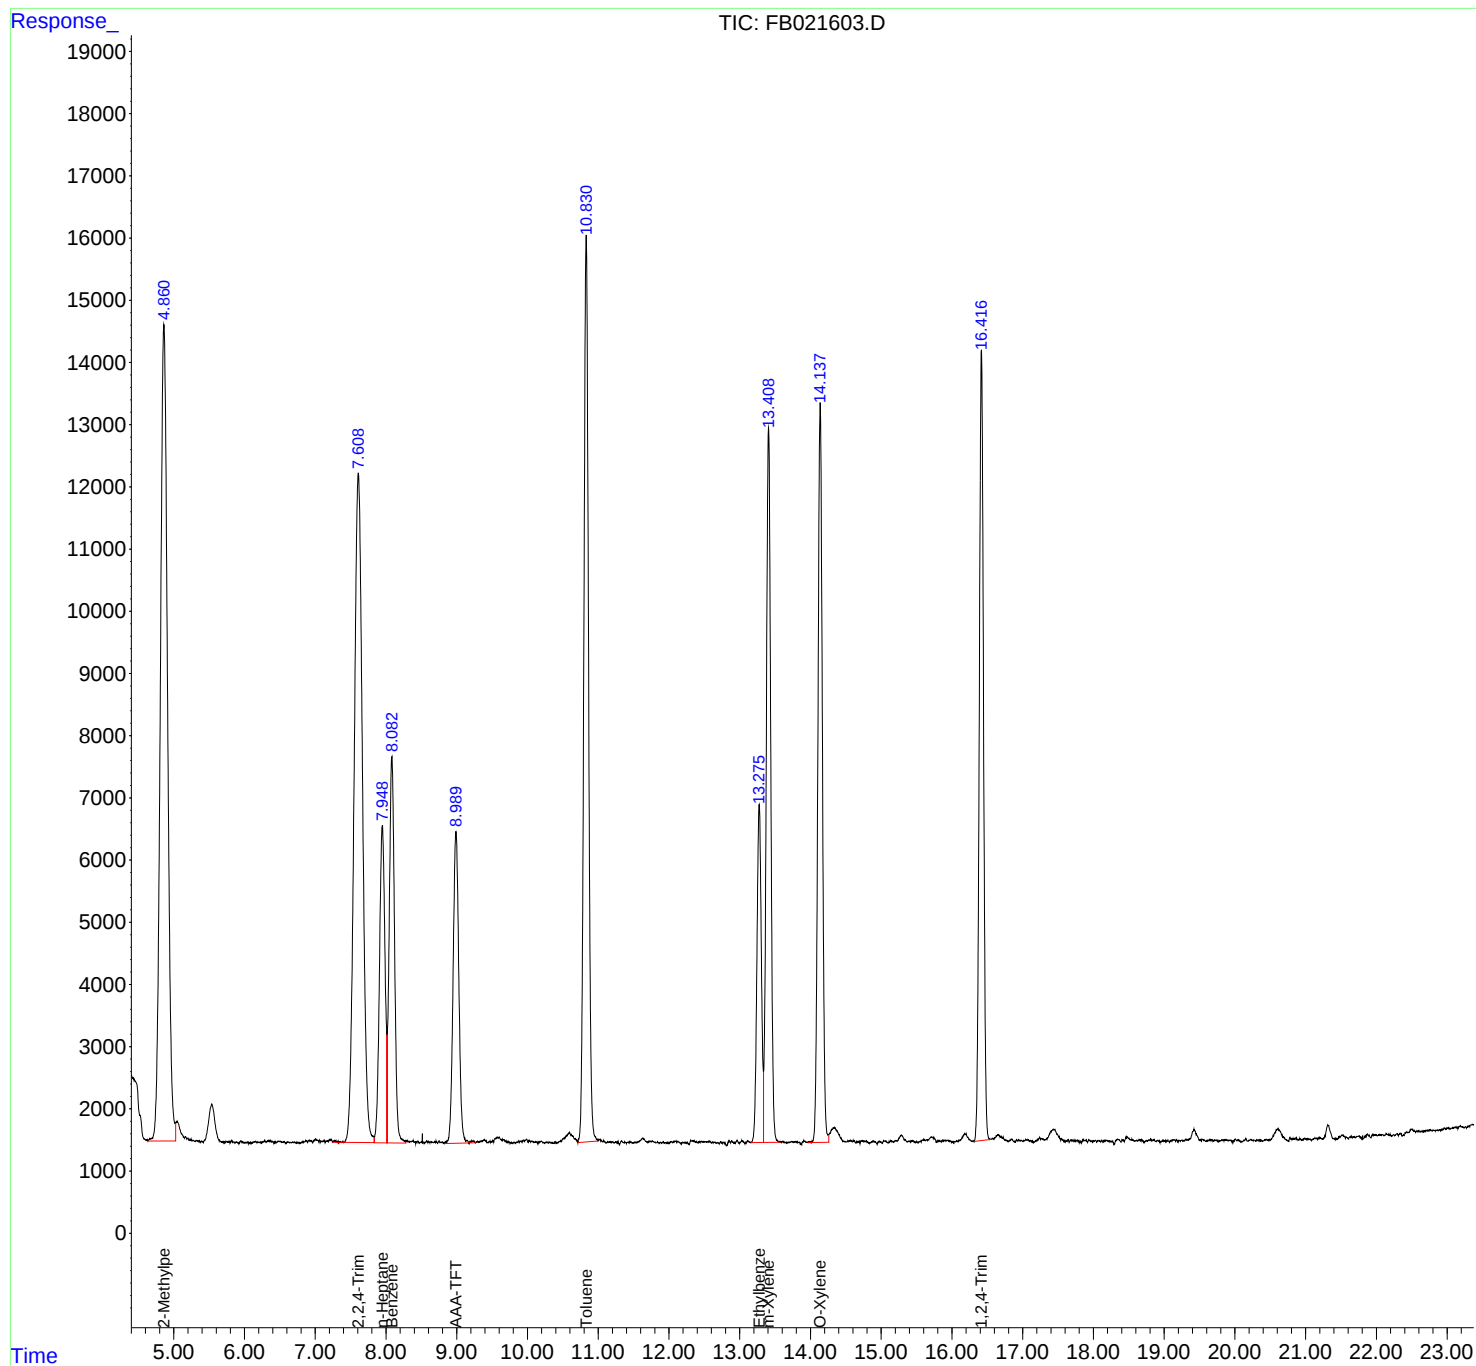


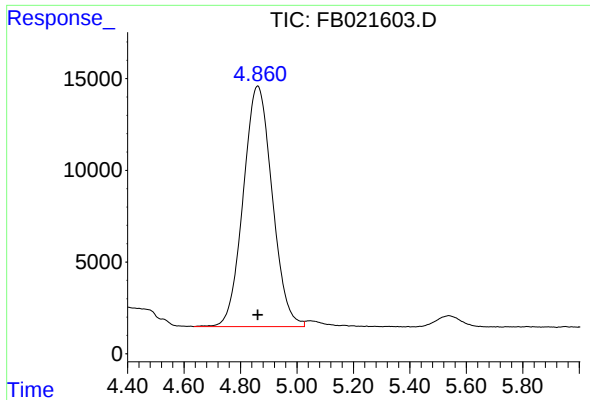

#1 2-Methylpentane


R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 933994
Conc: 27.36 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-01-062819MS

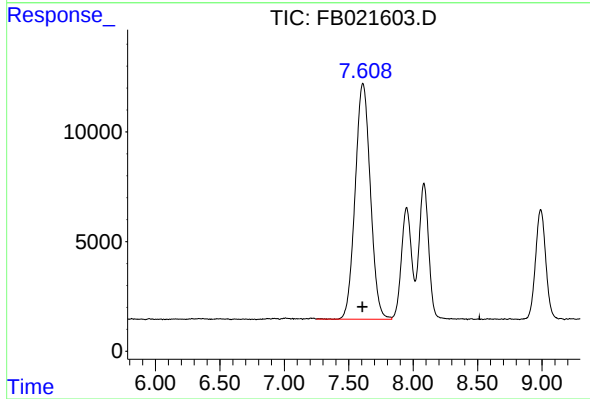


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
Delta R.T.: 0.002 min
Response: 881631
Conc: 28.53 ng/ml

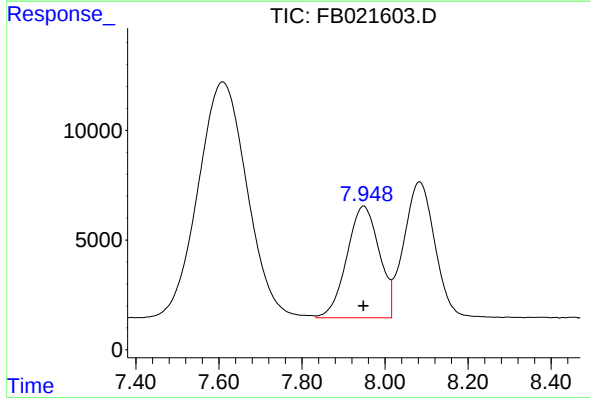


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: 0.001 min
Response: 276595
Conc: 9.45 ng/ml

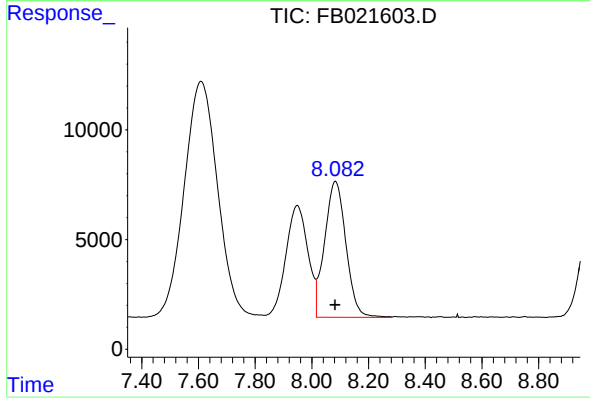

#4 Benzene


R.T.: 8.084 min
Delta R.T.: 0.001 min
Response: 324116
Conc: 9.66 ng/ml

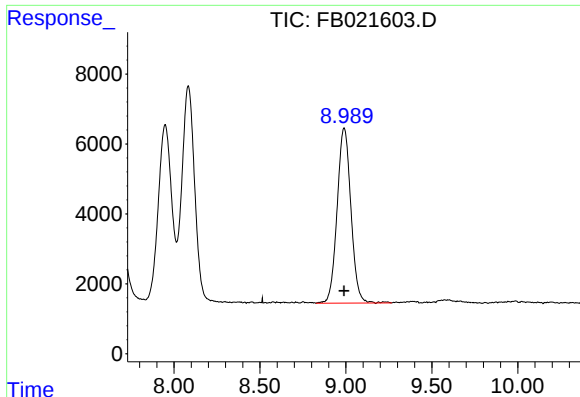

#5 AAA-TFT


R.T.: 8.990 min
Delta R.T.: 0.002 min
Response: 279481
Conc: 20.21 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-01-062819MS

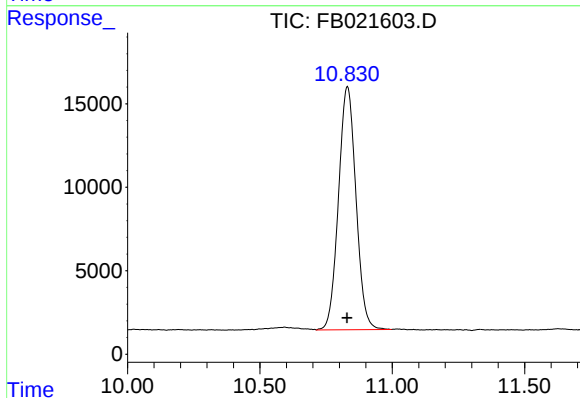


#6 Toluene

R.T.: 10.831 min
Delta R.T.: 0.001 min
Response: 668668
Conc: 29.27 ng/ml

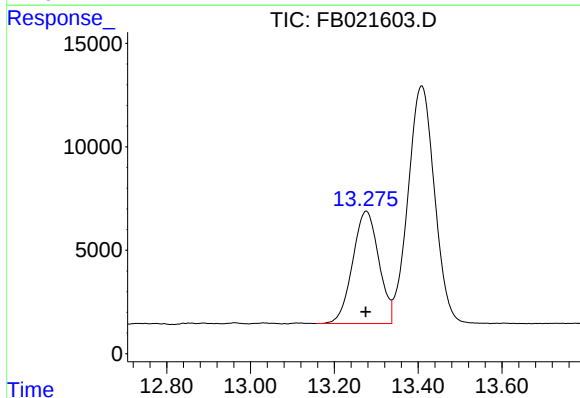


#7 Ethylbenzene

R.T.: 13.277 min
Delta R.T.: 0.001 min
Response: 235047
Conc: 9.93 ng/ml

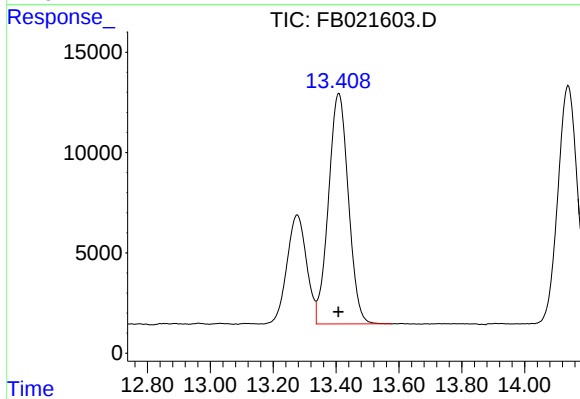

#8 m-Xylene


R.T.: 13.409 min
Delta R.T.: 0.001 min
Response: 504812
Conc: 19.92 ng/ml

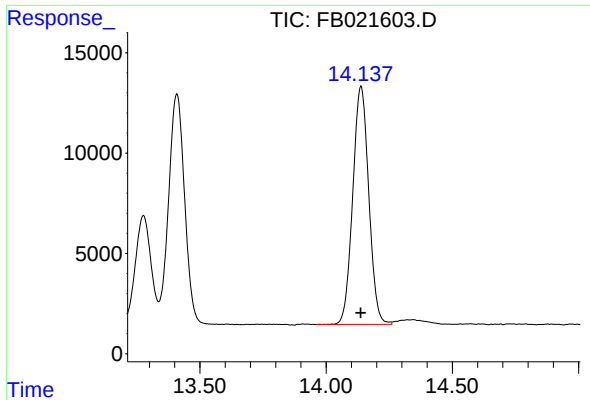

#9 O-Xylene

R.T.: 14.139 min
Delta R.T.: 0.000 min
Response: 523292
Conc: 19.95 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-01-062819MS

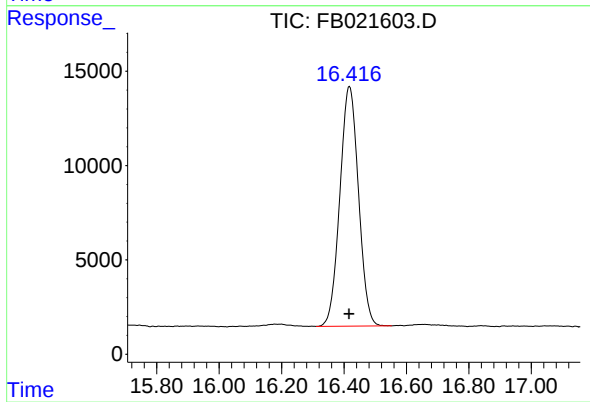

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min
Delta R.T.: 0.000 min
Response: 526739
Conc: 20.05 ng/ml