

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070119\
 Data File : FB021604.D
 Signal(s) : FID2B.CH
 Acq On : 1 Jul 2019 14:42
 Operator : MJ/SJ
 Sample : K3158-09MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OK-01-062819MSD

Integration File: Calibration.e
 Quant Time: Jul 02 00:43:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.991	282697	20.446 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.863	991822	29.054 ng/ml
2) t 2,2,4-Trimethylpentane	7.611	909089	29.418 ng/ml
3) t n-Heptane	7.950	286515	9.789 ng/ml
4) t Benzene	8.085	347965	10.367 ng/ml
6) t Toluene	10.831	703819	30.812 ng/ml
7) t Ethylbenzene	13.277	240349	10.153 ng/ml
8) t m-Xylene	13.410	511506	20.181 ng/ml
9) t O-Xylene	14.139	531557	20.268 ng/ml
10) t 1,2,4-Trimethylbenzene	16.418	536827	20.432 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070119\
Data File : FB021604.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2019 14:42
Operator : MJ/SJ
Sample : K3158-09MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OK-01-062819MSD

Integration File: Calibration.e
Quant Time: Jul 02 00:43:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

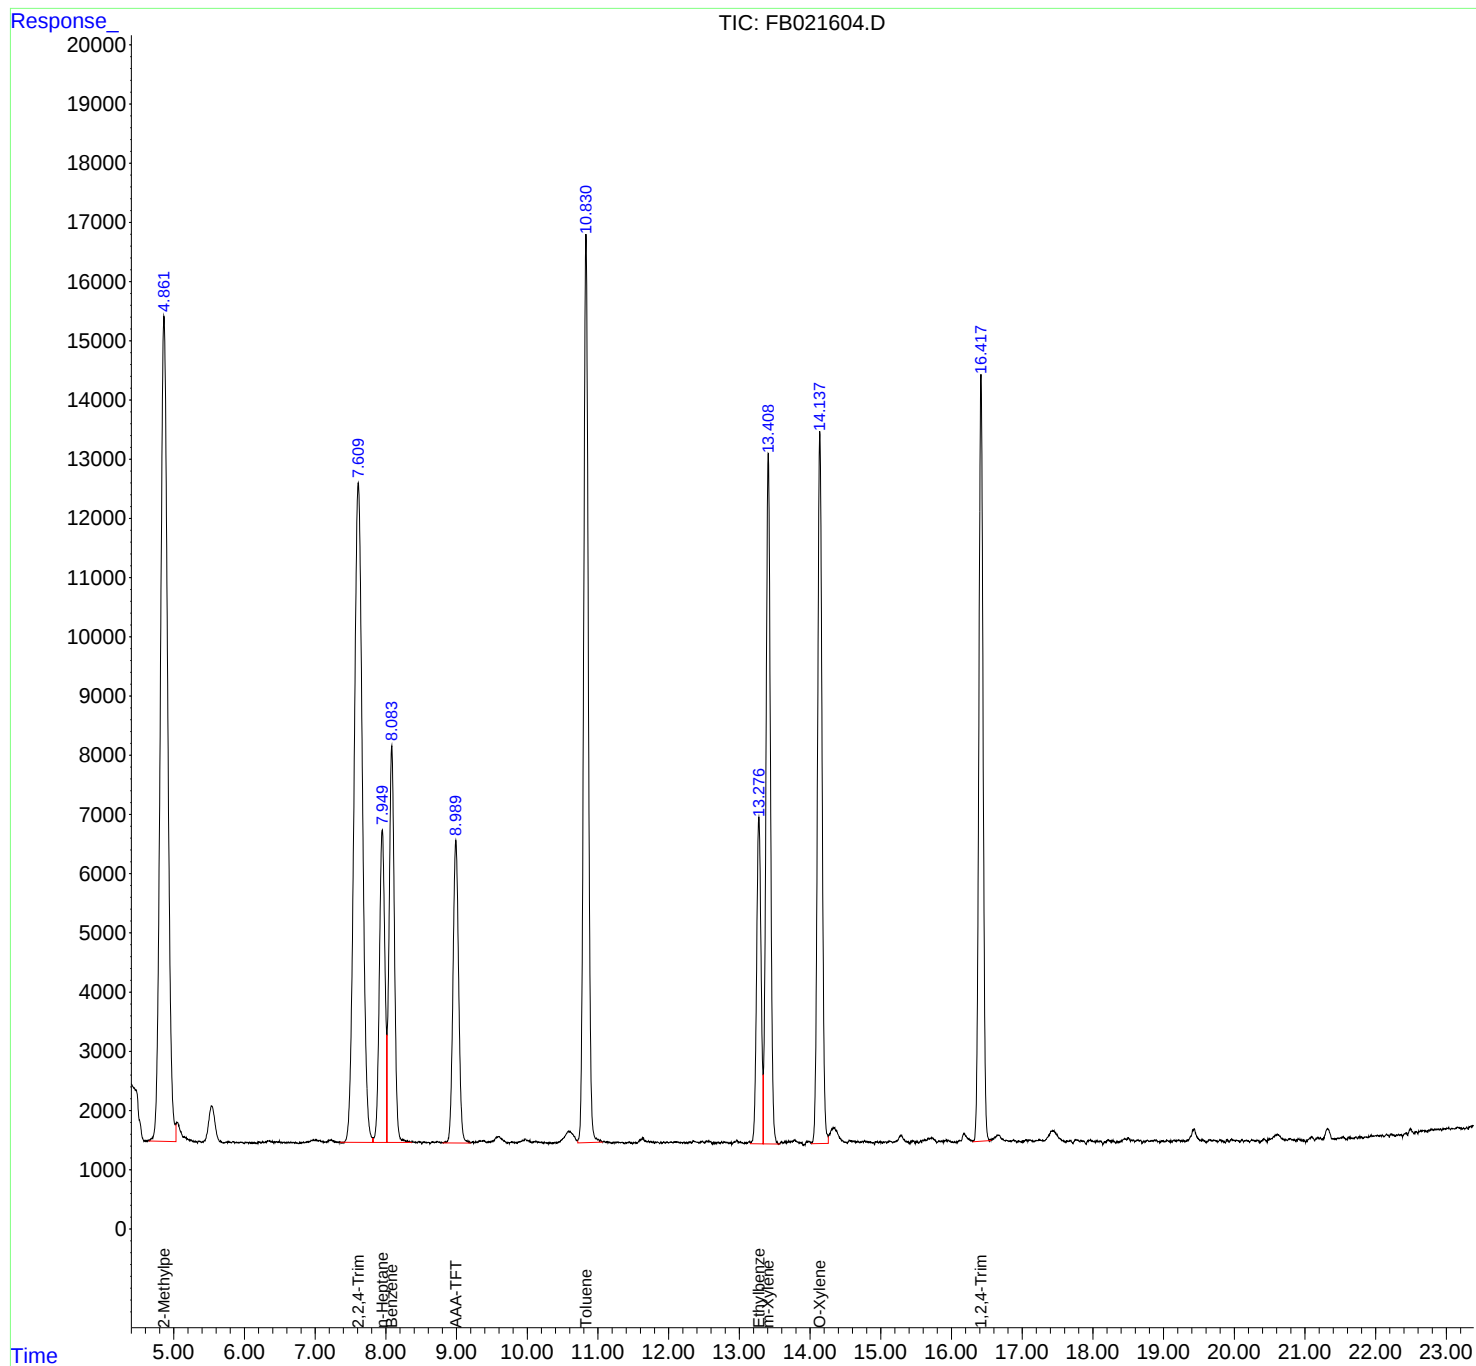


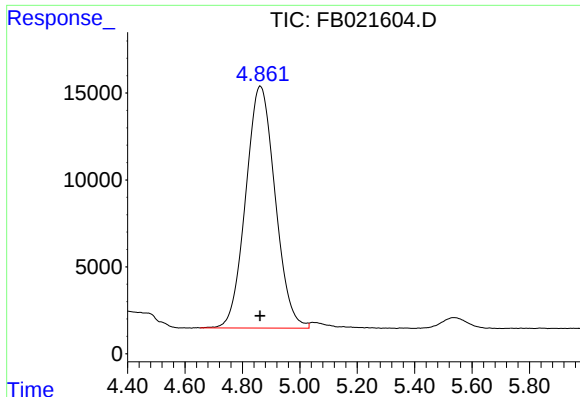

#1 2-Methylpentane


R.T.: 4.863 min
Delta R.T.: 0.002 min
Response: 991822
Conc: 29.05 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-01-062819MSD

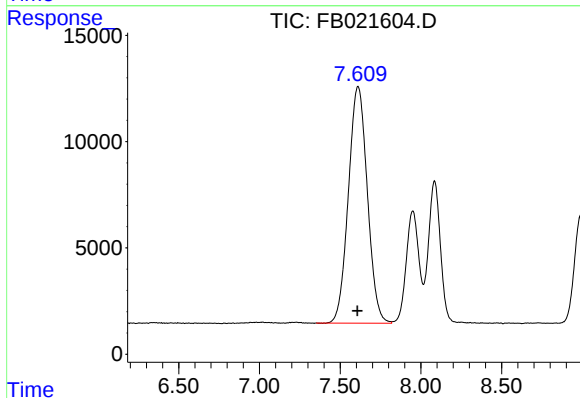


#2 2,2,4-Trimethylpentane

R.T.: 7.611 min
Delta R.T.: 0.003 min
Response: 909089
Conc: 29.42 ng/ml

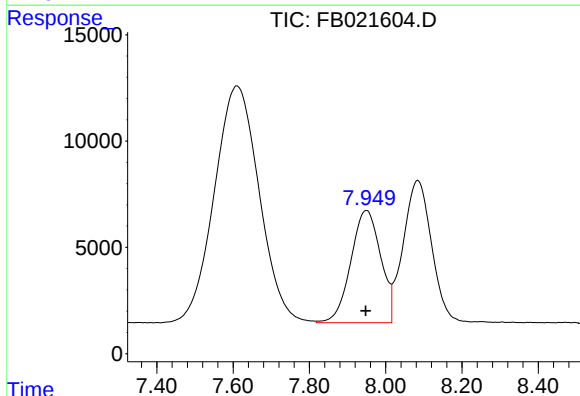


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: 0.002 min
Response: 286515
Conc: 9.79 ng/ml

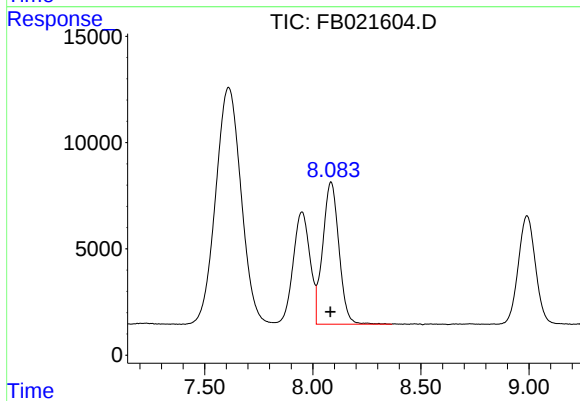

#4 Benzene


R.T.: 8.085 min
Delta R.T.: 0.002 min
Response: 347965
Conc: 10.37 ng/ml

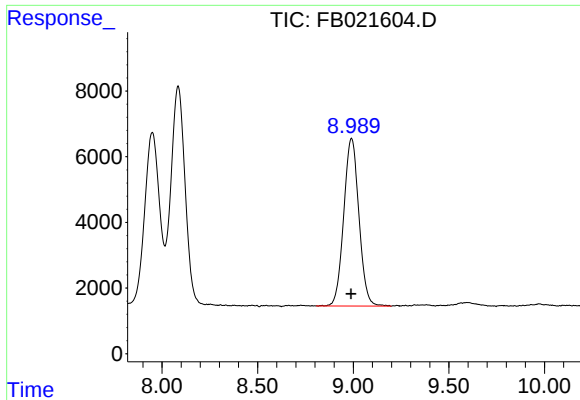

#5 AAA-TFT


R.T.: 8.991 min
 Delta R.T.: 0.002 min
 Response: 282697
 Conc: 20.45 ng/ml

Instrument :
 FID_B
 ClientSampleId :
 OK-01-062819MSD

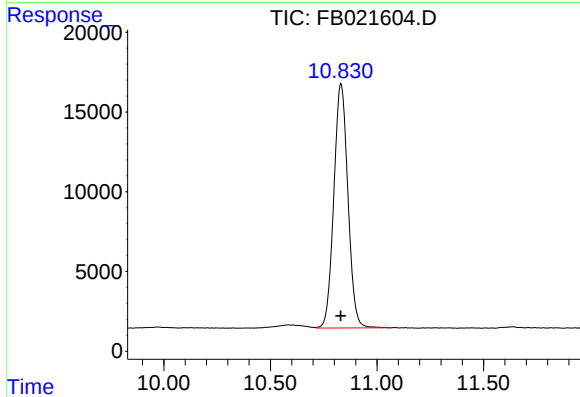


#6 Toluene

R.T.: 10.831 min
 Delta R.T.: 0.002 min
 Response: 703819
 Conc: 30.81 ng/ml

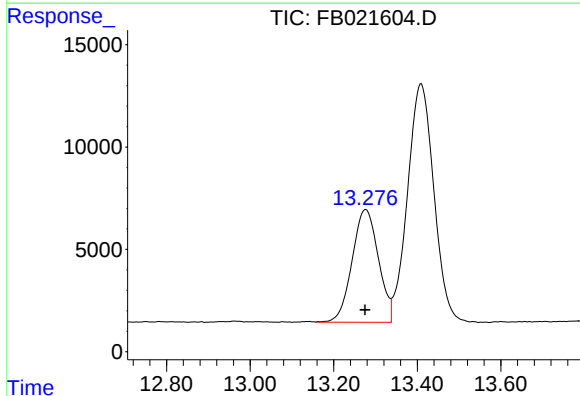


#7 Ethylbenzene

R.T.: 13.277 min
 Delta R.T.: 0.002 min
 Response: 240349
 Conc: 10.15 ng/ml

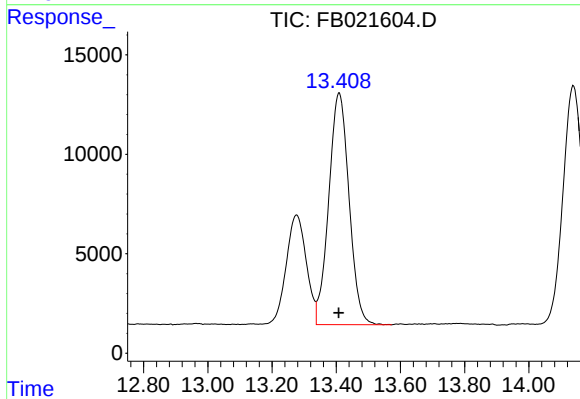

#8 m-Xylene


R.T.: 13.410 min
 Delta R.T.: 0.002 min
 Response: 511506
 Conc: 20.18 ng/ml

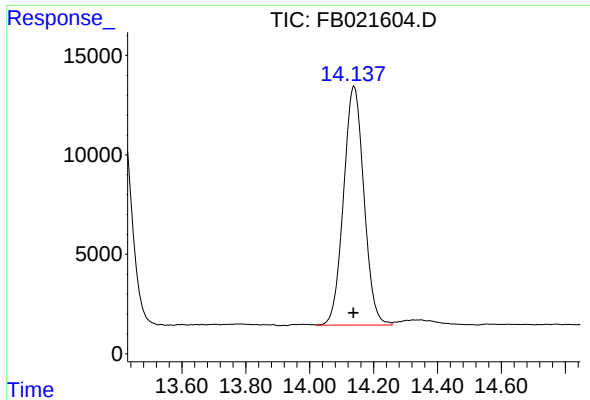

#9 O-Xylene

R.T.: 14.139 min
Delta R.T.: 0.001 min
Response: 531557
Conc: 20.27 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-01-062819MSD

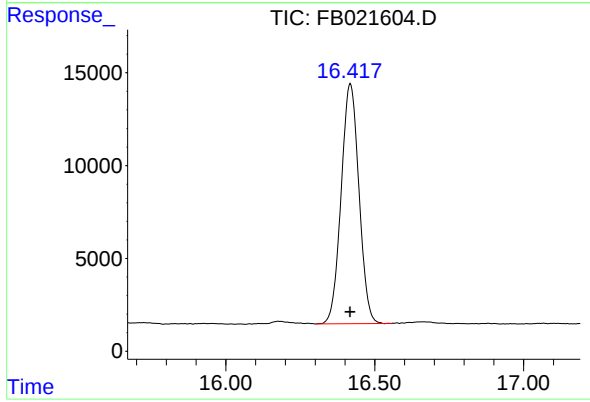

#10 1,2,4-Trimethylbenzene

R.T.: 16.418 min
Delta R.T.: 0.001 min
Response: 536827
Conc: 20.43 ng/ml