

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070119\
 Data File : FB021608.D
 Signal(s) : FID2B.CH
 Acq On : 1 Jul 2019 16:45
 Operator : MJ/SJ
 Sample : 20 PPB GRO STD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 PPB GRO STD

Integration File: Calibration.e
 Quant Time: Jul 02 00:44:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.989	286960	20.754 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.861	1004142	29.415 ng/ml
2) t 2,2,4-Trimethylpentane	7.609	937453	30.335 ng/ml
3) t n-Heptane	7.948	295422	10.094 ng/ml
4) t Benzene	8.083	344109	10.252 ng/ml
6) t Toluene	10.830	713908	31.253 ng/ml
7) t Ethylbenzene	13.275	247039	10.435 ng/ml
8) t m-Xylene	13.408	525262	20.724 ng/ml
9) t O-Xylene	14.138	542349	20.679 ng/ml
10) t 1,2,4-Trimethylbenzene	16.417	553810	21.078 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070119\
Data File : FB021608.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2019 16:45
Operator : MJ/SJ
Sample : 20 PPB GRO STD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

Integration File: Calibration.e
Quant Time: Jul 02 00:44:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

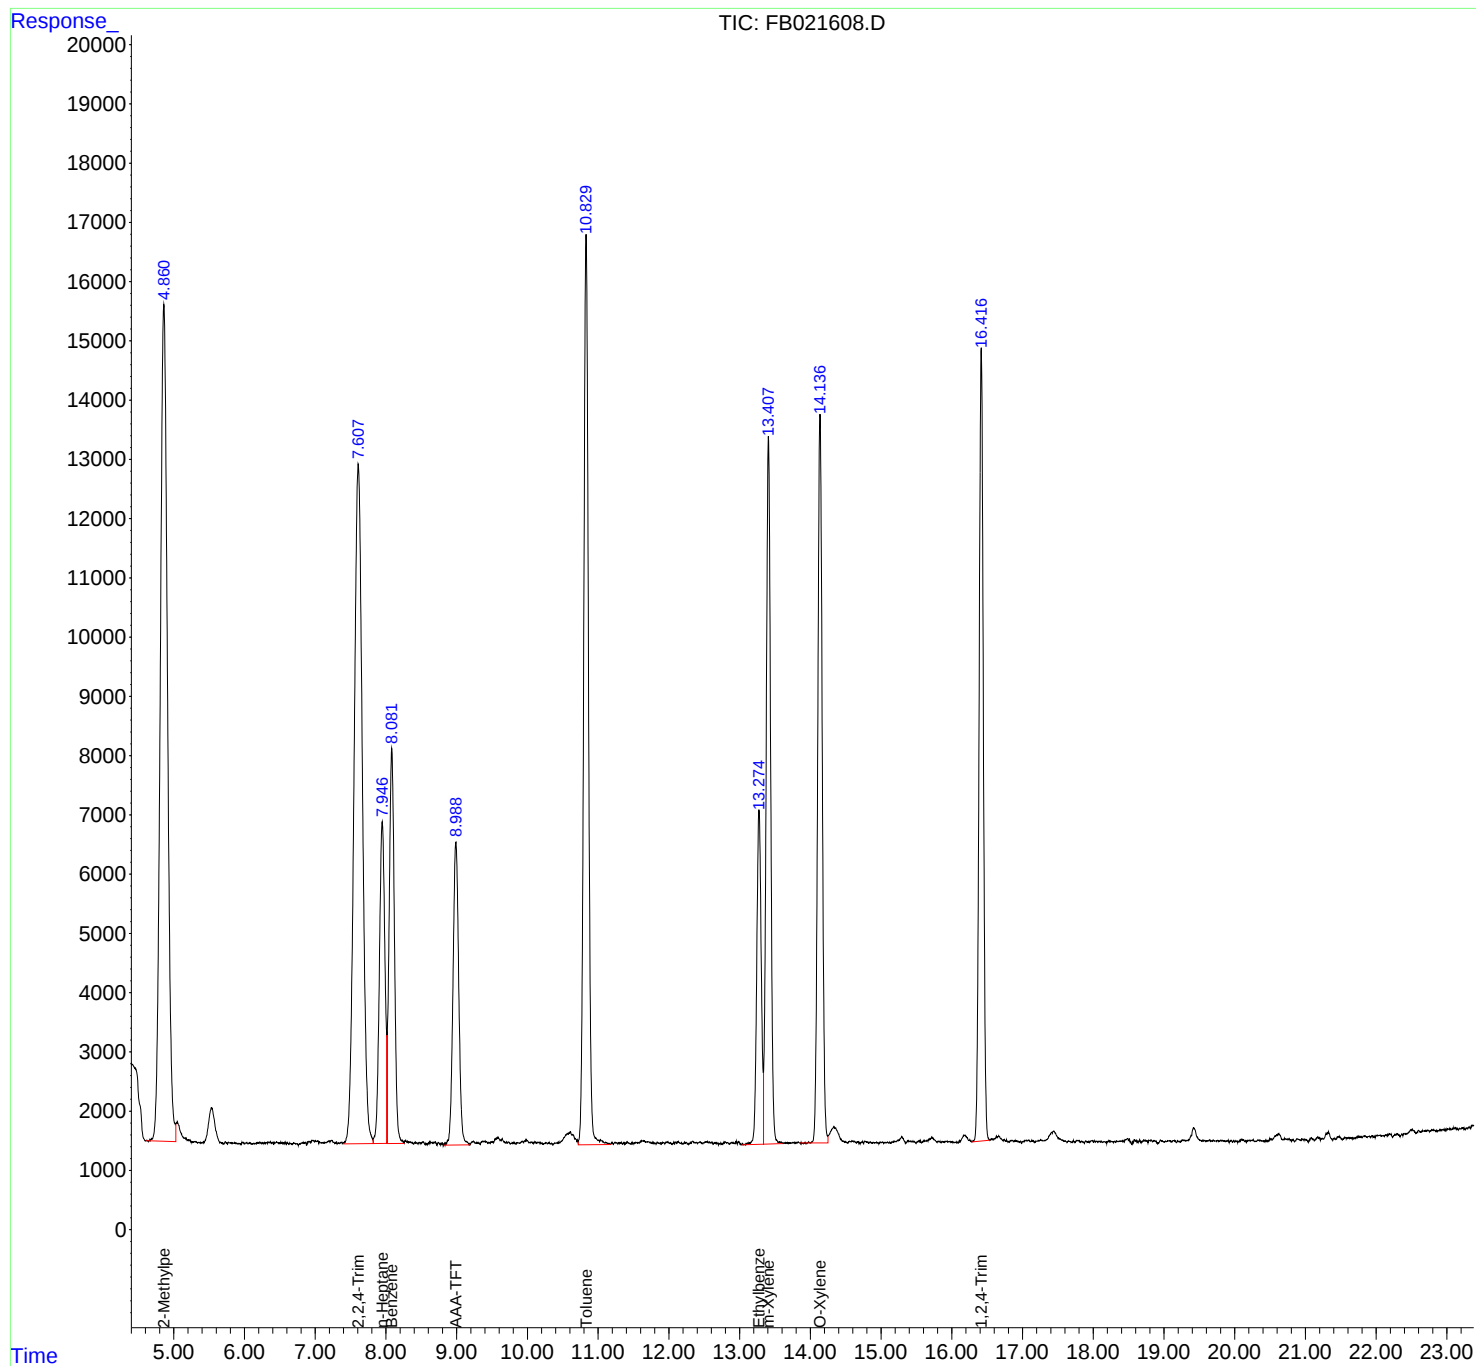


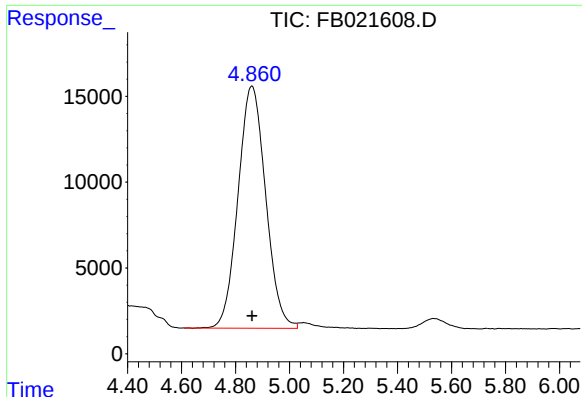

#1 2-Methylpentane


R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 1004142
Conc: 29.41 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

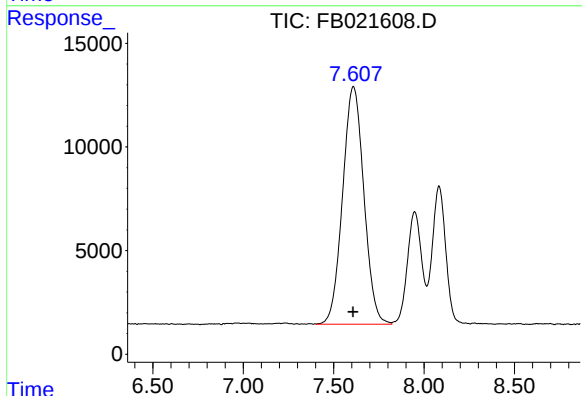


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: 0.001 min
Response: 937453
Conc: 30.34 ng/ml

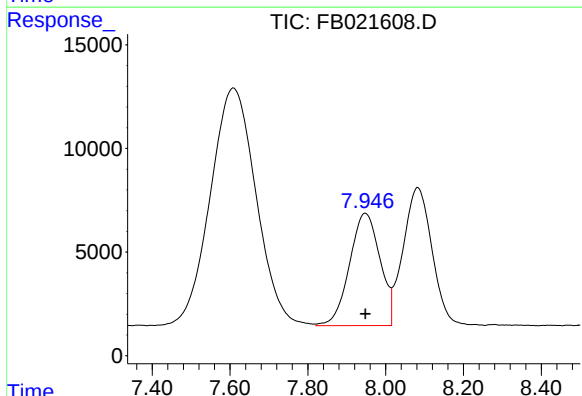


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: 0.000 min
Response: 295422
Conc: 10.09 ng/ml

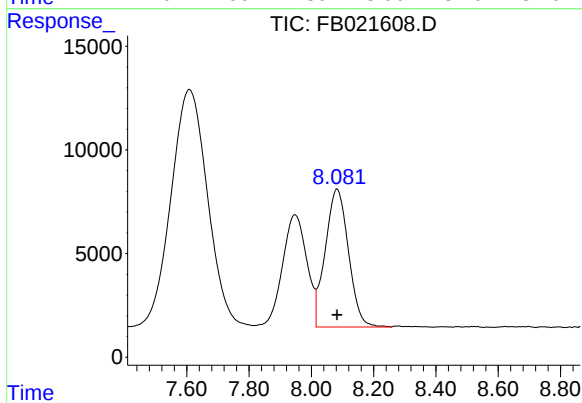

#4 Benzene


R.T.: 8.083 min
Delta R.T.: 0.000 min
Response: 344109
Conc: 10.25 ng/ml

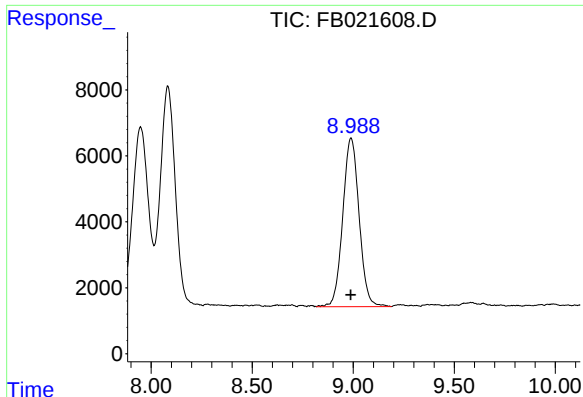

#5 AAA-TFT


R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 286960
Conc: 20.75 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

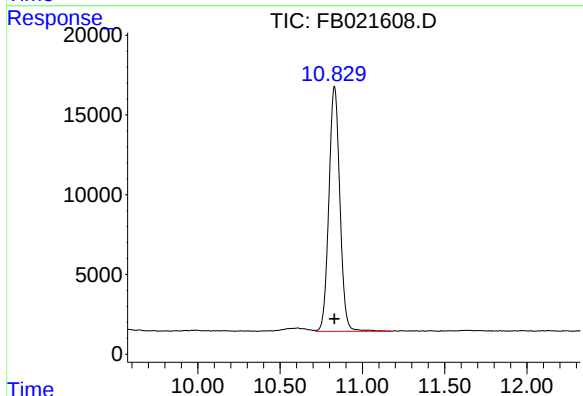


#6 Toluene

R.T.: 10.830 min
Delta R.T.: 0.000 min
Response: 713908
Conc: 31.25 ng/ml

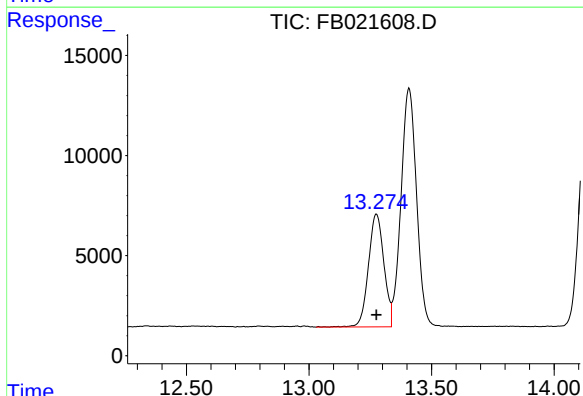


#7 Ethylbenzene

R.T.: 13.275 min
Delta R.T.: 0.000 min
Response: 247039
Conc: 10.44 ng/ml

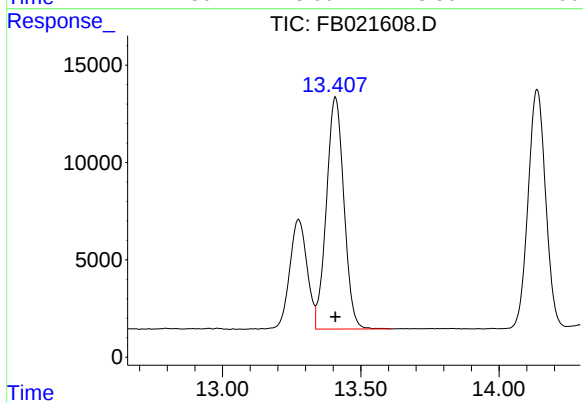

#8 m-Xylene


R.T.: 13.408 min
Delta R.T.: 0.000 min
Response: 525262
Conc: 20.72 ng/ml

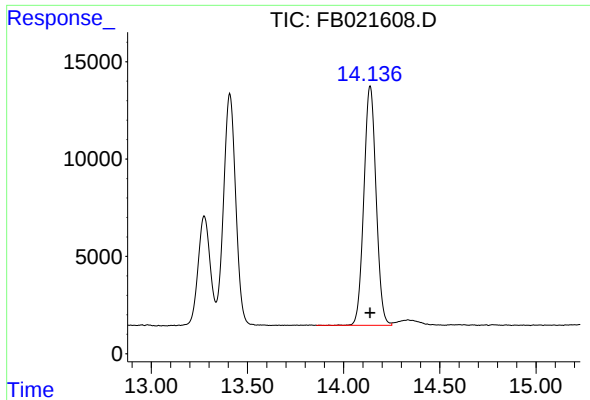

#9 O-Xylene

R.T.: 14.138 min
Delta R.T.: 0.000 min
Response: 542349
Conc: 20.68 ng/ml

Instrument :
FID_B
ClientSampleId :
20 PPB GRO STD

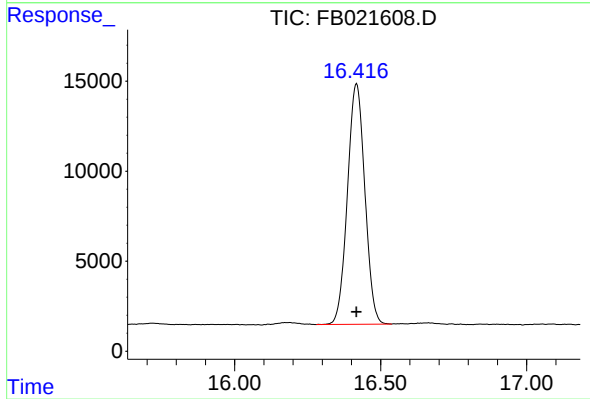

#10 1,2,4-Trimethylbenzene

R.T.: 16.417 min
Delta R.T.: 0.000 min
Response: 553810
Conc: 21.08 ng/ml