

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070119\
 Data File : FB021596.D
 Signal(s) : FID2B.CH
 Acq On : 1 Jul 2019 10:38
 Operator : MJ/SJ
 Sample : BSF0701S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0701S1

Integration File: Calibration.e
 Quant Time: Jul 02 00:42:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
 Quant Title :
 QLast Update : Mon Jun 24 16:18:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.987	261248	18.895 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.858	907581	26.586 ng/ml
2) t 2,2,4-Trimethylpentane	7.607	841255	27.222 ng/ml
3) t n-Heptane	7.945	264128	9.024 ng/ml
4) t Benzene	8.080	311161	9.271 ng/ml
6) t Toluene	10.828	664597	29.095 ng/ml
7) t Ethylbenzene	13.274	246752	10.423 ng/ml
8) t m-Xylene	13.407	531703	20.978 ng/ml
9) t O-Xylene	14.136	546073	20.821 ng/ml
10) t 1,2,4-Trimethylbenzene	16.416	549263	20.905 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070119\
Data File : FB021596.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2019 10:38
Operator : MJ/SJ
Sample : BSF0701S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0701S1

Integration File: Calibration.e
Quant Time: Jul 02 00:42:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062419.M
Quant Title :
QLast Update : Mon Jun 24 16:18:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

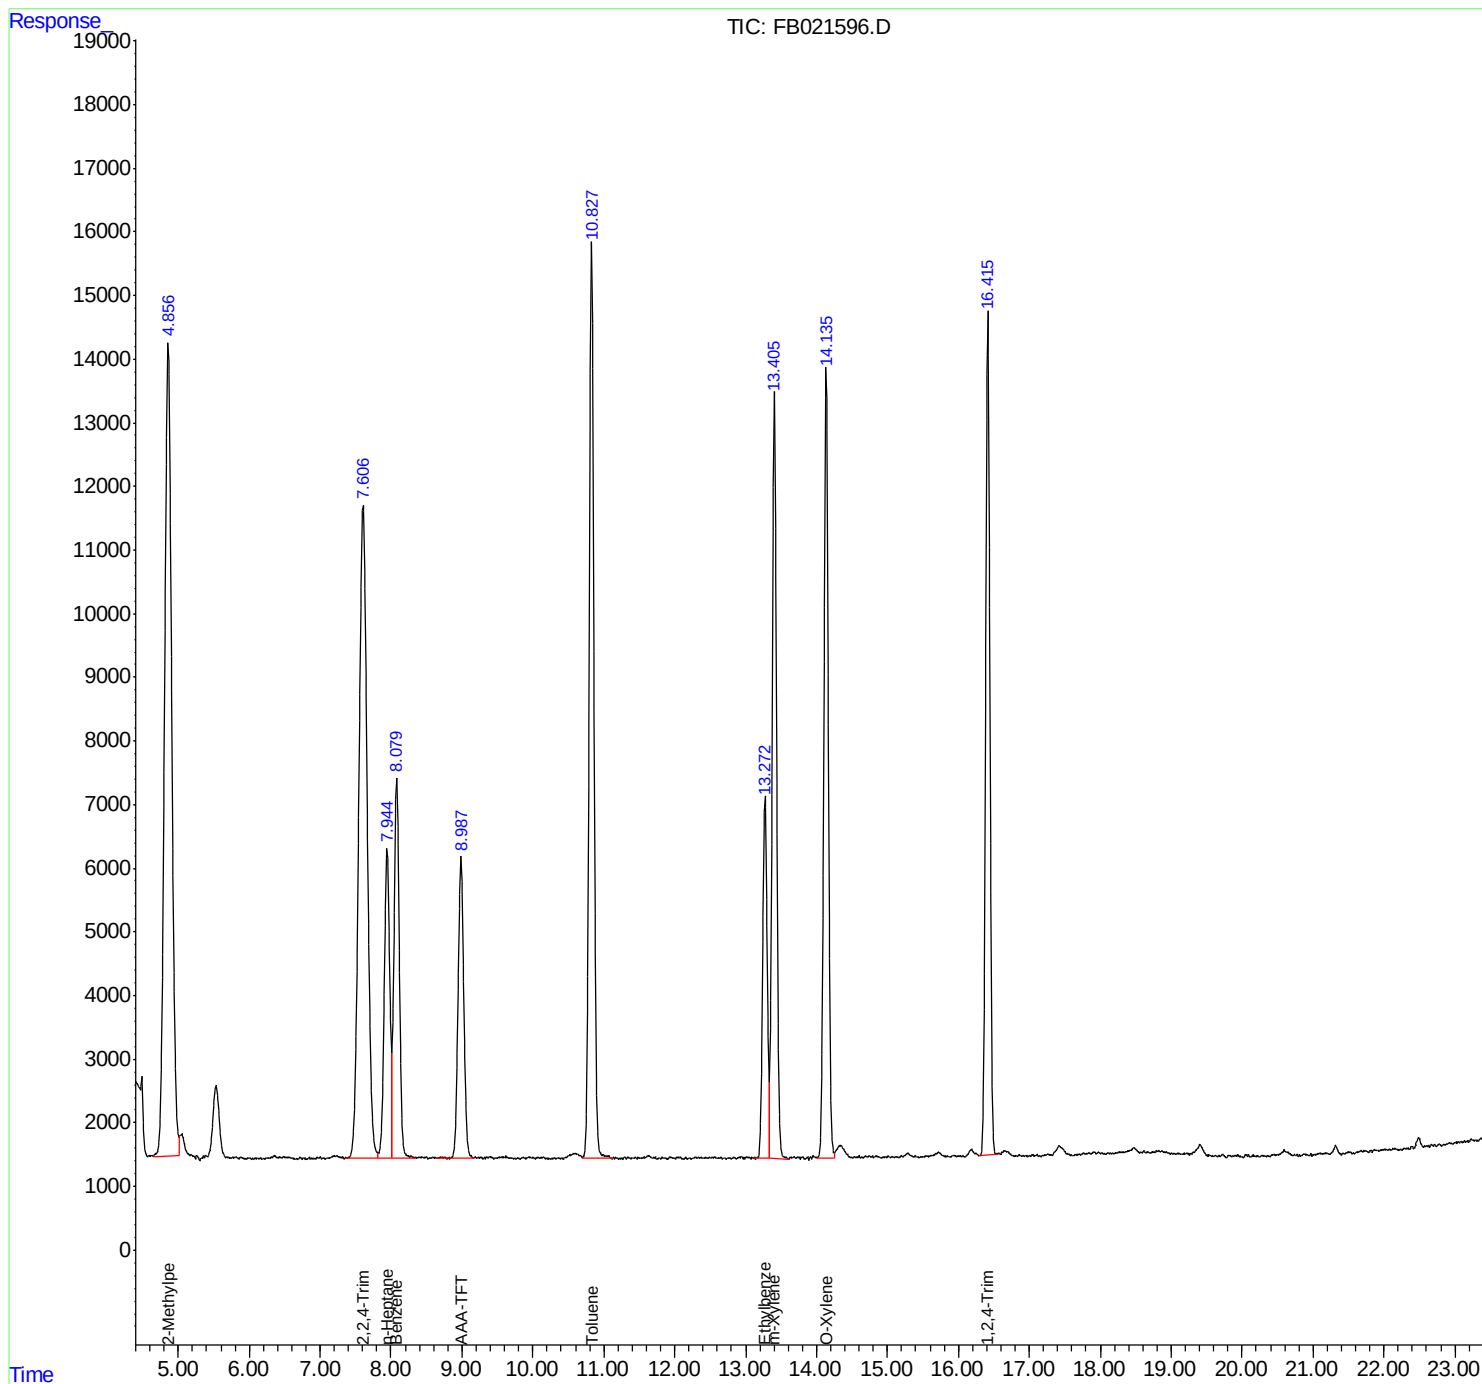


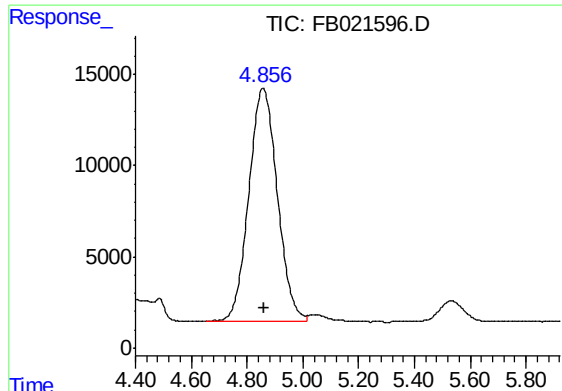

#1 2-Methylpentane


R.T.: 4.858 min
Delta R.T.: -0.003 min
Response: 907581
Conc: 26.59 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S1

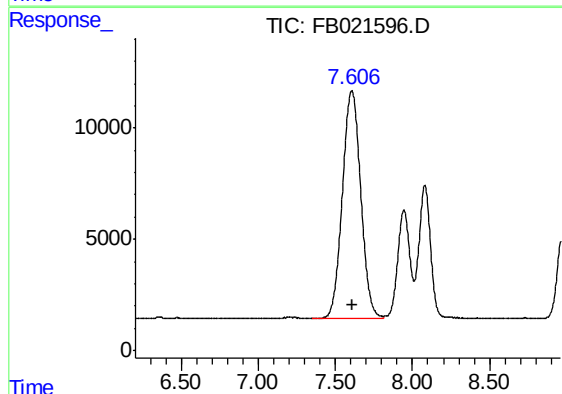


#2 2,2,4-Trimethylpentane

R.T.: 7.607 min
Delta R.T.: 0.000 min
Response: 841255
Conc: 27.22 ng/ml

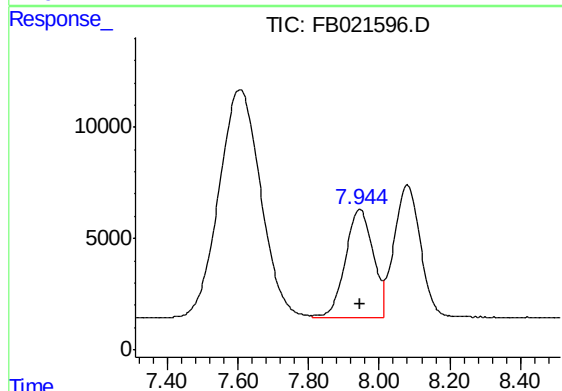


#3 n-Heptane

R.T.: 7.945 min
Delta R.T.: -0.003 min
Response: 264128
Conc: 9.02 ng/ml

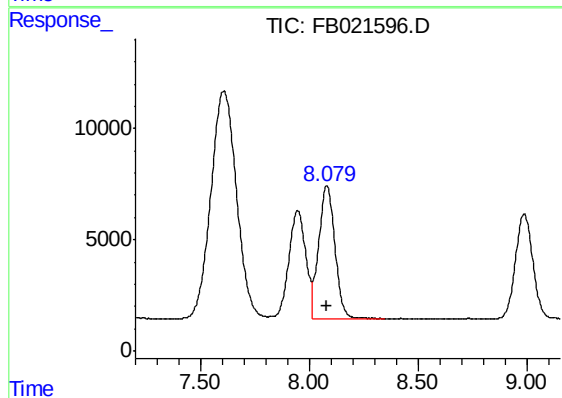

#4 Benzene


R.T.: 8.080 min
Delta R.T.: -0.002 min
Response: 311161
Conc: 9.27 ng/ml

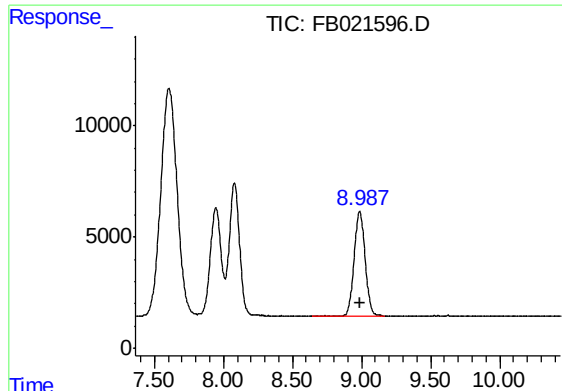

#5 AAA-TFT


R.T.: 8.987 min
Delta R.T.: -0.002 min
Response: 261248
Conc: 18.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S1

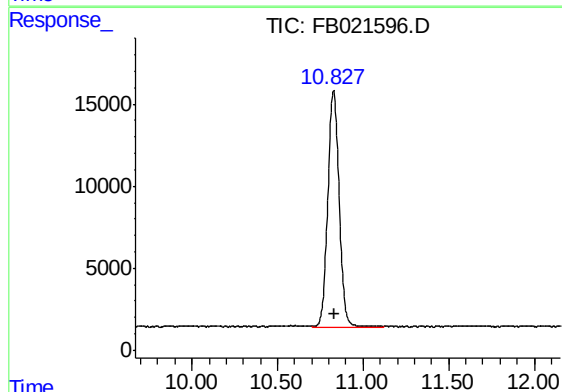


#6 Toluene

R.T.: 10.828 min
Delta R.T.: -0.001 min
Response: 664597
Conc: 29.09 ng/ml

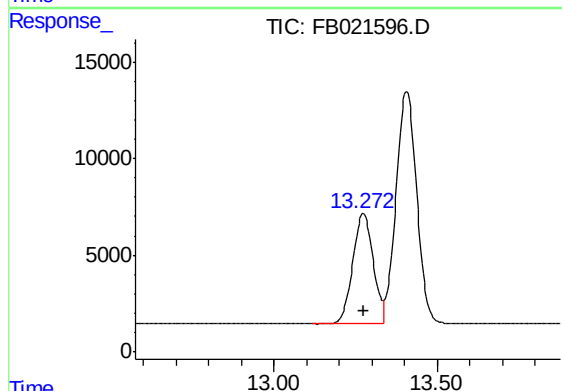


#7 Ethylbenzene

R.T.: 13.274 min
Delta R.T.: -0.001 min
Response: 246752
Conc: 10.42 ng/ml

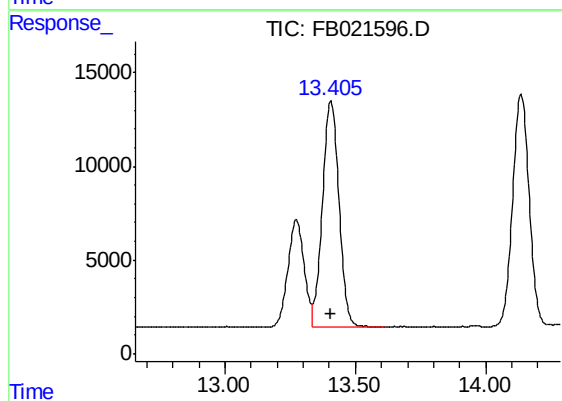

#8 m-Xylene


R.T.: 13.407 min
Delta R.T.: -0.001 min
Response: 531703
Conc: 20.98 ng/ml

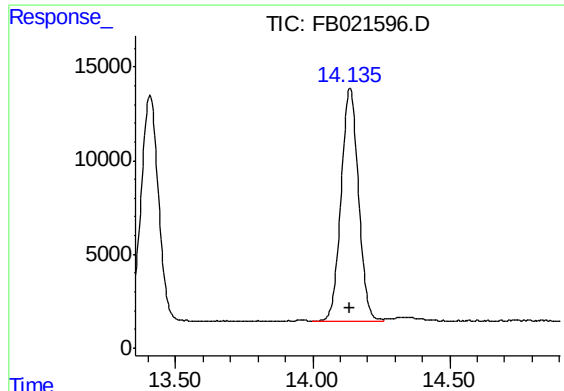

#9 O-Xylene

R.T.: 14.136 min
Delta R.T.: -0.001 min
Response: 546073
Conc: 20.82 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S1

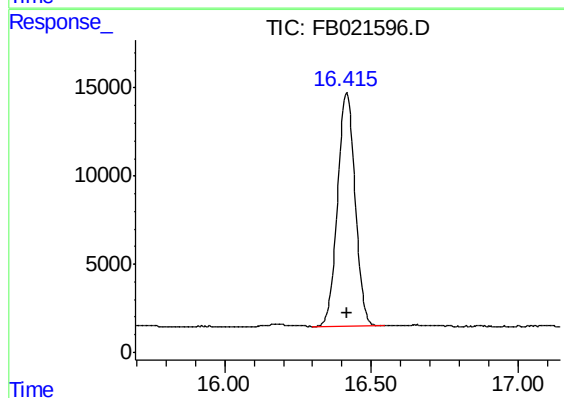

#10 1,2,4-Trimethylbenzene

R.T.: 16.416 min
Delta R.T.: -0.001 min
Response: 549263
Conc: 20.91 ng/ml