

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070120\
 Data File : FB024522.D
 Signal(s) : FID2B.CH
 Acq On : 1 Jul 2020 10:02
 Operator : DD/AJ
 Sample : VBF0701S1
 Misc : 5.00gm/5.00ml DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 VBF0701S1

Integration File: Calibration.e
 Quant Time: Jul 02 01:03:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	490015	20.253 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.684	1046	0.033 ng/ml
2) t 2,2,4-Trimethylpentane	7.432	185	0.006 ng/ml
6) t Toluene	10.639	6100	0.155 ng/ml
7) t Ethylbenzene	13.080	1774	0.051 ng/ml
8) t m-Xylene	13.199	1393	0.041 ng/ml
9) t o-Xylene	13.933	5420	0.162 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	4886	0.176 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070120\
Data File : FB024522.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2020 10:02
Operator : DD/AJ
Sample : VBF0701S1
Misc : 5.00gm/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0701S1

Integration File: Calibration.e
Quant Time: Jul 02 01:03:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

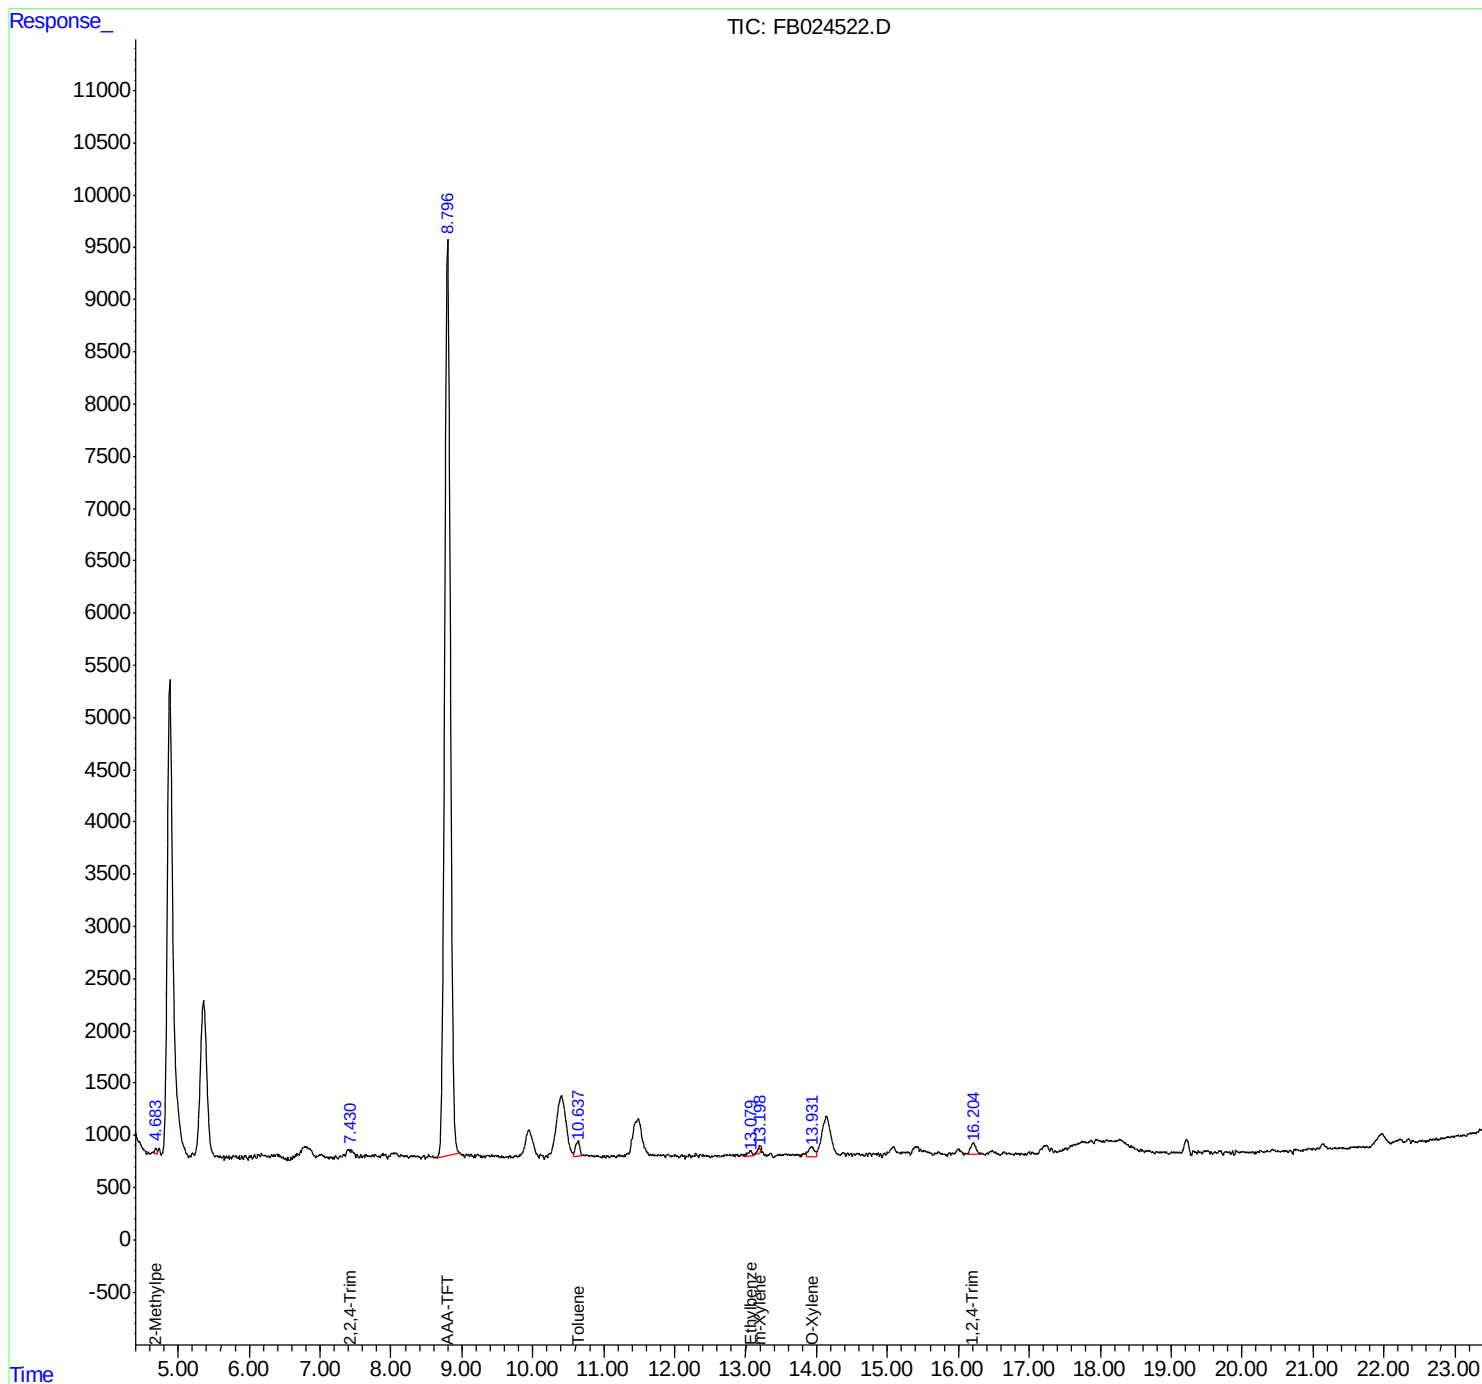


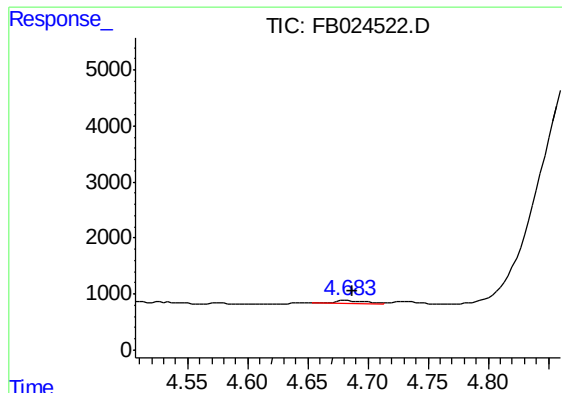

#1 2-Methylpentane


R.T.: 4.684 min
Delta R.T.: -0.003 min
Response: 1046
Conc: 0.03 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0701S1

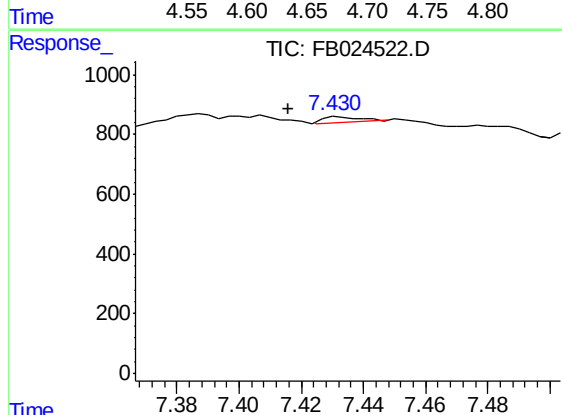


#2 2,2,4-Trimethylpentane

R.T.: 7.432 min
Delta R.T.: 0.016 min
Response: 185
Conc: 0.01 ng/ml

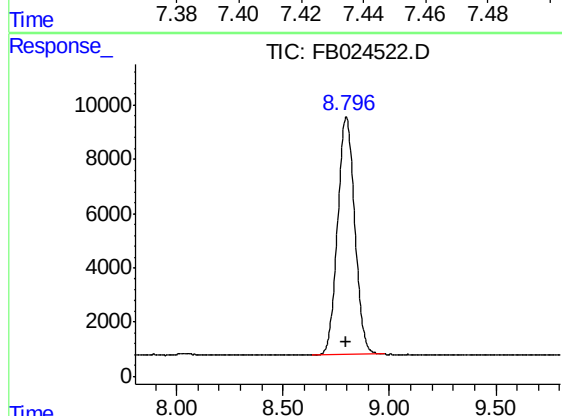


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 490015
Conc: 20.25 ng/ml

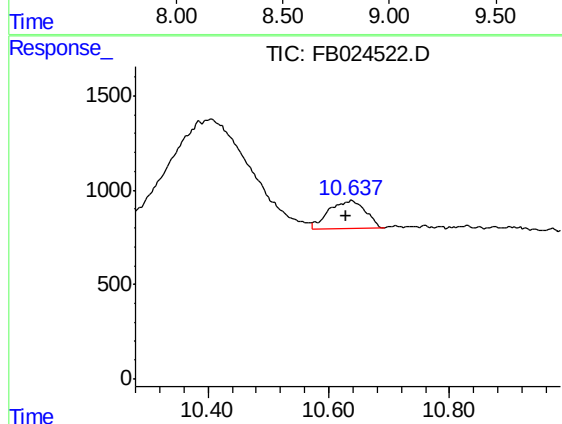

#6 Toluene


R.T.: 10.639 min
Delta R.T.: 0.011 min
Response: 6100
Conc: 0.16 ng/ml

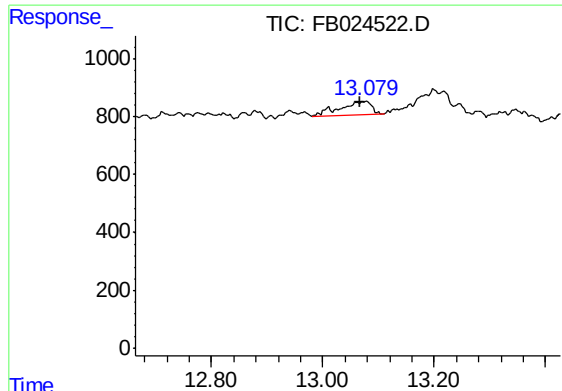

#7 Ethylbenzene


R.T.: 13.080 min
Delta R.T.: 0.012 min
Response: 1774
Conc: 0.05 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0701S1

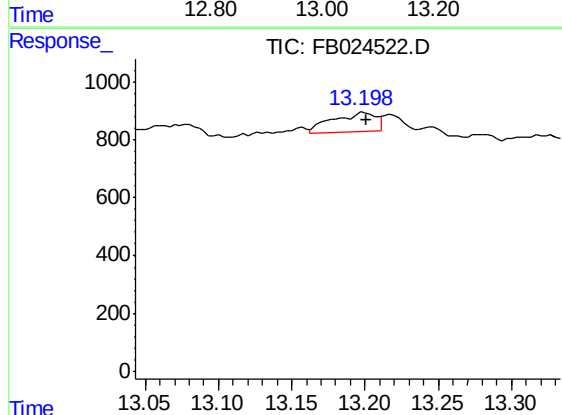


#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: -0.002 min
Response: 1393
Conc: 0.04 ng/ml

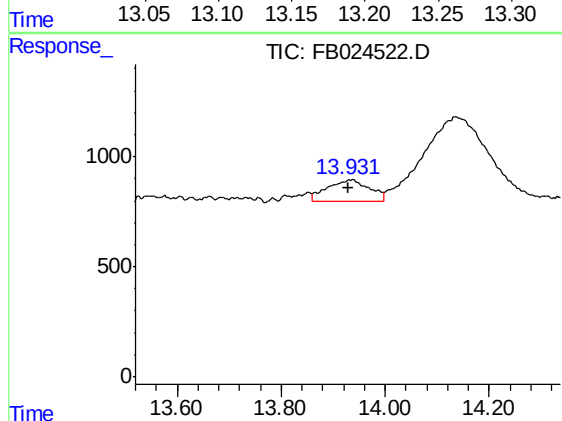

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.004 min
Response: 5420
Conc: 0.16 ng/ml

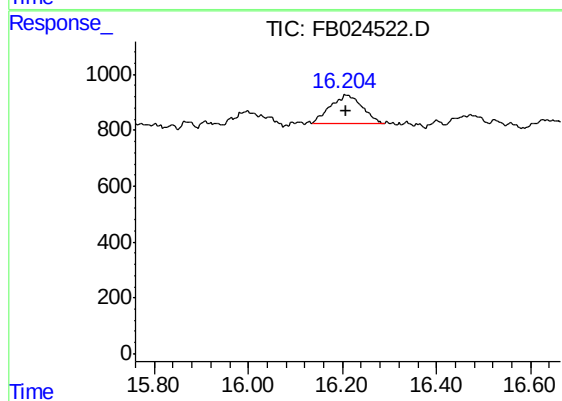

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: 0.000 min
Response: 4886
Conc: 0.18 ng/ml