

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070120\
 Data File : FB024523.D
 Signal(s) : FID2B.CH
 Acq On : 1 Jul 2020 10:32
 Operator : DD/AJ
 Sample : BSF0701S1
 Misc : 5.01gm/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0701S1

Integration File: Calibration.e
 Quant Time: Jul 02 01:03:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	526524	21.762 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	995401	31.142 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	1081204	32.252 ng/ml
3) t n-Heptane	7.757	355112	10.501 ng/ml
4) t Benzene	7.890	423891	10.486 ng/ml
6) t Toluene	10.629	1208706	30.757 ng/ml
7) t Ethylbenzene	13.070	367527	10.474 ng/ml
8) t m-Xylene	13.202	722394	21.094 ng/ml
9) t O-Xylene	13.930	707611	21.106 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	589867	21.245 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070120\
Data File : FB024523.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2020 10:32
Operator : DD/AJ
Sample : BSF0701S1
Misc : 5.01gm/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0701S1

Integration File: Calibration.e
Quant Time: Jul 02 01:03:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

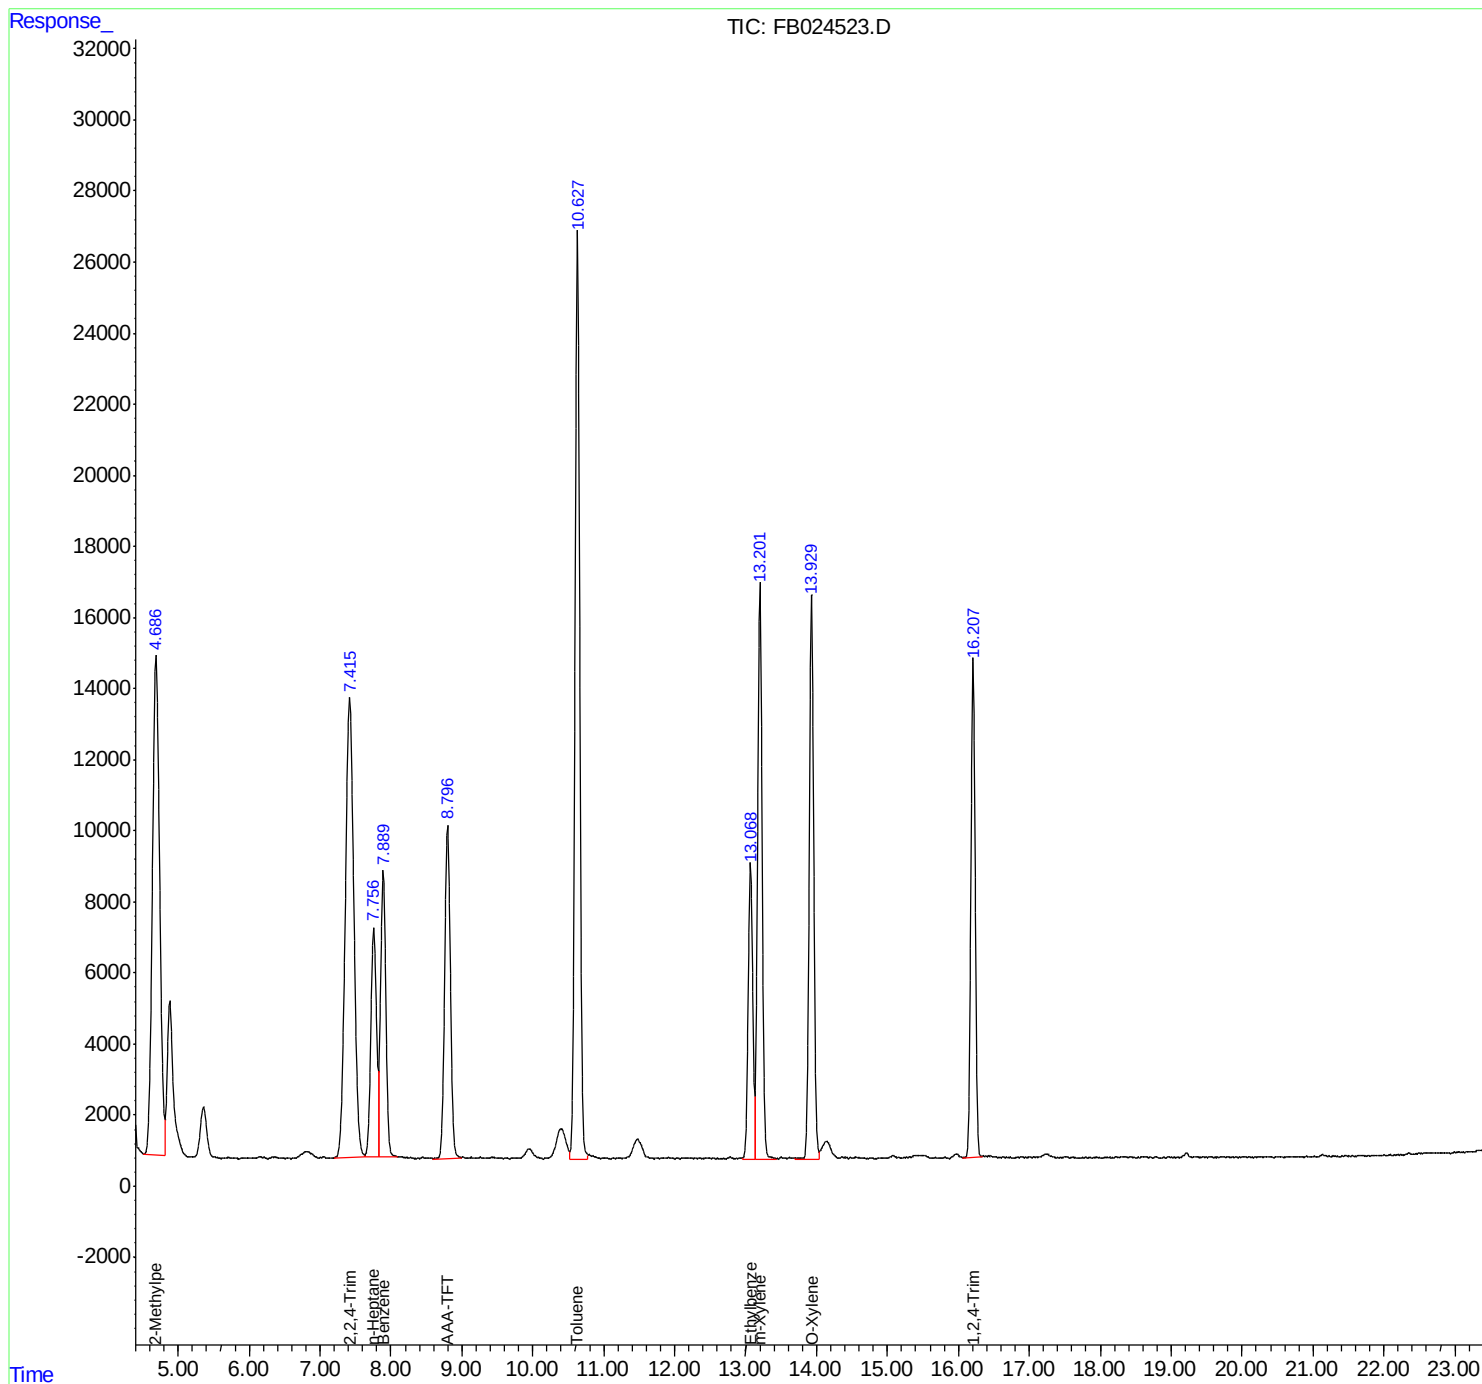


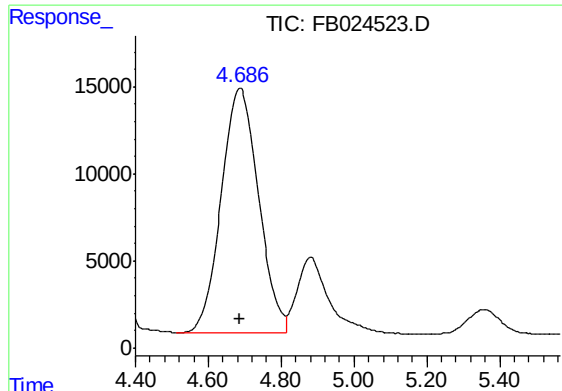

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 995401
Conc: 31.14 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S1

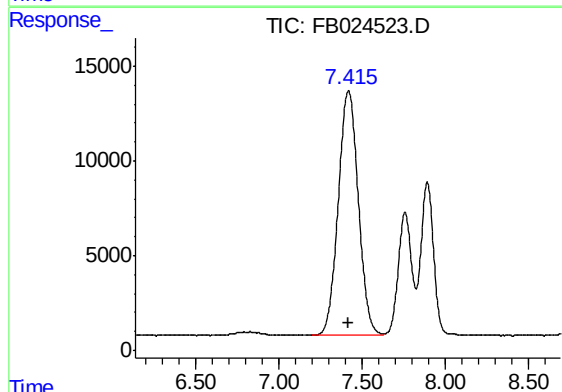


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.001 min
Response: 1081204
Conc: 32.25 ng/ml

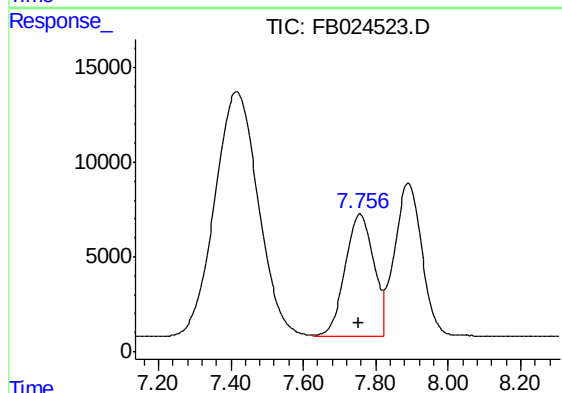


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.002 min
Response: 355112
Conc: 10.50 ng/ml

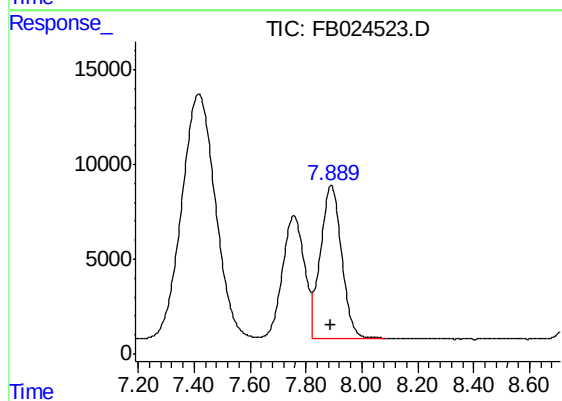

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.000 min
Response: 423891
Conc: 10.49 ng/ml

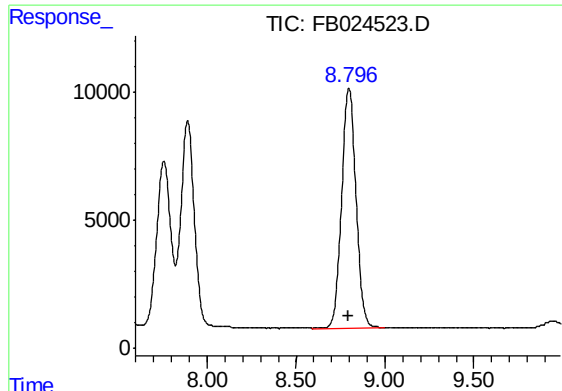

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.000 min
Response: 526524
Conc: 21.76 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S1

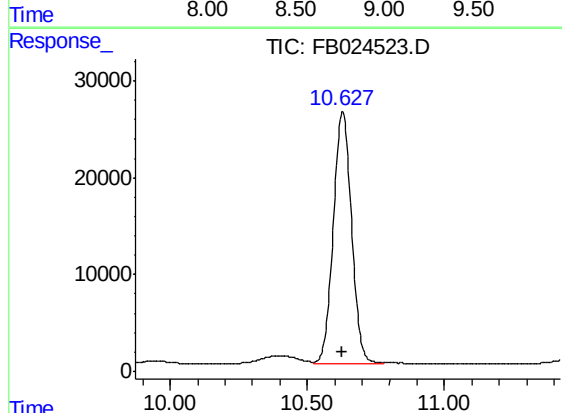


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.000 min
Response: 1208706
Conc: 30.76 ng/ml

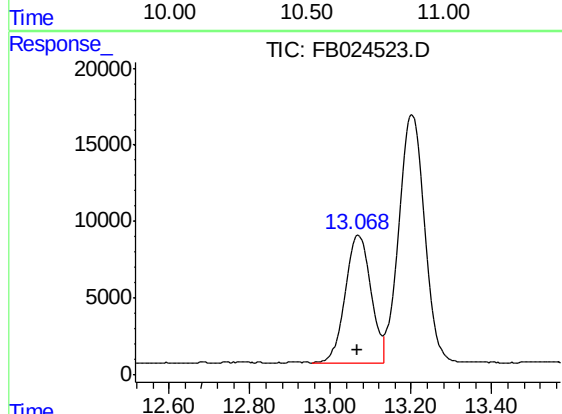


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: 0.002 min
Response: 367527
Conc: 10.47 ng/ml

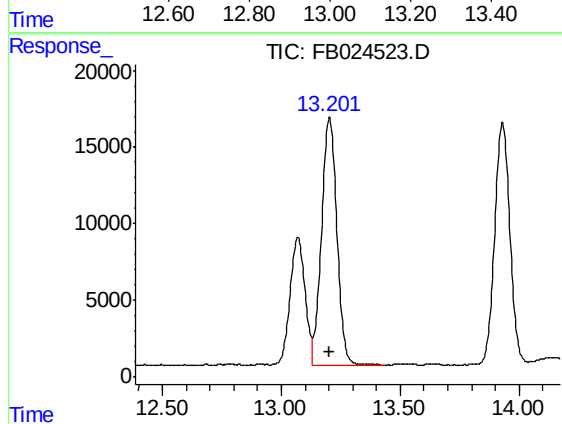

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: 0.001 min
Response: 722394
Conc: 21.09 ng/ml

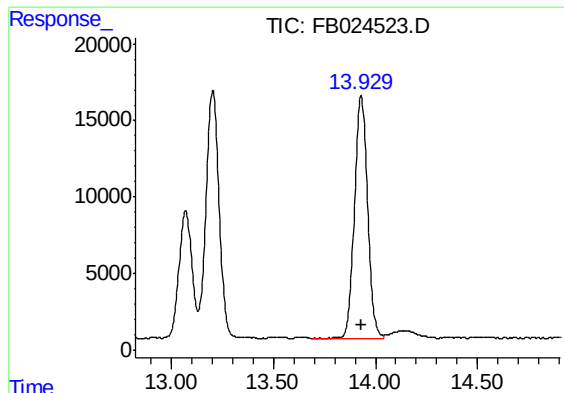

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.001 min
Response: 707611
Conc: 21.11 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S1

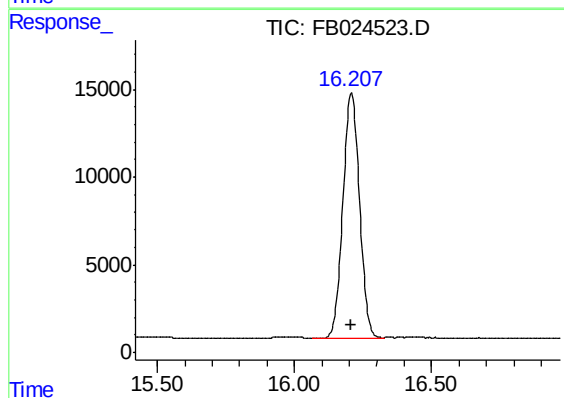

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.001 min
Response: 589867
Conc: 21.24 ng/ml