

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070120\
 Data File : FB024527.D
 Signal(s) : FID2B.CH
 Acq On : 1 Jul 2020 12:35
 Operator : DD/AJ
 Sample : L2814-15MS
 Misc : 5.01gm/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 PL-02-063020MS

Integration File: Calibration.e
 Quant Time: Jul 02 01:04:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	541918	22.399 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	862942	26.998 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	842122	25.120 ng/ml
3) t n-Heptane	7.759	278442	8.234 ng/ml
4) t Benzene	7.894	406500	10.056 ng/ml
6) t Toluene	10.631	1135134	28.885 ng/ml
7) t Ethylbenzene	13.071	344566	9.819 ng/ml
8) t m-Xylene	13.204	665806	19.442 ng/ml
9) t O-Xylene	13.932	650432	19.401 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	526751	18.971 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070120\
Data File : FB024527.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2020 12:35
Operator : DD/AJ
Sample : L2814-15MS
Misc : 5.01gm/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
PL-02-063020MS

Integration File: Calibration.e
Quant Time: Jul 02 01:04:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

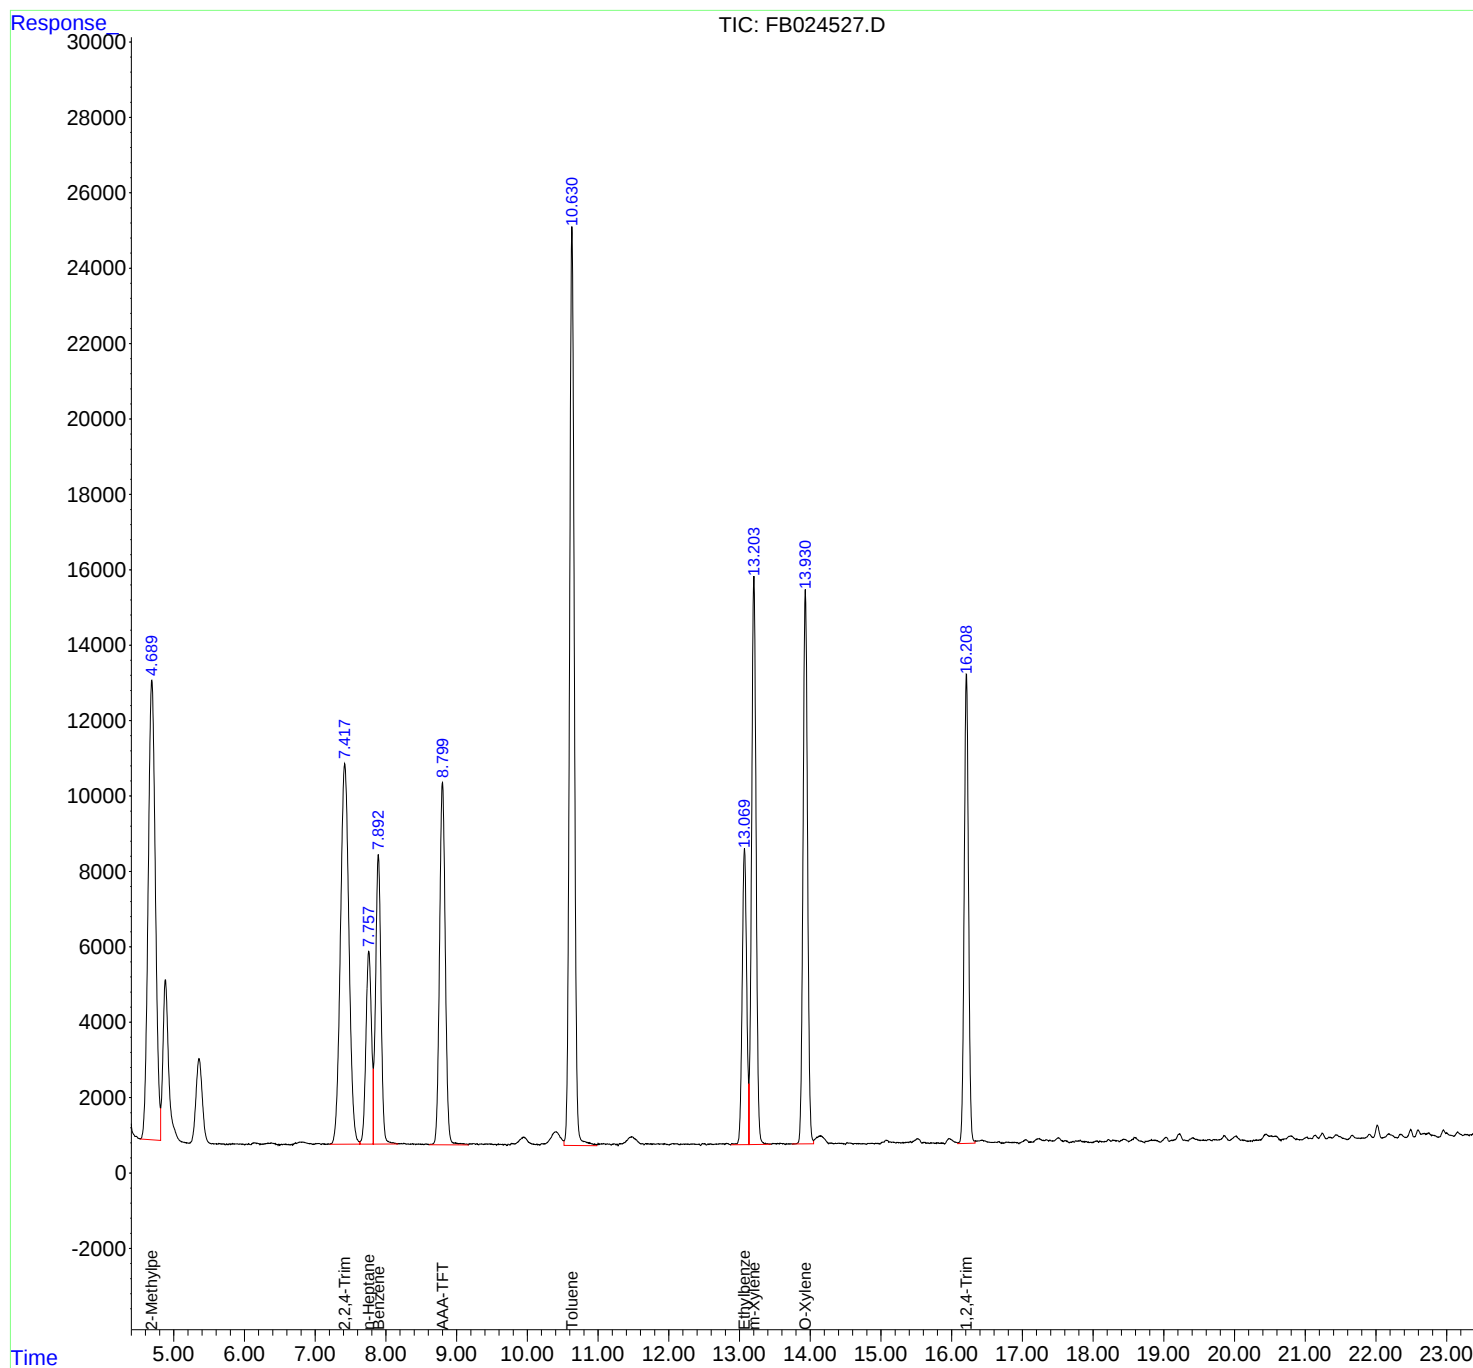


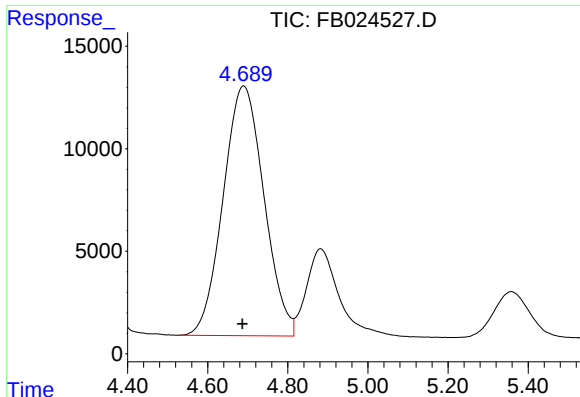

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: 0.003 min
Response: 862942
Conc: 27.00 ng/ml

Instrument :
FID_B
ClientSampleId :
PL-02-063020MS

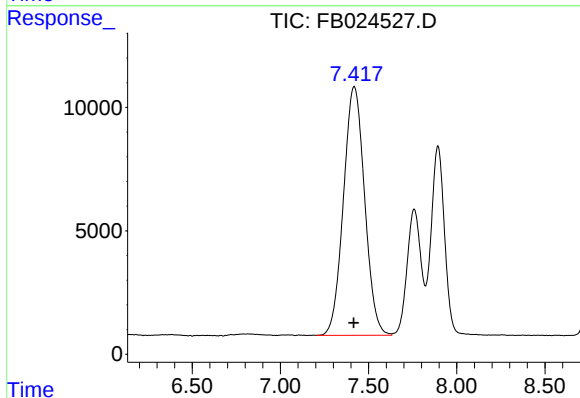


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.002 min
Response: 842122
Conc: 25.12 ng/ml

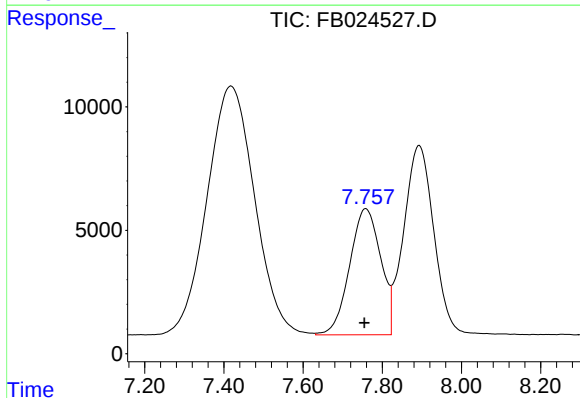


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.004 min
Response: 278442
Conc: 8.23 ng/ml

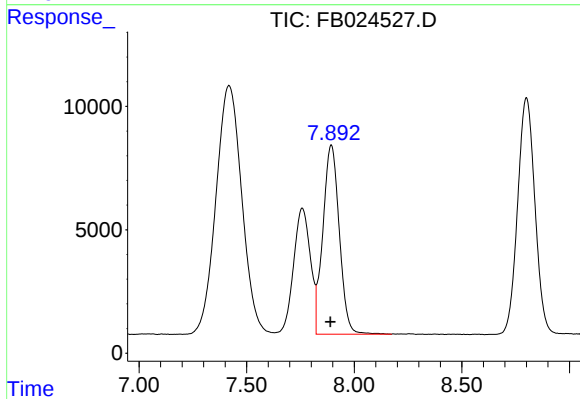

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.004 min
Response: 406500
Conc: 10.06 ng/ml

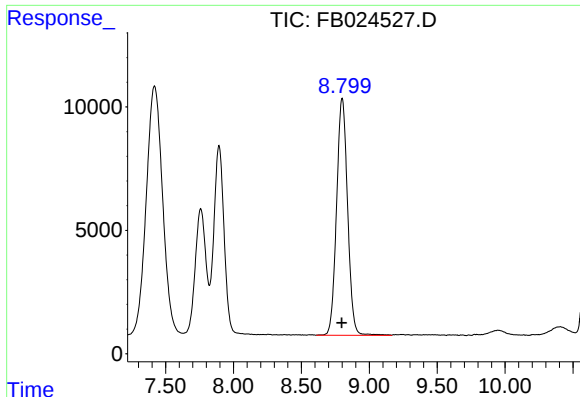

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.003 min
Response: 541918
Conc: 22.40 ng/ml

Instrument :
FID_B
ClientSampleId :
PL-02-063020MS

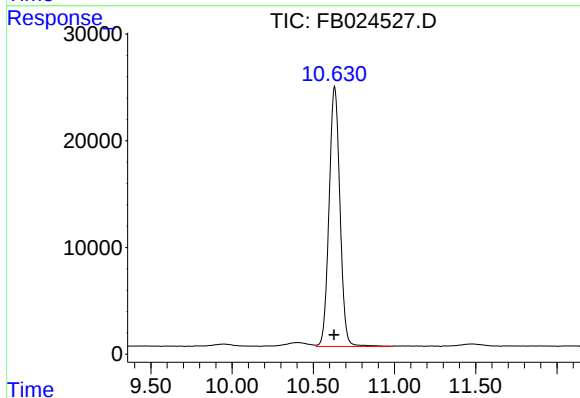


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.003 min
Response: 1135134
Conc: 28.89 ng/ml

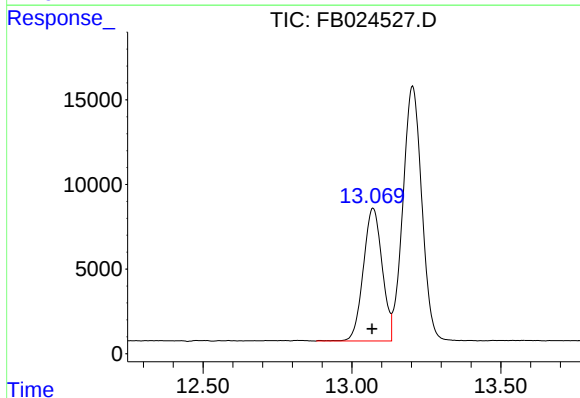


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.003 min
Response: 344566
Conc: 9.82 ng/ml

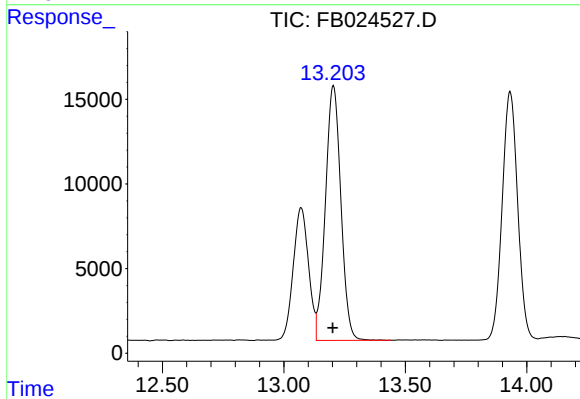

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.003 min
Response: 665806
Conc: 19.44 ng/ml

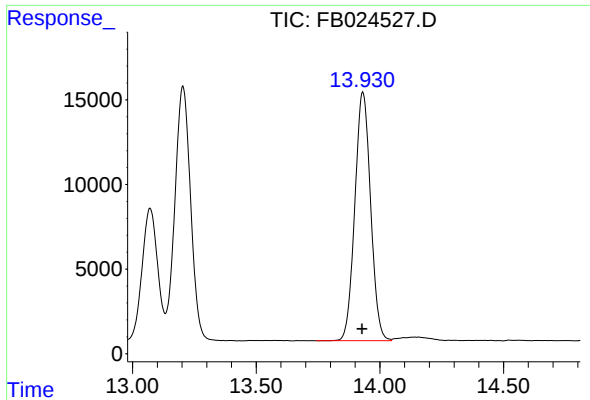

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.003 min
Response: 650432
Conc: 19.40 ng/ml

Instrument :
FID_B
ClientSampleId :
PL-02-063020MS

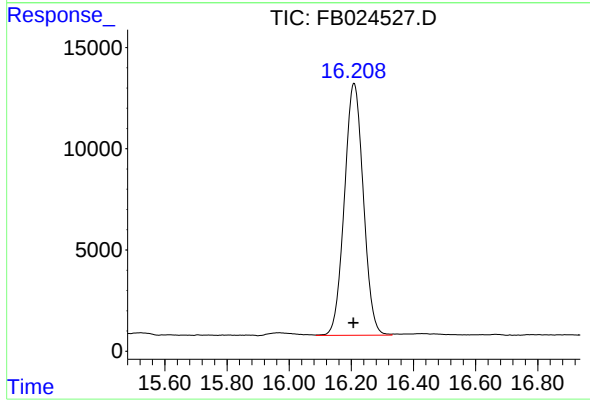

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.003 min
Response: 526751
Conc: 18.97 ng/ml