

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070120\
 Data File : FB024528.D
 Signal(s) : FID2B.CH
 Acq On : 1 Jul 2020 13:06
 Operator : DD/AJ
 Sample : L2814-15MSD
 Misc : 5.03gm/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 PL-02-063020MSD

Integration File: Calibration.e
 Quant Time: Jul 02 01:04:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
 Quant Title :
 QLast Update : Tue Jun 09 11:17:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	486329	20.101 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	727205	22.751 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	723658	21.586 ng/ml
3) t n-Heptane	7.759	237209	7.014 ng/ml
4) t Benzene	7.892	360722	8.923 ng/ml
6) t Toluene	10.631	957752	24.371 ng/ml
7) t Ethylbenzene	13.071	272965	7.779 ng/ml
8) t m-Xylene	13.204	530451	15.489 ng/ml
9) t O-Xylene	13.931	530592	15.826 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	412332	14.851 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


```
Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070120\  
Data File : FB024528.D  
Signal(s) : FID2B.CH  
Acq On    : 1 Jul 2020 13:06  
Operator  : DD/AJ  
Sample    : L2814-15MSD  
Misc      : 5.03gm/5.00ml DI WATER  
ALS Vial  : 8 Sample Multiplier: 1
```

Instrument :
FID_B
ClientSampleId :
PL-02-063020MSD

Integration File: Calibration.e
Quant Time: Jul 02 01:04:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060920.M
Quant Title :
QLast Update : Tue Jun 09 11:17:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

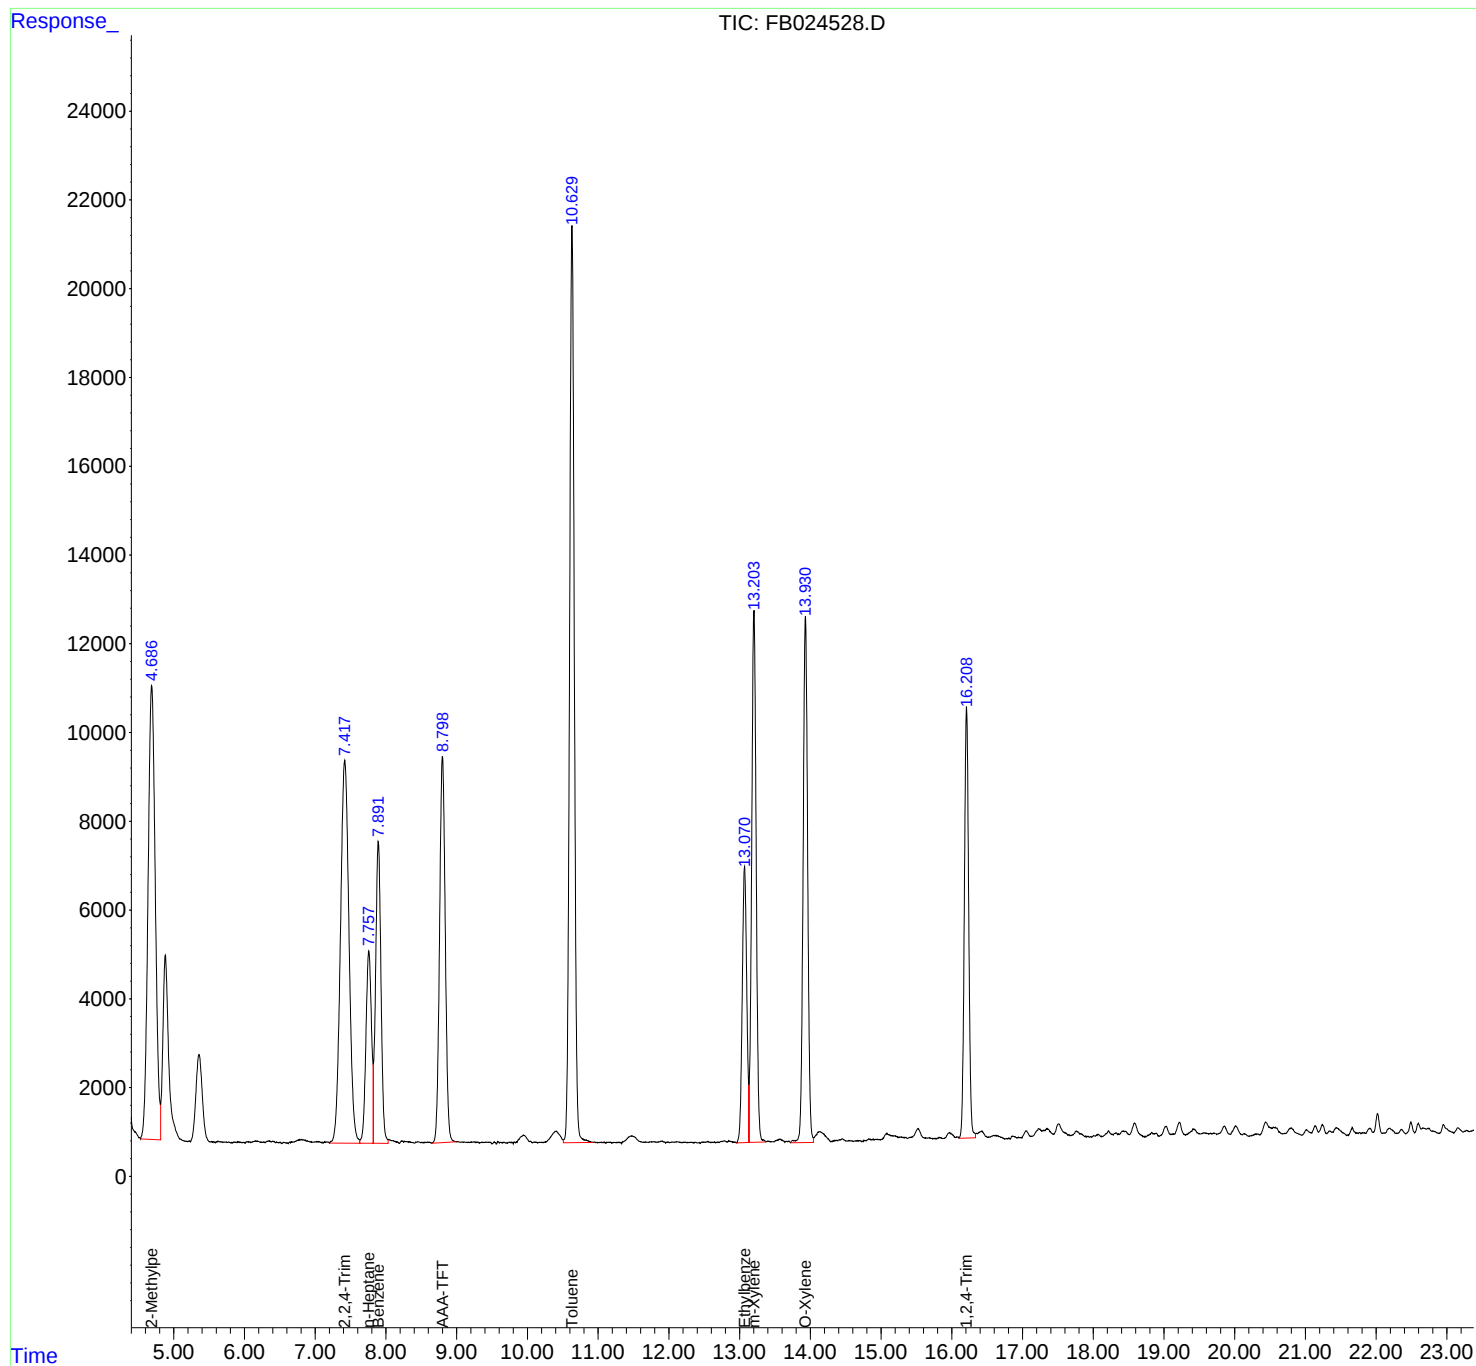


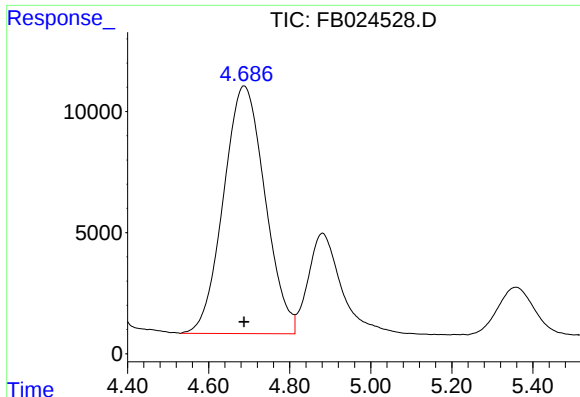

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 727205
Conc: 22.75 ng/ml

Instrument :
FID_B
ClientSampleId :
PL-02-063020MSD

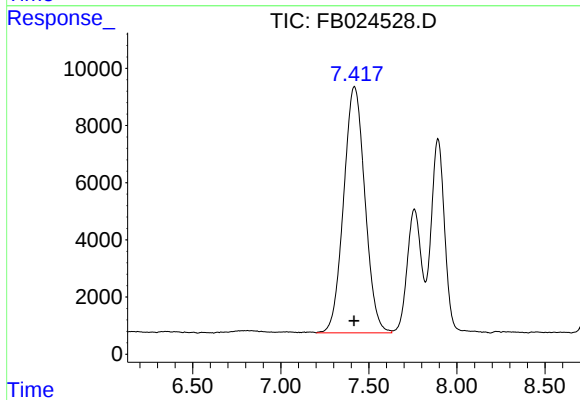


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.002 min
Response: 723658
Conc: 21.59 ng/ml

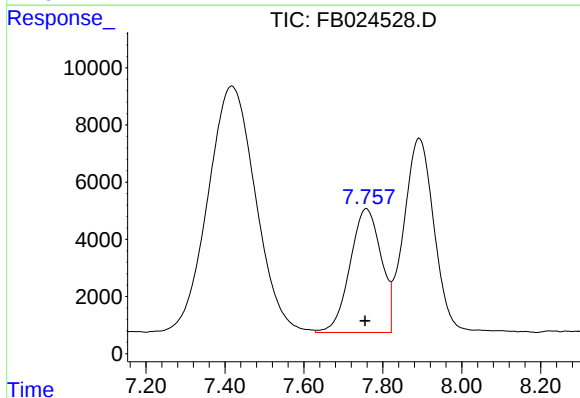


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.004 min
Response: 237209
Conc: 7.01 ng/ml

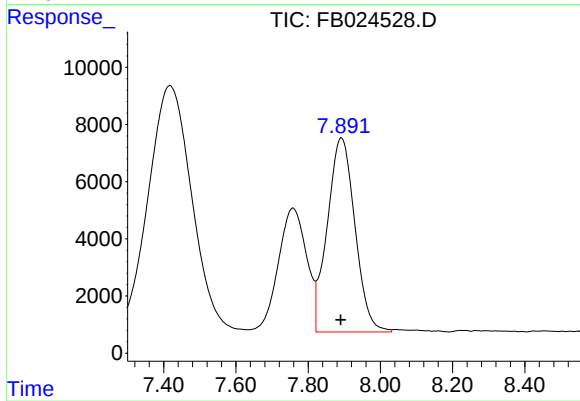

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.002 min
Response: 360722
Conc: 8.92 ng/ml

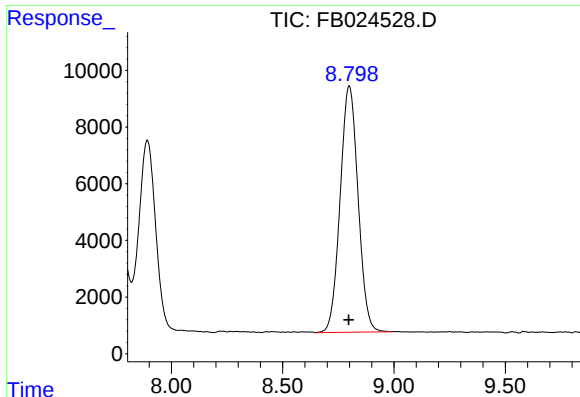

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.003 min
Response: 486329
Conc: 20.10 ng/ml

Instrument :
FID_B
ClientSampleId :
PL-02-063020MSD

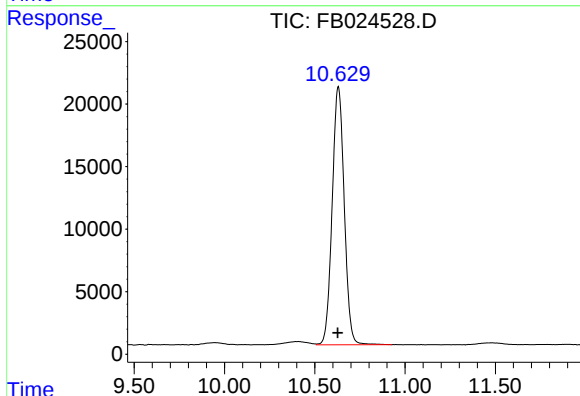


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.003 min
Response: 957752
Conc: 24.37 ng/ml

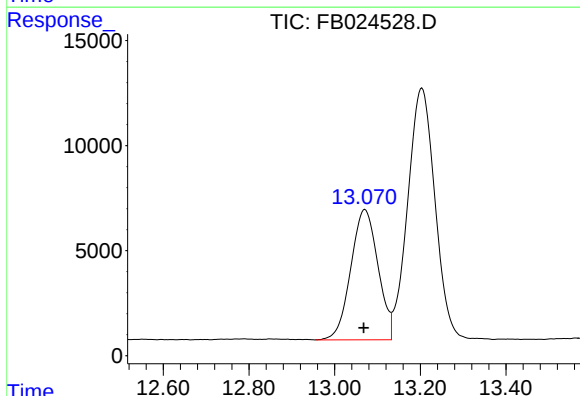


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.003 min
Response: 272965
Conc: 7.78 ng/ml

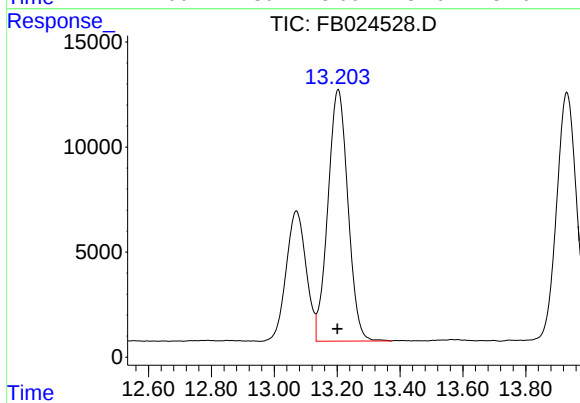

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.003 min
Response: 530451
Conc: 15.49 ng/ml

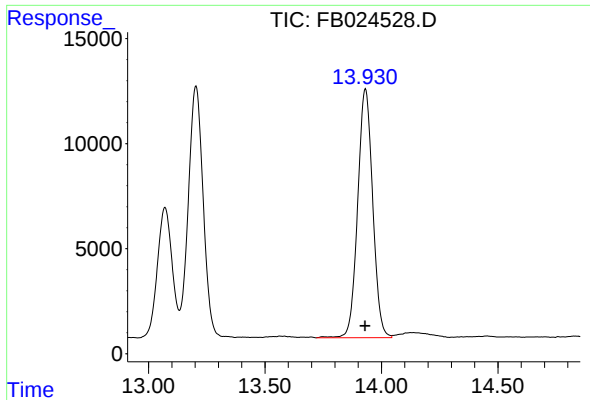

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.003 min
Response: 530592
Conc: 15.83 ng/ml

Instrument :
FID_B
ClientSampleId :
PL-02-063020MSD

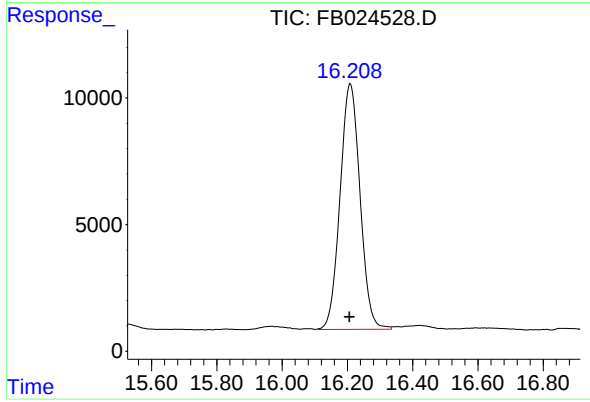

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.002 min
Response: 412332
Conc: 14.85 ng/ml