

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070121\
Data File : FB025972.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2021 10:55
Operator : AJ/MA
Sample : BSF0701S1
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 01 13:53:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.230	567369	23.477 ng/ml
Target Compounds				
1) t	2-Methylpentane	5.206	750109	28.503 ng/ml
2) t	2,2,4-Trimethylpentane	7.892	634747	31.509 ng/ml
3) t	n-Heptane	8.209	353877	9.845 ng/ml
4) t	Benzene	8.360	401178	9.610 ng/ml
6) t	Toluene	11.046	1134044	27.558 ng/ml
7) t	Ethylbenzene	13.449	338151	8.873 ng/ml
8) t	m-Xylene	13.579	652068	16.587 ng/ml
9) t	O-Xylene	14.302	597219	18.730 ng/ml
10) t	1,2,4-Trimethylbenzene	16.553	351597	17.863 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070121\
Data File : FB025972.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2021 10:55
Operator : AJ/MA
Sample : BSF0701S1
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jul 01 13:53:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060921.M
Quant Title :
QLast Update : Wed Jun 09 13:39:17 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

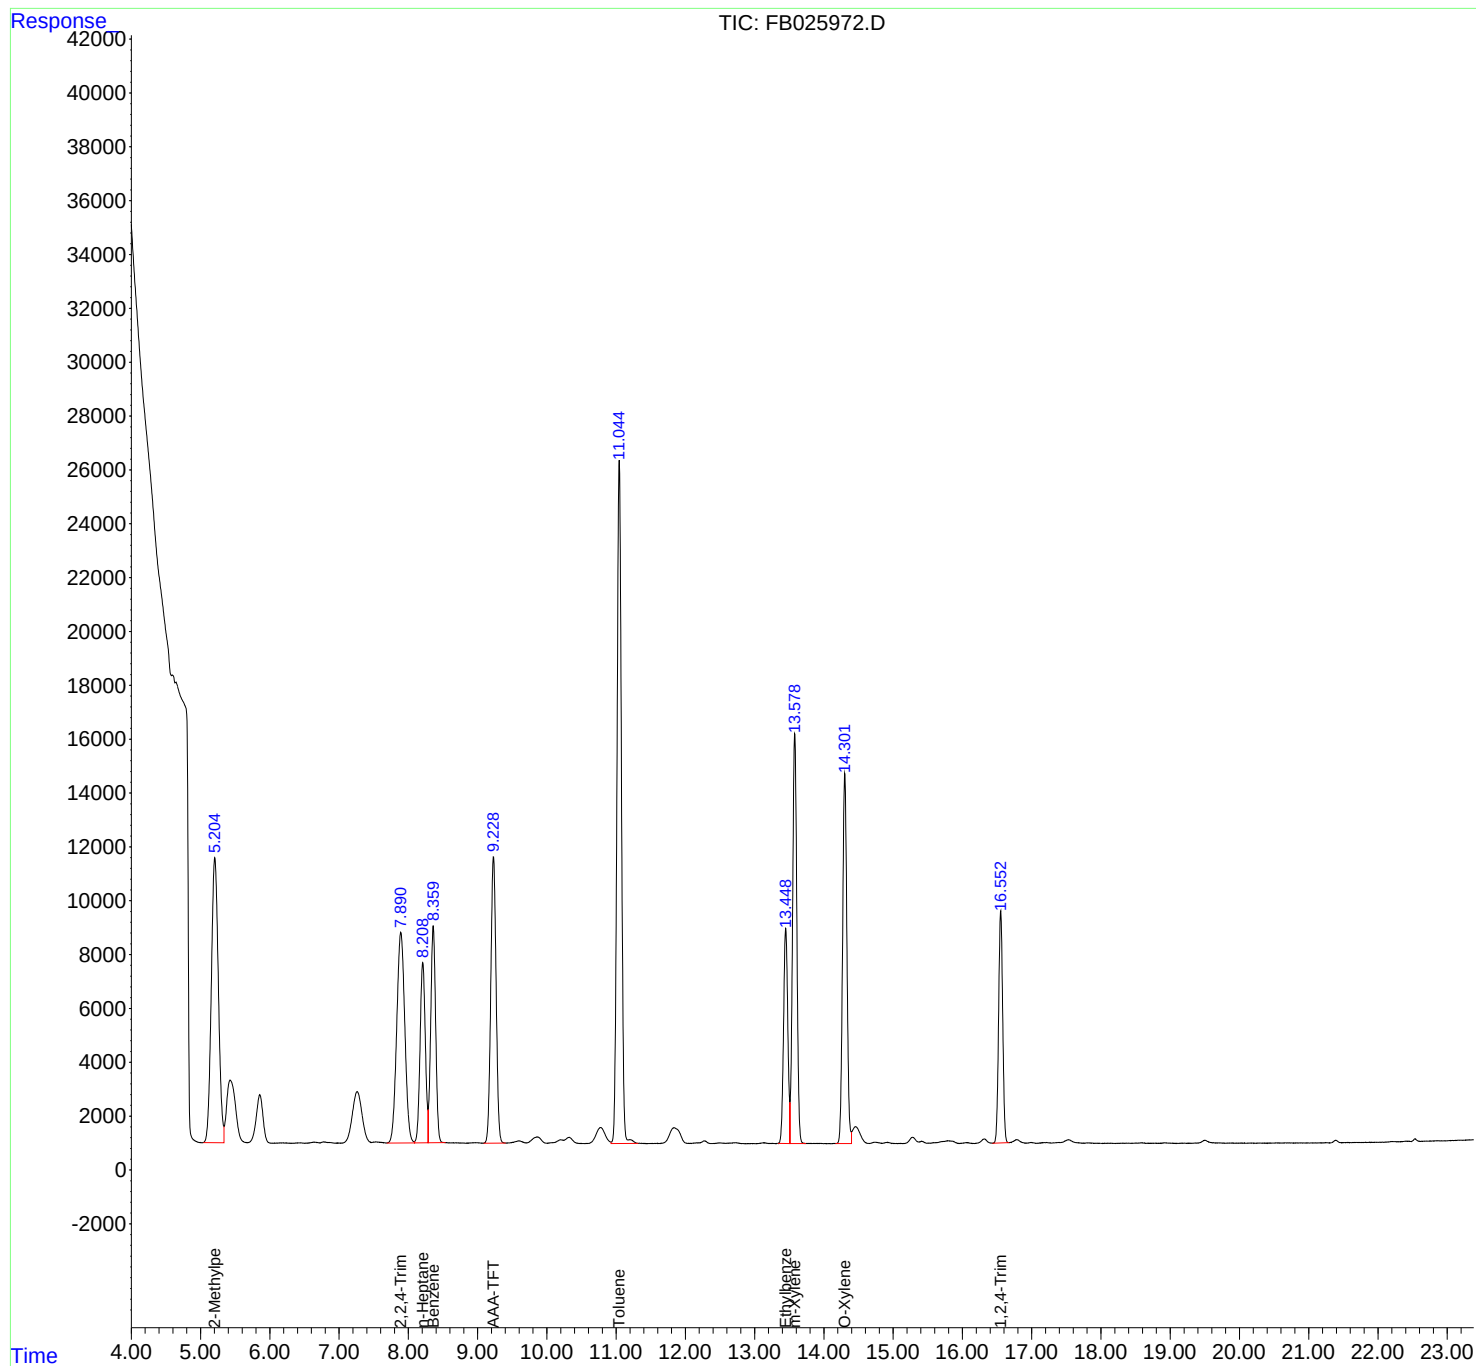

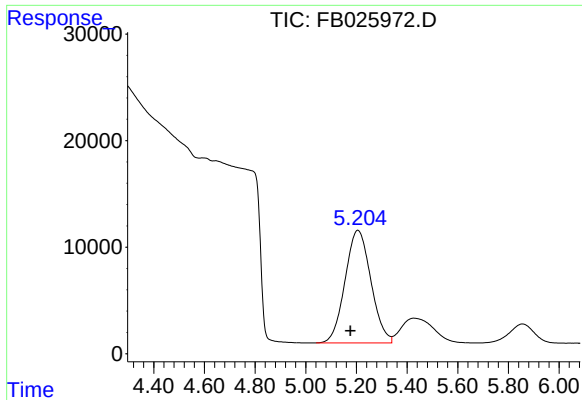


#1 2-Methylpentane

R.T.: 5.206 min
Delta R.T.: 0.029 min
Response: 750109
Conc: 28.50 ng/ml

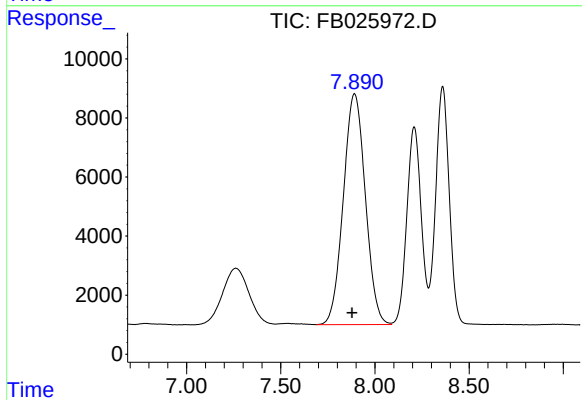


#2 2,2,4-Trimethylpentane

R.T.: 7.892 min
Delta R.T.: 0.014 min
Response: 634747
Conc: 31.51 ng/ml

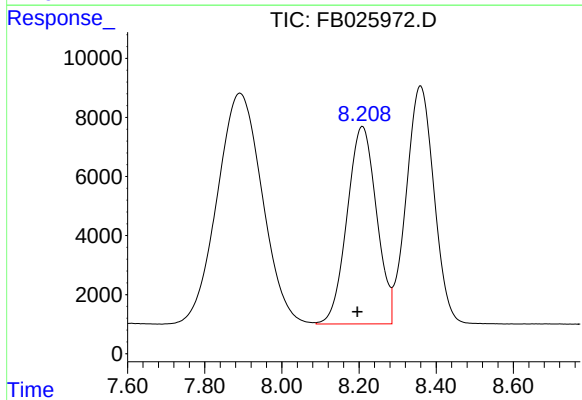


#3 n-Heptane

R.T.: 8.209 min
Delta R.T.: 0.013 min
Response: 353877
Conc: 9.84 ng/ml

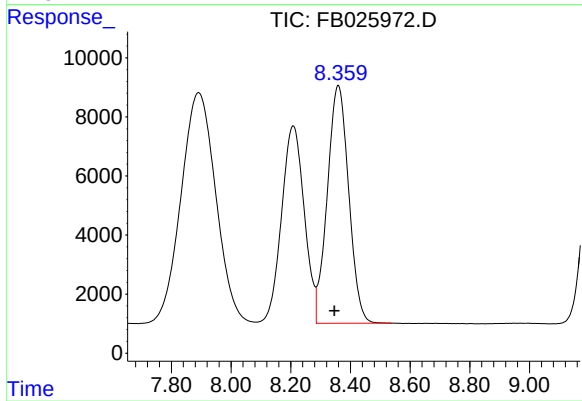


#4 Benzene

R.T.: 8.360 min
Delta R.T.: 0.013 min
Response: 401178
Conc: 9.61 ng/ml

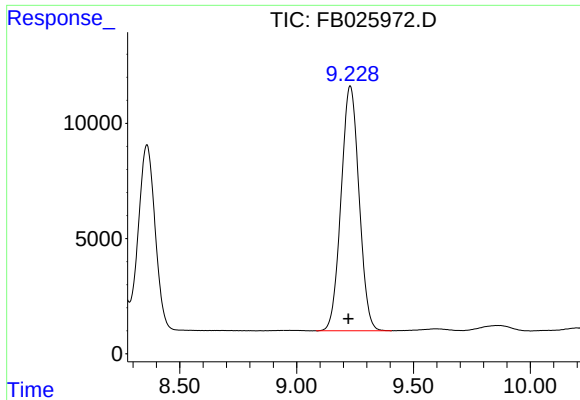


#5 AAA-TFT

R.T.: 9.230 min
Delta R.T.: 0.009 min
Response: 567369
Conc: 23.48 ng/ml

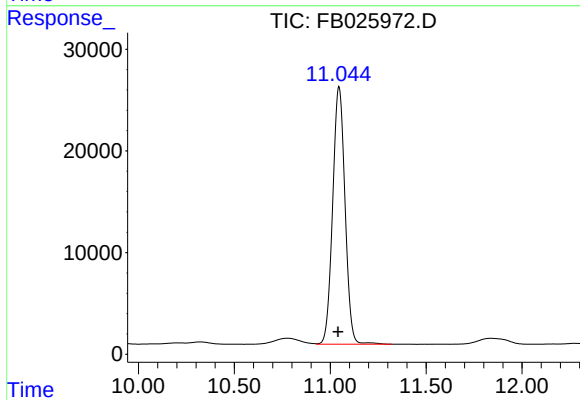


#6 Toluene

R.T.: 11.046 min
Delta R.T.: 0.004 min
Response: 1134044
Conc: 27.56 ng/ml

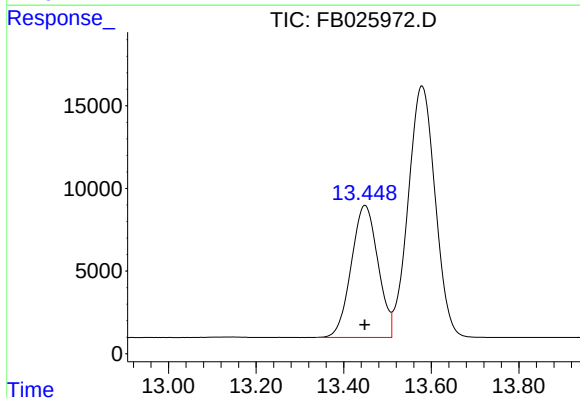


#7 Ethylbenzene

R.T.: 13.449 min
Delta R.T.: 0.001 min
Response: 338151
Conc: 8.87 ng/ml

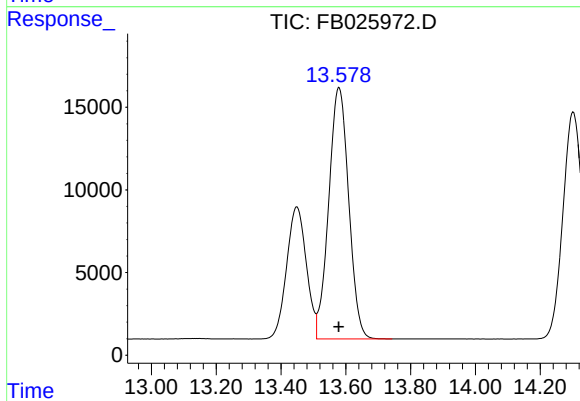


#8 m-Xylene

R.T.: 13.579 min
Delta R.T.: 0.000 min
Response: 652068
Conc: 16.59 ng/ml

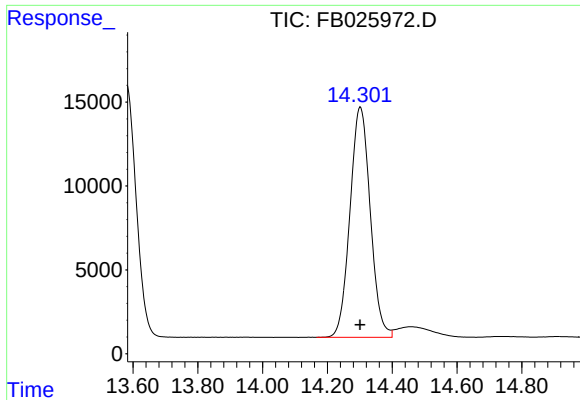

#9 O-Xylene

R.T.: 14.302 min
Delta R.T.: 0.000 min
Response: 597219
Conc: 18.73 ng/ml

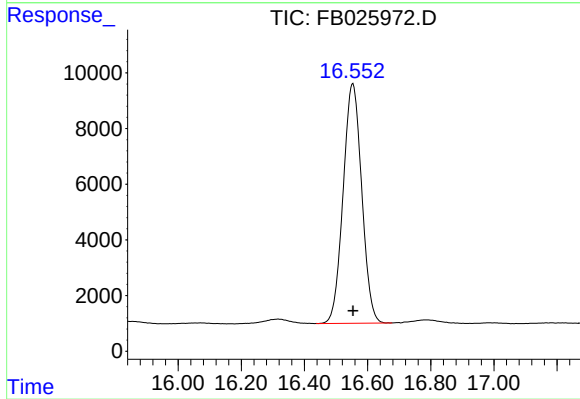

#10 1,2,4-Trimethylbenzene

R.T.: 16.553 min
Delta R.T.: 0.000 min
Response: 351597
Conc: 17.86 ng/ml