

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070122\
 Data File : FB027615.D
 Signal(s) : FID2B.CH
 Acq On : 2 Jul 2022 4:24
 Operator : AJ/MA
 Sample : N3564-34MS
 Misc : 5.05G/5.00 ML DI WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Jul 02 05:07:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.855	126893	11.313 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	14097	0.837 ng/ml
2) t 2,2,4-Trimethylpentane	7.388	5695	0.324 ng/ml
3) t n-Heptane	7.782	20540	1.172 ng/ml
4) t Benzene	7.824	10246	0.502 ng/ml
7) t Ethylbenzene	13.026	51936	2.868 ng/ml
9) t O-Xylene	13.934	10812	0.622 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070122\
Data File : FB027615.D
Signal(s) : FID2B.CH
Acq On : 2 Jul 2022 4:24
Operator : AJ/MA
Sample : N3564-34MS
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Jul 02 05:07:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

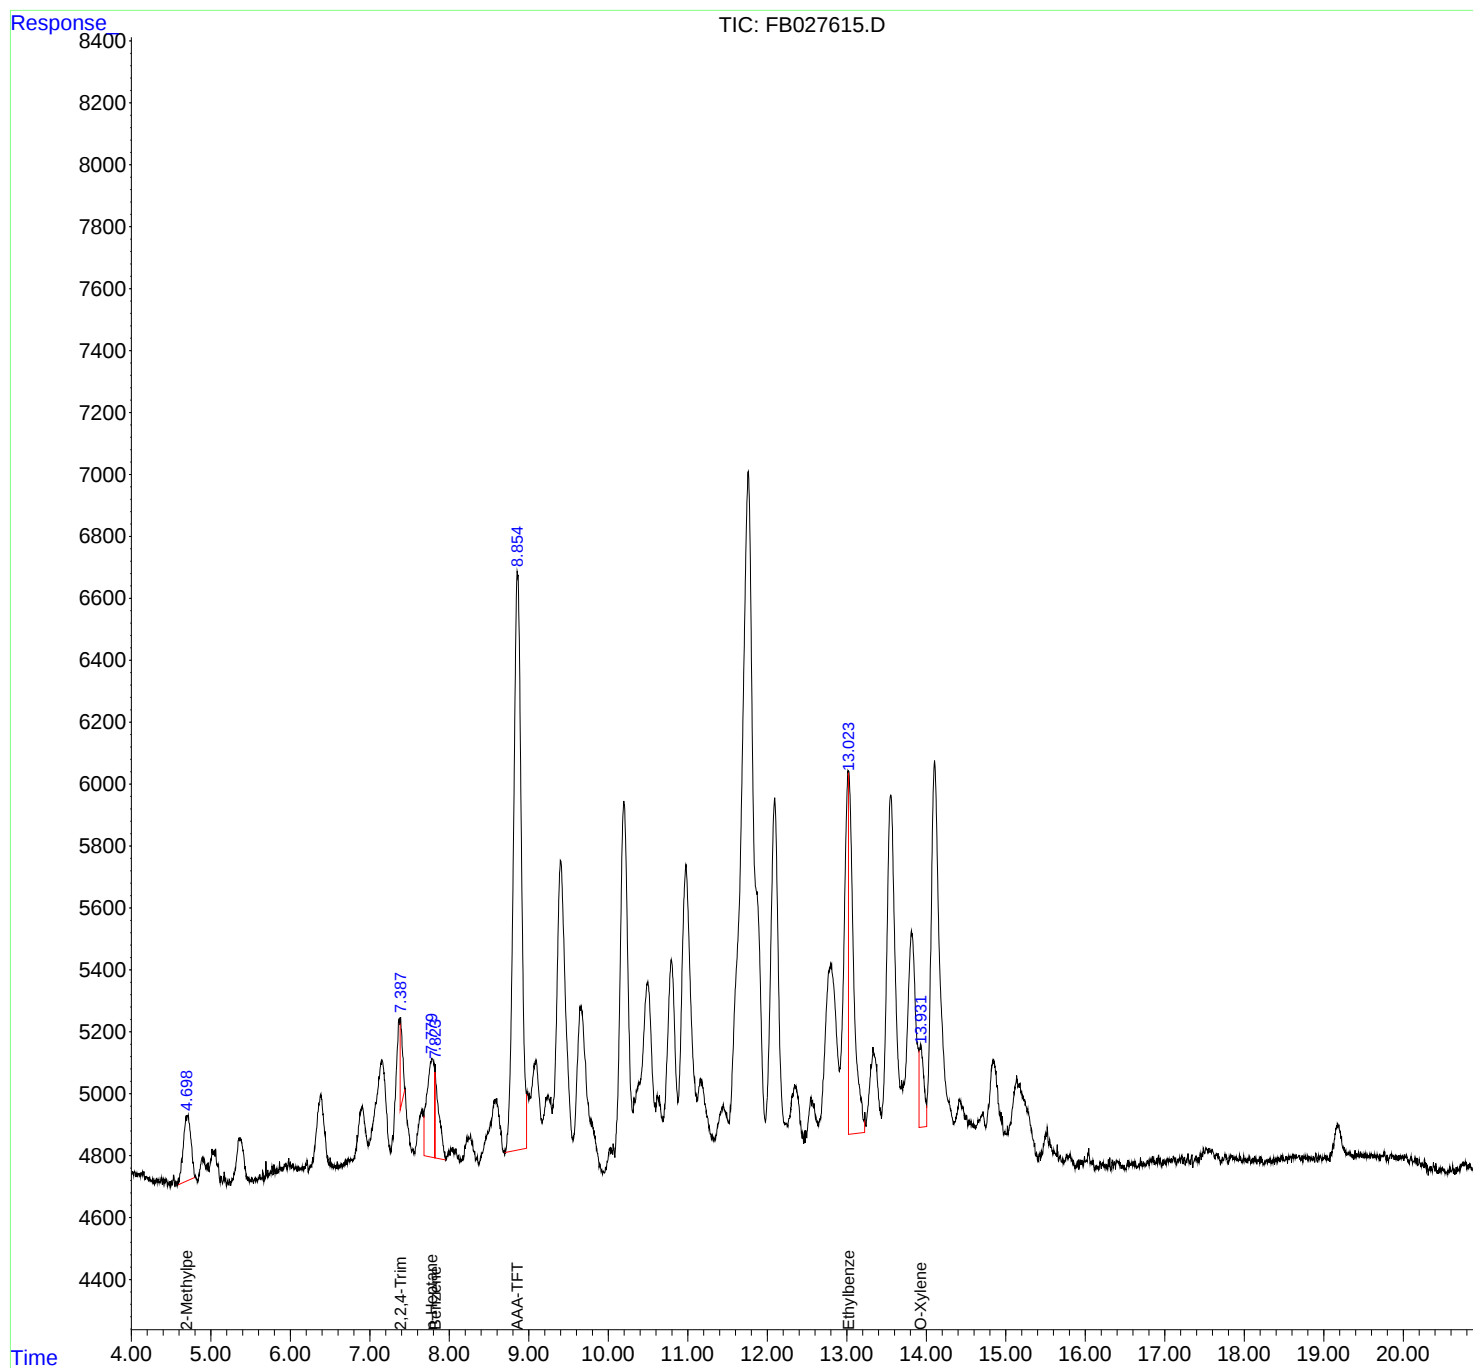


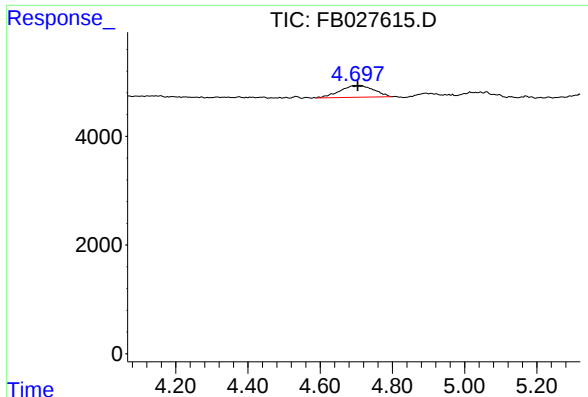

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: -0.015 min
Response: 14097
Conc: 0.84 ng/ml

Instrument :
FID_B
ClientSampleId :

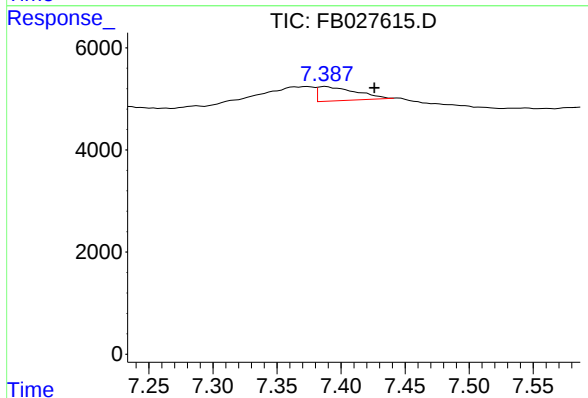


#2 2,2,4-Trimethylpentane

R.T.: 7.388 min
Delta R.T.: -0.038 min
Response: 5695
Conc: 0.32 ng/ml

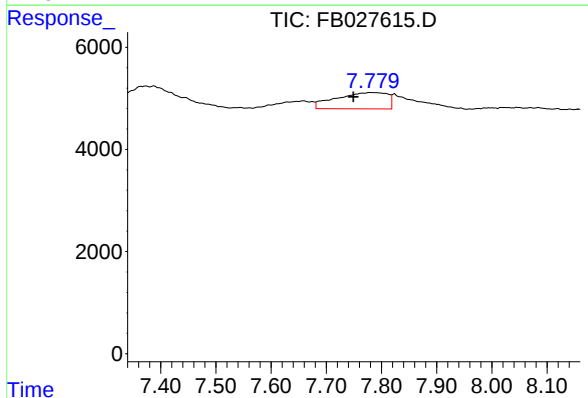


#3 n-Heptane

R.T.: 7.782 min
Delta R.T.: 0.032 min
Response: 20540
Conc: 1.17 ng/ml

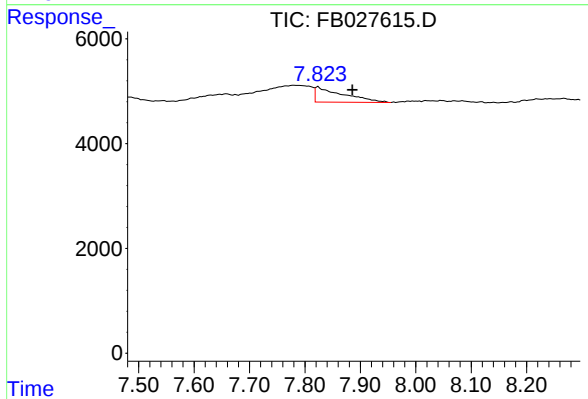

#4 Benzene


R.T.: 7.824 min
Delta R.T.: -0.062 min
Response: 10246
Conc: 0.50 ng/ml

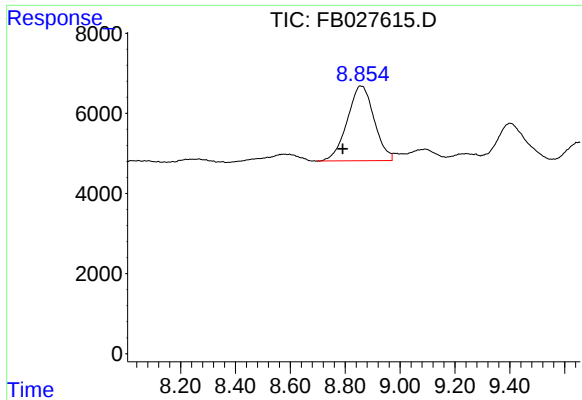

#5 AAA-TFT


R.T.: 8.855 min
Delta R.T.: 0.064 min
Response: 126893
Conc: 11.31 ng/ml

Instrument :
FID_B
ClientSampleId :

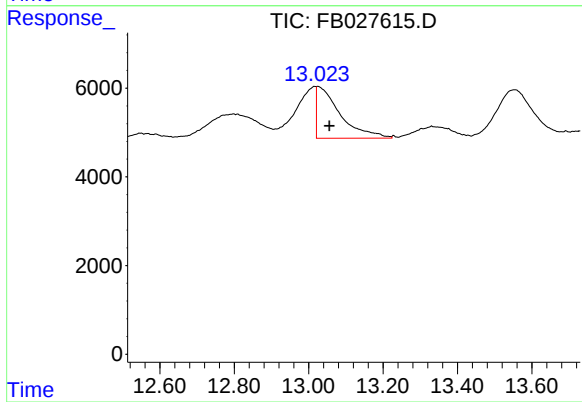

#7 Ethylbenzene

R.T.: 13.026 min
Delta R.T.: -0.031 min
Response: 51936
Conc: 2.87 ng/ml

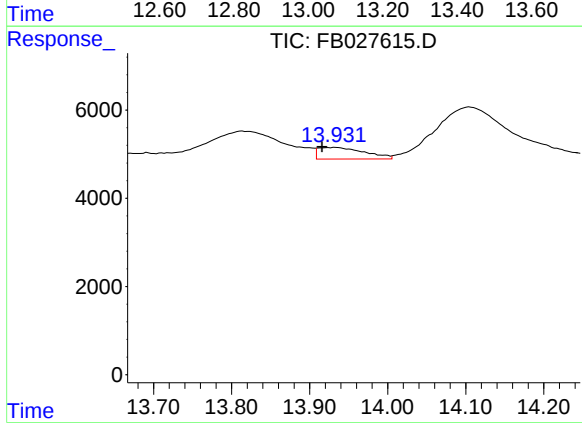

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.018 min
Response: 10812
Conc: 0.62 ng/ml