

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070122\
 Data File : FB027590.D
 Signal(s) : FID2B.CH
 Acq On : 1 Jul 2022 12:07
 Operator : AJ/MA
 Sample : N3214-09
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 MDL-WATER-03-QT2-2022

Integration File: Calibration.e
 Quant Time: Jul 02 05:25:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	265682	23.686 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	50856	3.019 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	31631	1.801 ng/ml
3) t n-Heptane	7.763	10929	0.624 ng/ml
4) t Benzene	7.894	11654	0.571 ng/ml
6) t Toluene	10.626	36944	1.908 ng/ml
7) t Ethylbenzene	13.055	10574	0.584 ng/ml
8) t m-Xylene	13.191	22839	1.281 ng/ml
9) t O-Xylene	13.919	23156	1.333 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	22847	1.330 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070122\
Data File : FB027590.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2022 12:07
Operator : AJ/MA
Sample : N3214-09
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
MDL-WATER-03-QT2-2022

Integration File: Calibration.e
Quant Time: Jul 02 05:25:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

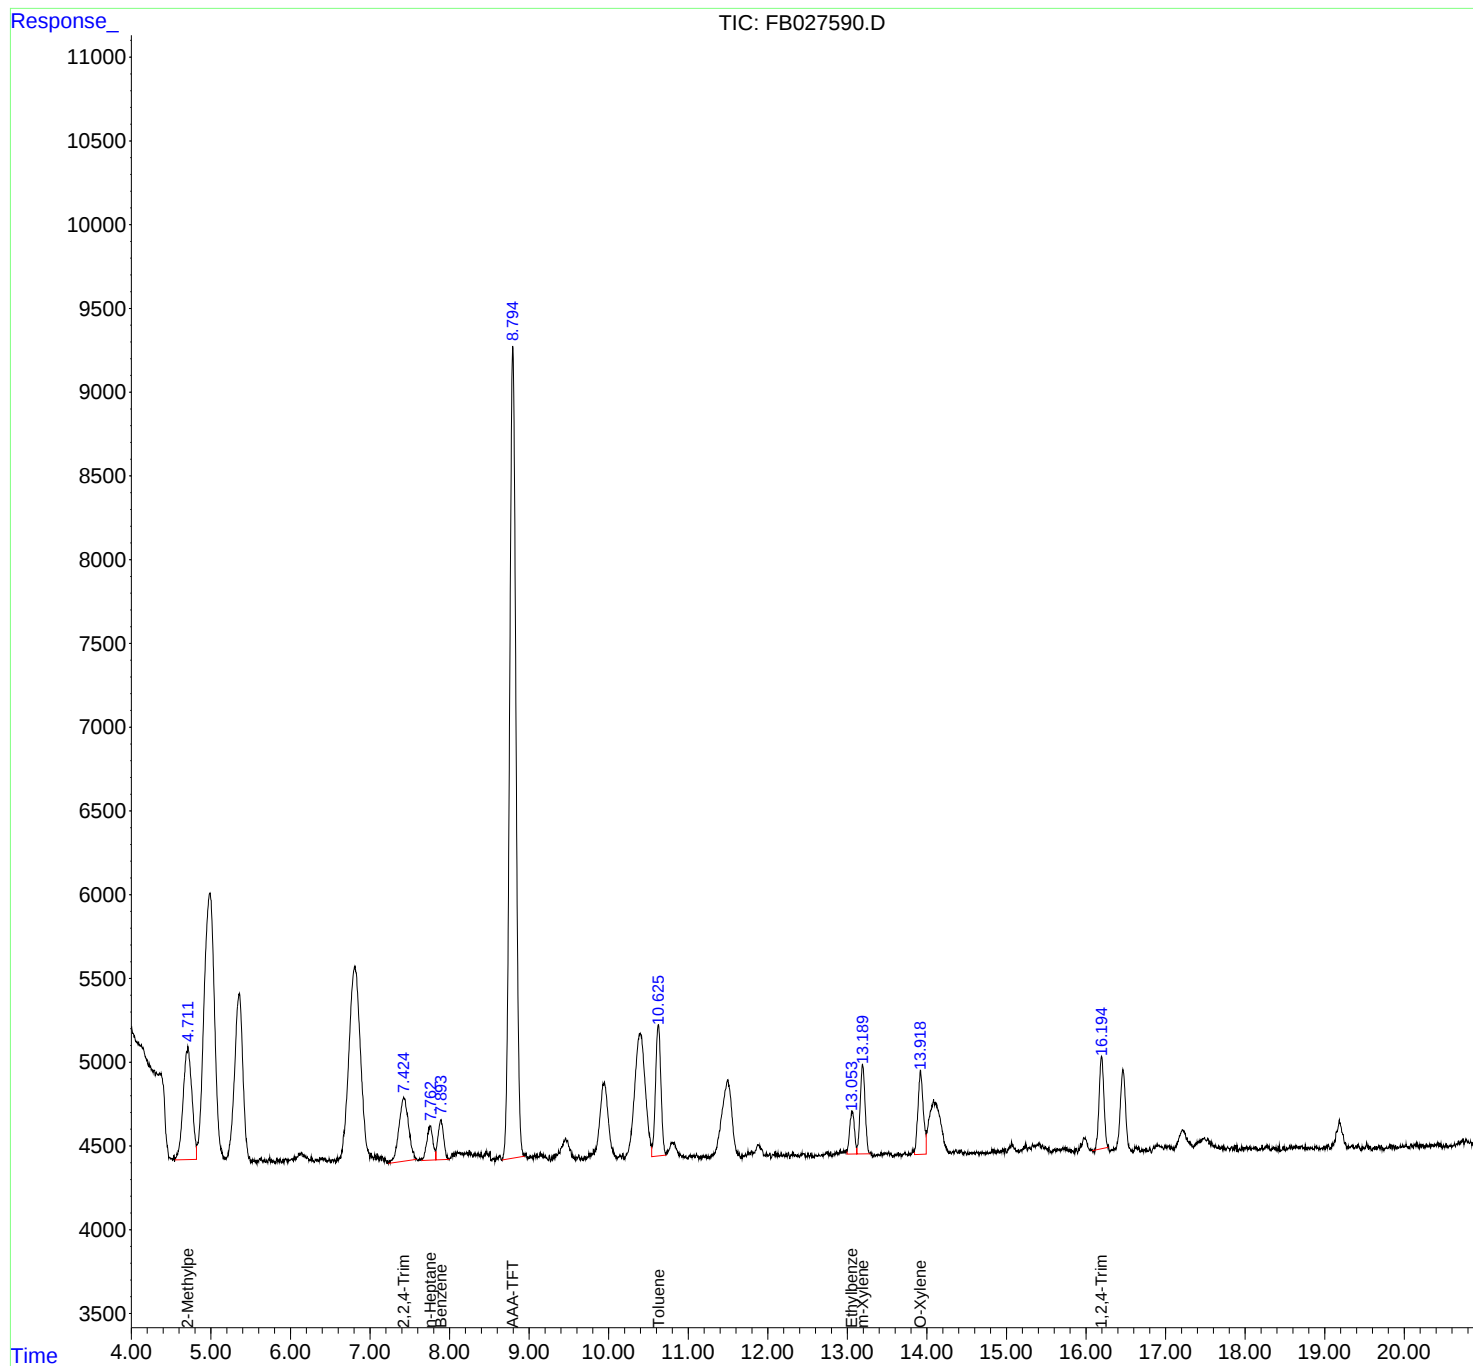


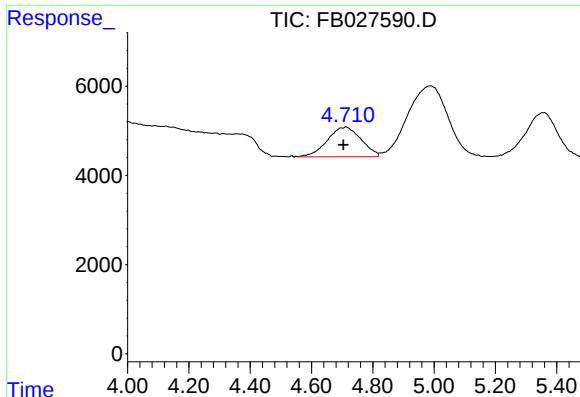

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: 0.009 min
Response: 50856
Conc: 3.02 ng/ml

Instrument :
FID_B
ClientSampleId :
MDL-WATER-03-QT2-2022

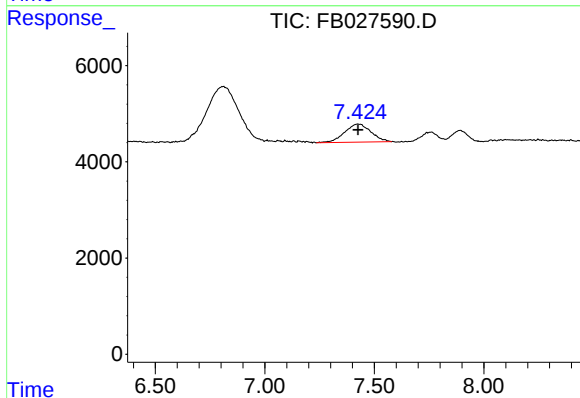


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: 0.000 min
Response: 31631
Conc: 1.80 ng/ml

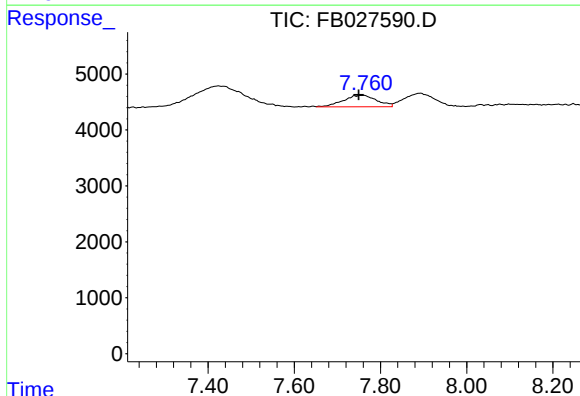


#3 n-Heptane

R.T.: 7.763 min
Delta R.T.: 0.013 min
Response: 10929
Conc: 0.62 ng/ml

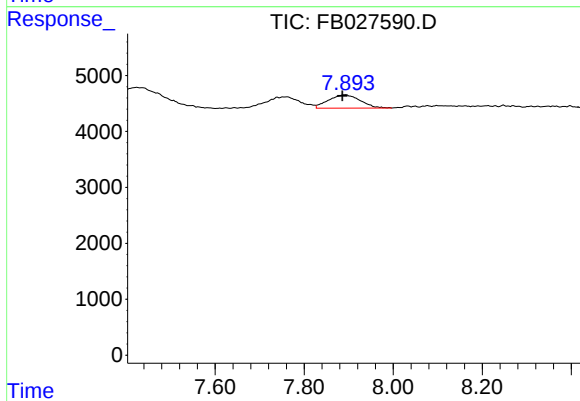

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.008 min
Response: 11654
Conc: 0.57 ng/ml

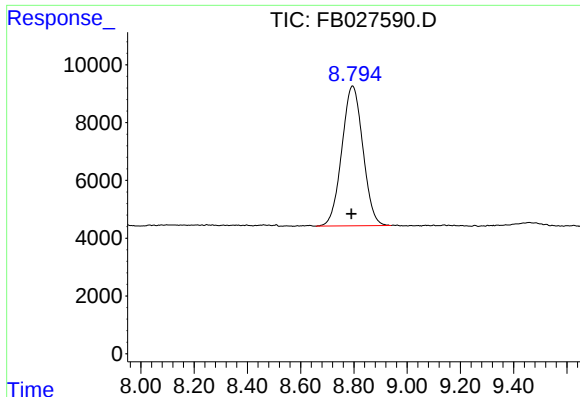

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: 0.005 min
Response: 265682
Conc: 23.69 ng/ml

Instrument :
FID_B
ClientSampleId :
MDL-WATER-03-QT2-2022

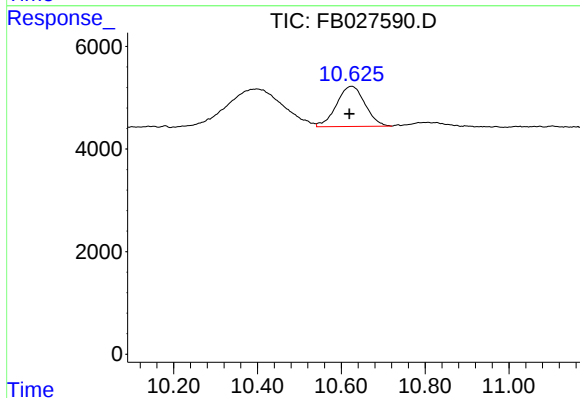


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.007 min
Response: 36944
Conc: 1.91 ng/ml

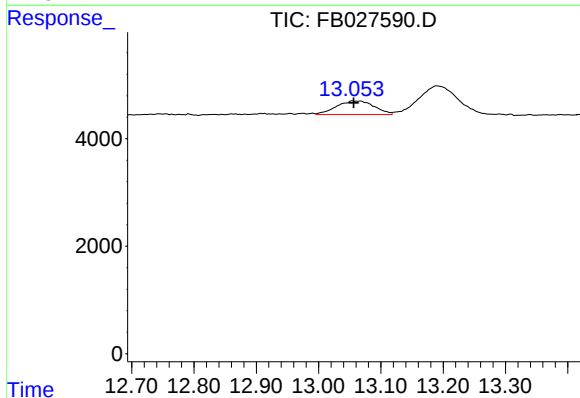


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.002 min
Response: 10574
Conc: 0.58 ng/ml

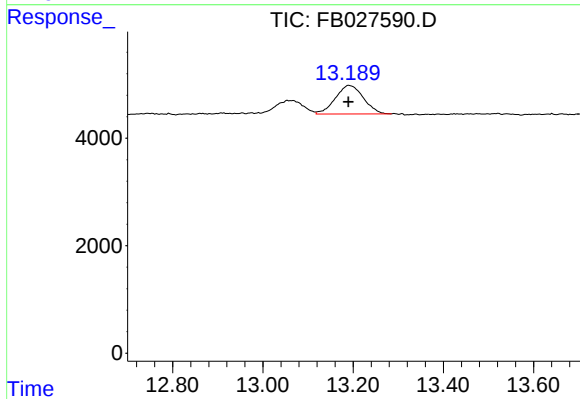

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 22839
Conc: 1.28 ng/ml

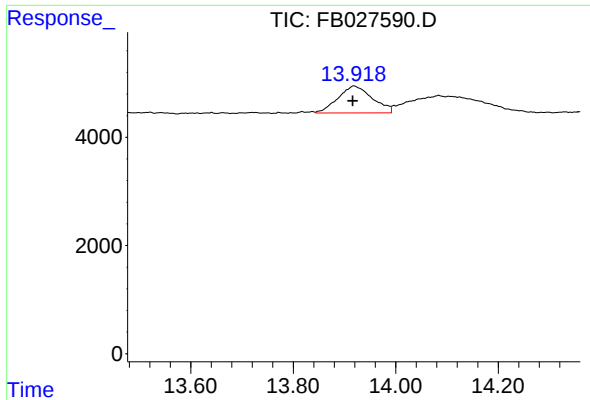

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.003 min
Response: 23156
Conc: 1.33 ng/ml

Instrument :
FID_B
ClientSampleId :
MDL-WATER-03-QT2-2022

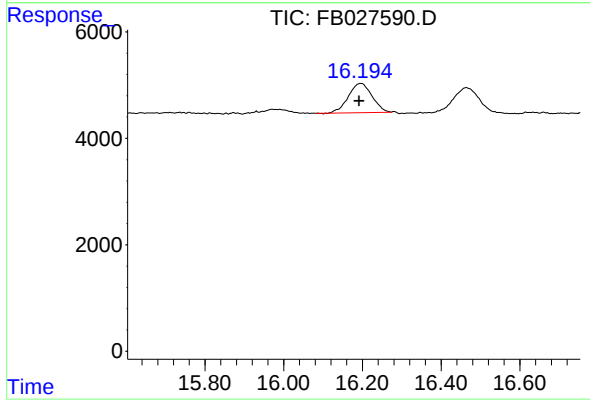

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.005 min
Response: 22847
Conc: 1.33 ng/ml