

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070122\
 Data File : FB027595.D
 Signal(s) : FID2B.CH
 Acq On : 1 Jul 2022 15:17
 Operator : AJ/MA
 Sample : BSF0701S3
 Misc : 5.00G/5.00 ML WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0701S3

Integration File: Calibration.e
 Quant Time: Jul 02 05:05:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	210758	18.790 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.717	471460	27.984 ng/ml
2) t 2,2,4-Trimethylpentane	7.434	516440	29.413 ng/ml
3) t n-Heptane	7.756	158829	9.066 ng/ml
4) t Benzene	7.894	186647	9.153 ng/ml
6) t Toluene	10.626	534701	27.616 ng/ml
7) t Ethylbenzene	13.063	171544	9.473 ng/ml
8) t m-Xylene	13.195	341689	19.168 ng/ml
9) t O-Xylene	13.922	341779	19.670 ng/ml
10) t 1,2,4-Trimethylbenzene	16.197	341314	19.869 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070122\
Data File : FB027595.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2022 15:17
Operator : AJ/MA
Sample : BSF0701S3
Misc : 5.00G/5.00 ML WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0701S3

Integration File: Calibration.e
Quant Time: Jul 02 05:05:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

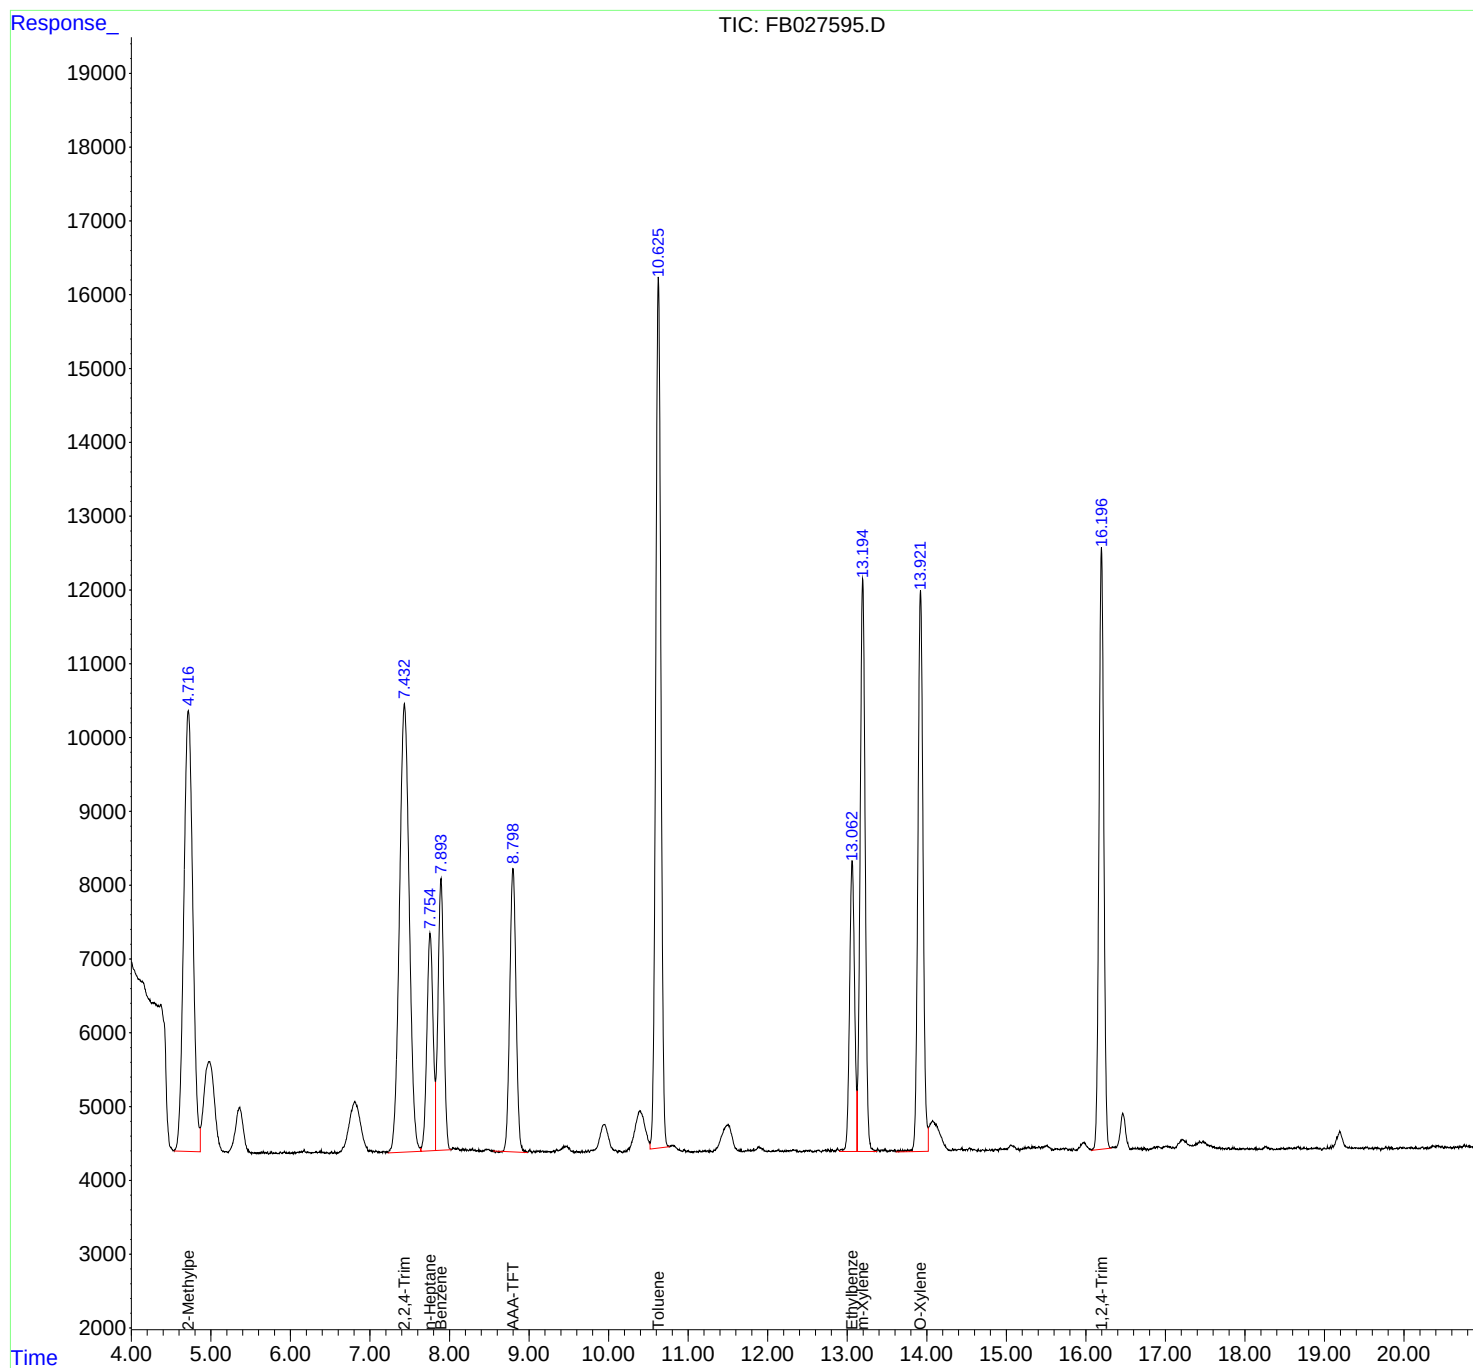


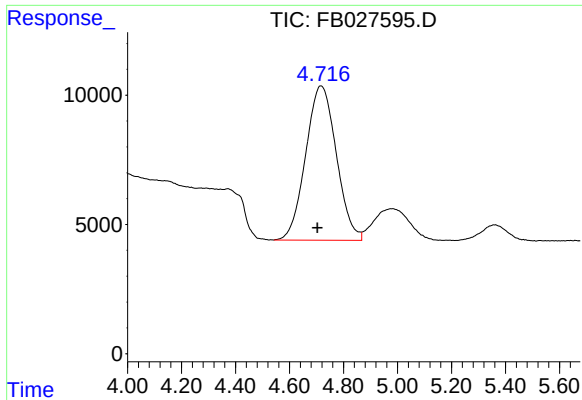

#1 2-Methylpentane


R.T.: 4.717 min
Delta R.T.: 0.013 min
Response: 471460
Conc: 27.98 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S3

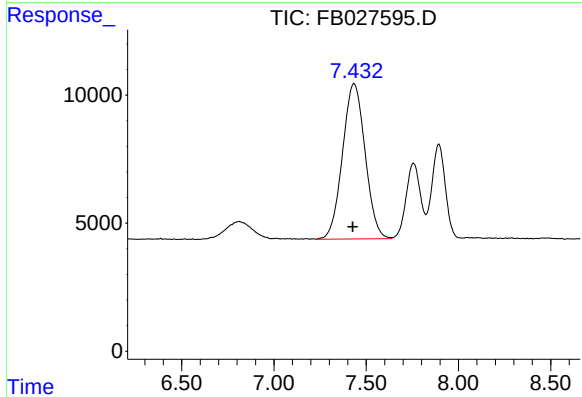


#2 2,2,4-Trimethylpentane

R.T.: 7.434 min
Delta R.T.: 0.008 min
Response: 516440
Conc: 29.41 ng/ml

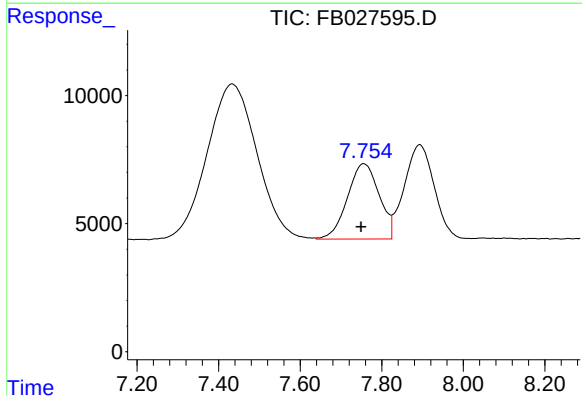


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.006 min
Response: 158829
Conc: 9.07 ng/ml

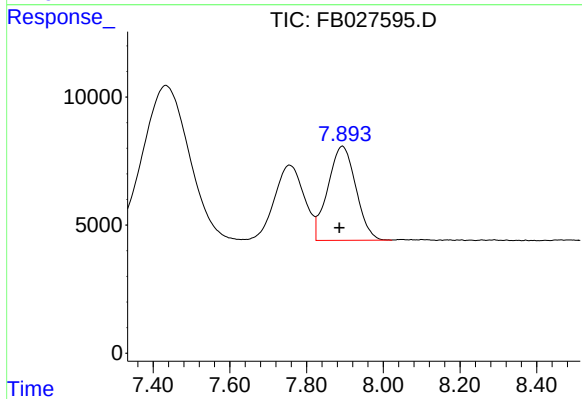

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.008 min
Response: 186647
Conc: 9.15 ng/ml

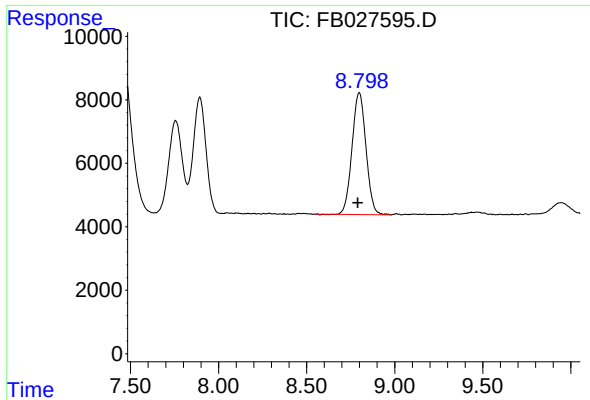

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.008 min
Response: 210758
Conc: 18.79 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S3

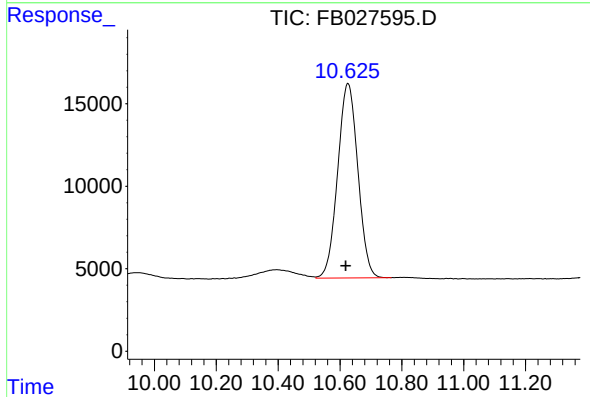


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.007 min
Response: 534701
Conc: 27.62 ng/ml

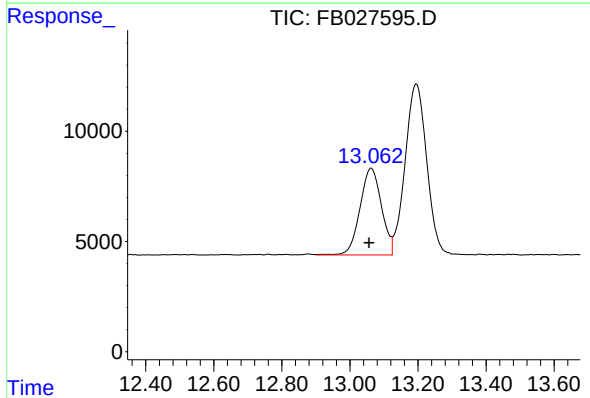


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.006 min
Response: 171544
Conc: 9.47 ng/ml

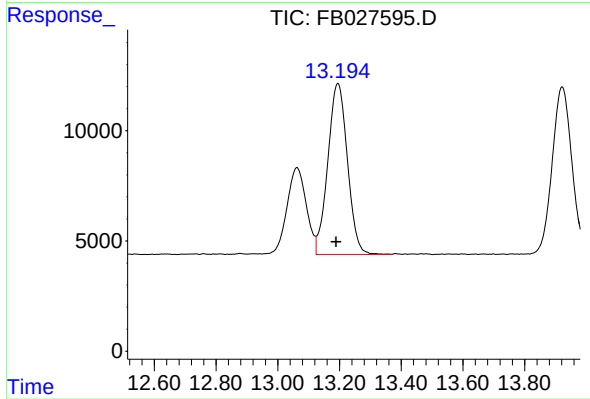

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: 0.006 min
Response: 341689
Conc: 19.17 ng/ml

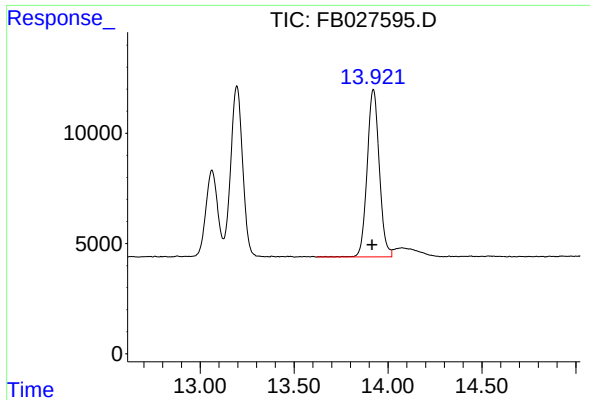

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: 0.006 min
Response: 341779
Conc: 19.67 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S3

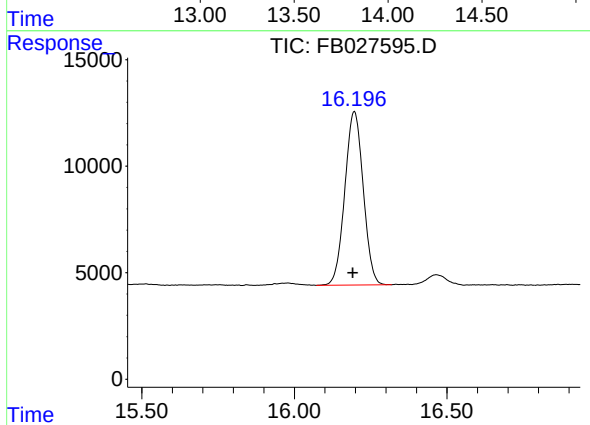

#10 1,2,4-Trimethylbenzene

R.T.: 16.197 min
Delta R.T.: 0.005 min
Response: 341314
Conc: 19.87 ng/ml