

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070122\
 Data File : FB027603.D
 Signal(s) : FID2B.CH
 Acq On : 1 Jul 2022 20:22
 Operator : AJ/MA
 Sample : BSF0701S4
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0701S4

Integration File: Calibration.e
 Quant Time: Jul 02 05:06:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	259592	23.143 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.719	481131	28.558 ng/ml
2) t 2,2,4-Trimethylpentane	7.438	511112	29.109 ng/ml
3) t n-Heptane	7.757	168567	9.622 ng/ml
4) t Benzene	7.895	203041	9.957 ng/ml
6) t Toluene	10.628	569159	29.396 ng/ml
7) t Ethylbenzene	13.064	182529	10.079 ng/ml
8) t m-Xylene	13.197	351612	19.725 ng/ml
9) t O-Xylene	13.924	349210	20.097 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	330212	19.223 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070122\
Data File : FB027603.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2022 20:22
Operator : AJ/MA
Sample : BSF0701S4
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0701S4

Integration File: Calibration.e
Quant Time: Jul 02 05:06:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

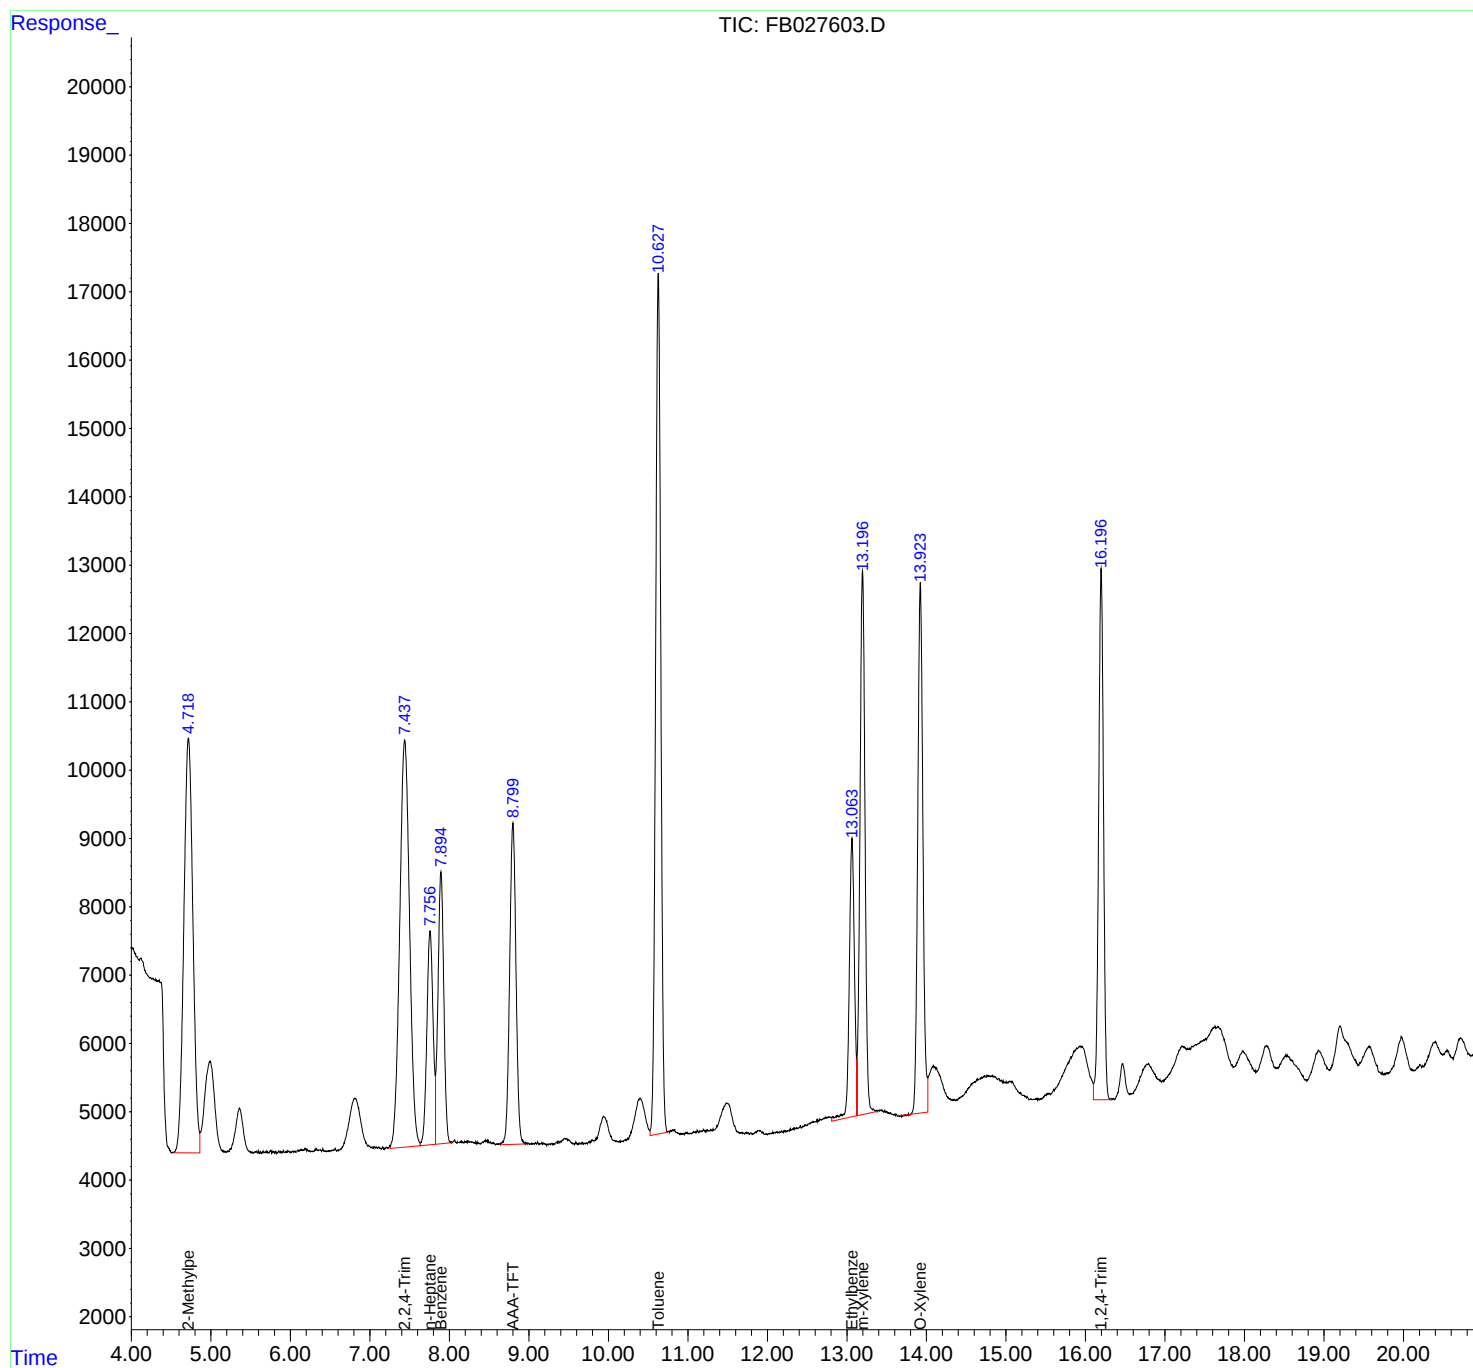


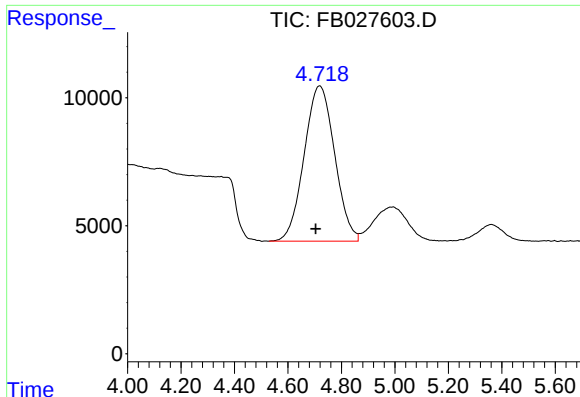

#1 2-Methylpentane


R.T.: 4.719 min
Delta R.T.: 0.015 min
Response: 481131
Conc: 28.56 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S4

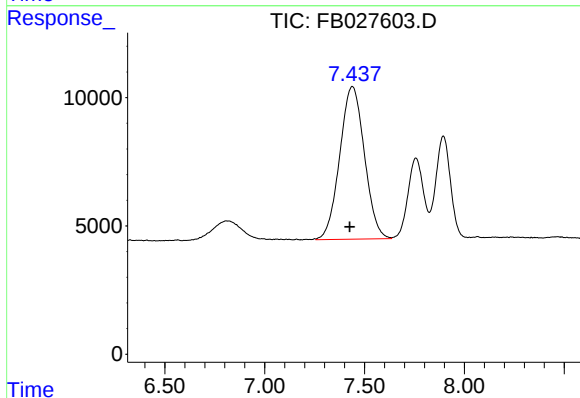


#2 2,2,4-Trimethylpentane

R.T.: 7.438 min
Delta R.T.: 0.012 min
Response: 511112
Conc: 29.11 ng/ml

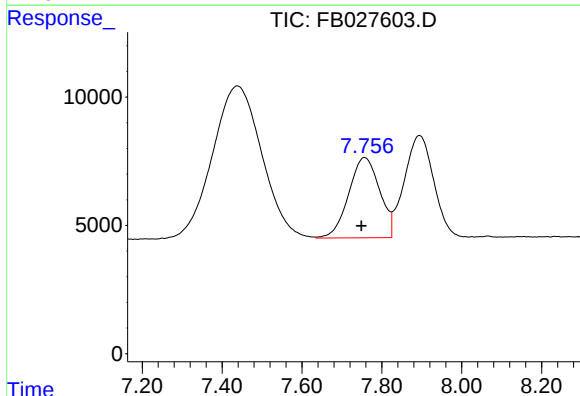


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.008 min
Response: 168567
Conc: 9.62 ng/ml

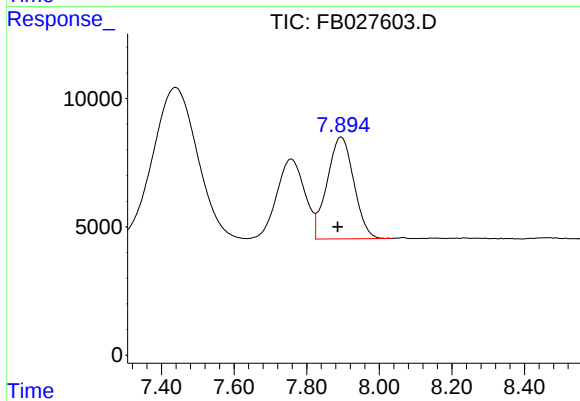

#4 Benzene


R.T.: 7.895 min
Delta R.T.: 0.009 min
Response: 203041
Conc: 9.96 ng/ml

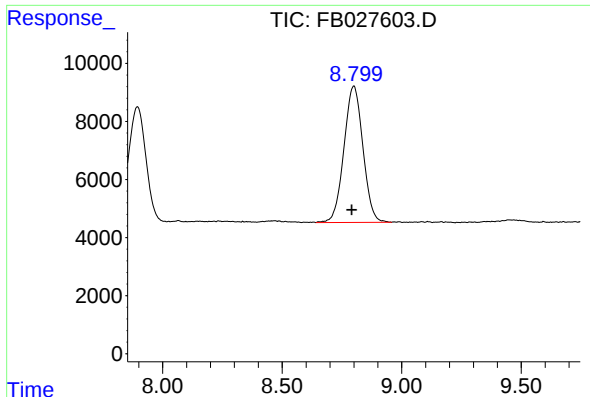

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.009 min
Response: 259592
Conc: 23.14 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S4

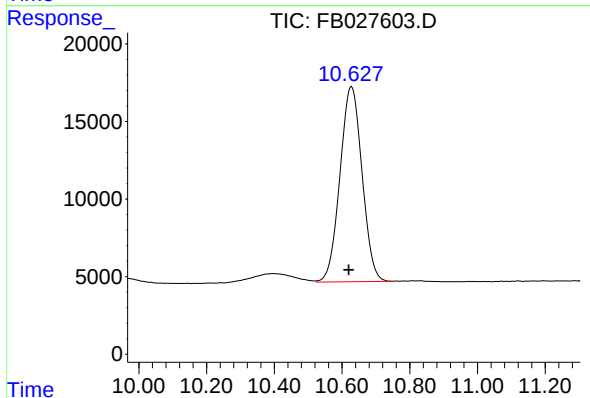


#6 Toluene

R.T.: 10.628 min
Delta R.T.: 0.009 min
Response: 569159
Conc: 29.40 ng/ml

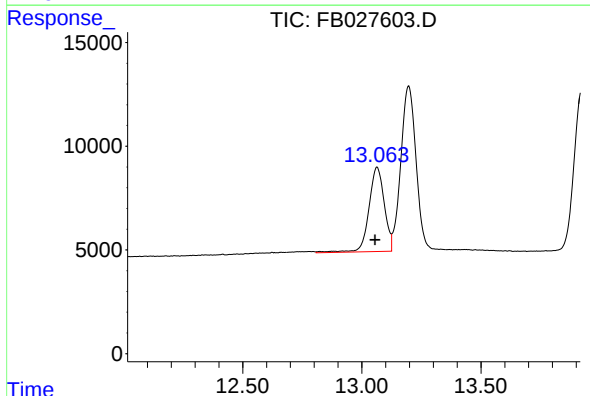


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.008 min
Response: 182529
Conc: 10.08 ng/ml

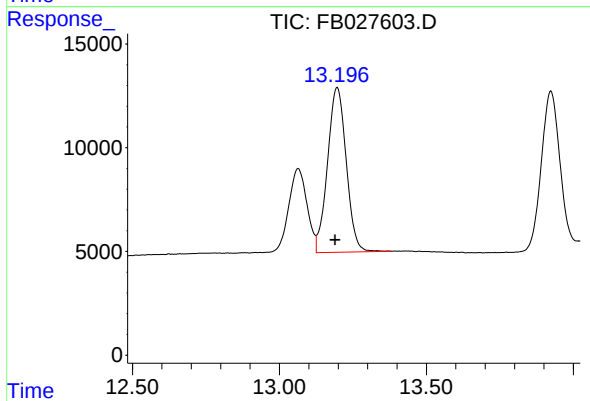

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.008 min
Response: 351612
Conc: 19.72 ng/ml

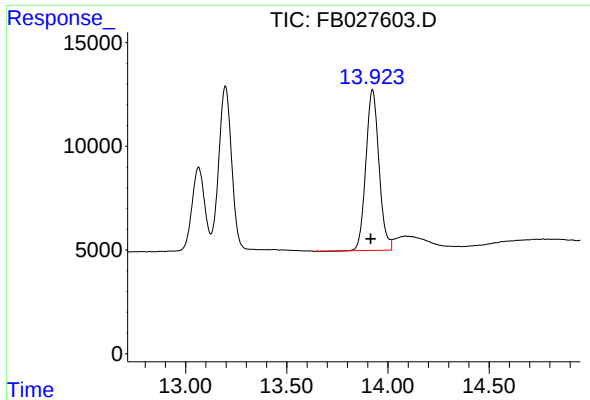

#9 O-Xylene

R.T.: 13.924 min
Delta R.T.: 0.008 min
Response: 349210
Conc: 20.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S4

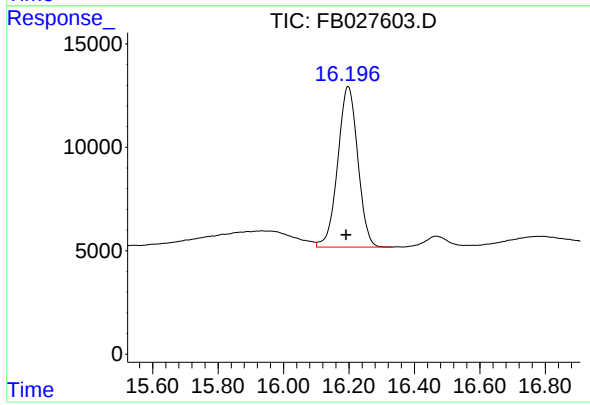

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: 0.007 min
Response: 330212
Conc: 19.22 ng/ml