

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070122\
 Data File : FB027617.D
 Signal(s) : FID2B.CH
 Acq On : 2 Jul 2022 5:38
 Operator : AJ/MA
 Sample : BSF0701S5
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0701S5

Integration File: Calibration.e
 Quant Time: Jul 02 06:24:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
 Quant Title :
 QLast Update : Mon Jun 13 09:22:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	240455	21.437 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	474483	28.164 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	494607	28.169 ng/ml
3) t n-Heptane	7.753	154933	8.844 ng/ml
4) t Benzene	7.891	188503	9.244 ng/ml
6) t Toluene	10.624	536099	27.688 ng/ml
7) t Ethylbenzene	13.060	166750	9.208 ng/ml
8) t m-Xylene	13.192	326115	18.294 ng/ml
9) t O-Xylene	13.919	321131	18.481 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	314645	18.316 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070122\
Data File : FB027617.D
Signal(s) : FID2B.CH
Acq On : 2 Jul 2022 5:38
Operator : AJ/MA
Sample : BSF0701S5
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0701S5

Integration File: Calibration.e
Quant Time: Jul 02 06:24:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB061022.M
Quant Title :
QLast Update : Mon Jun 13 09:22:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

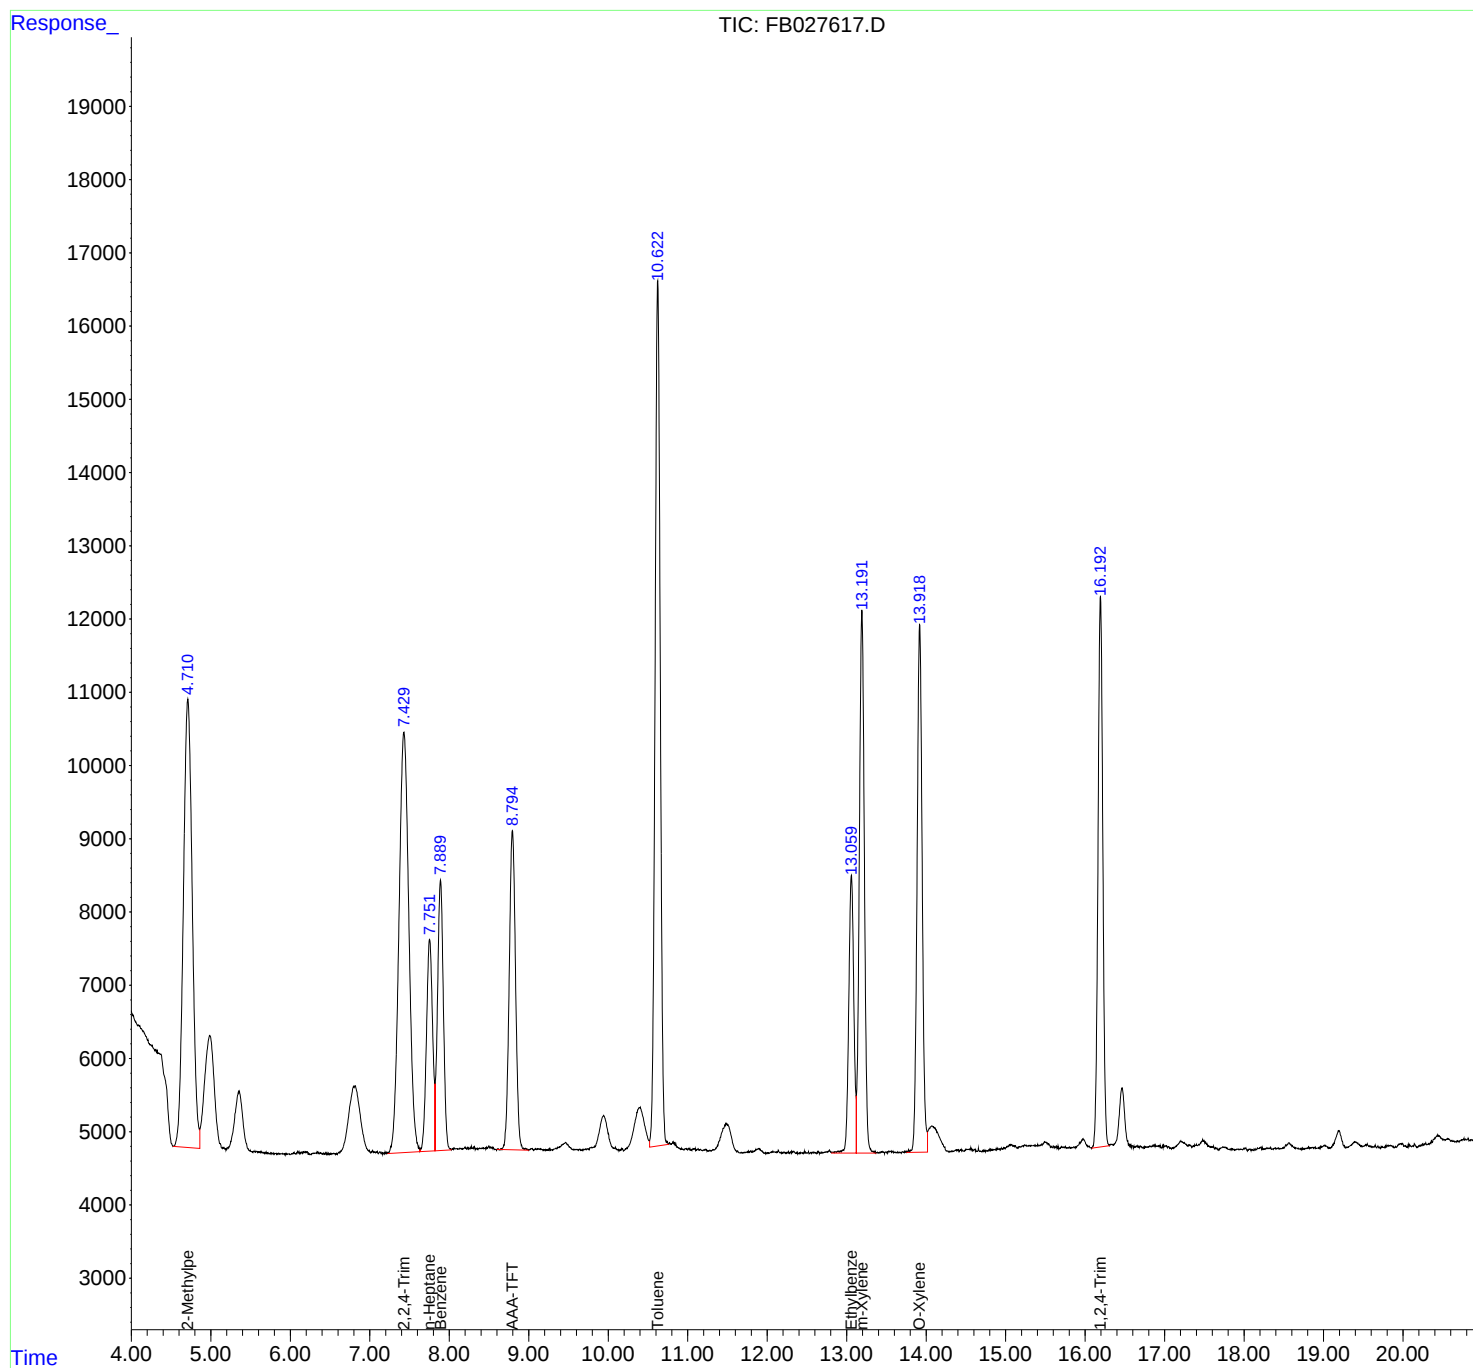


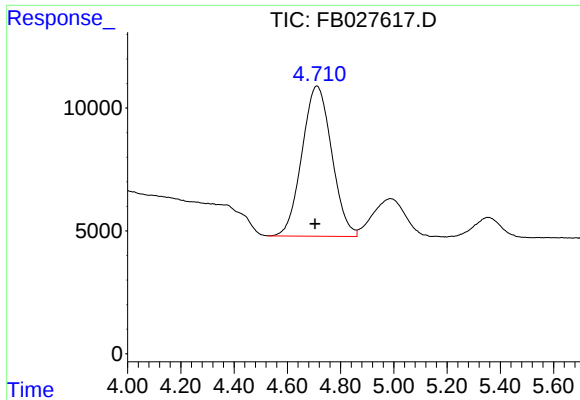

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.008 min
Response: 474483
Conc: 28.16 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S5

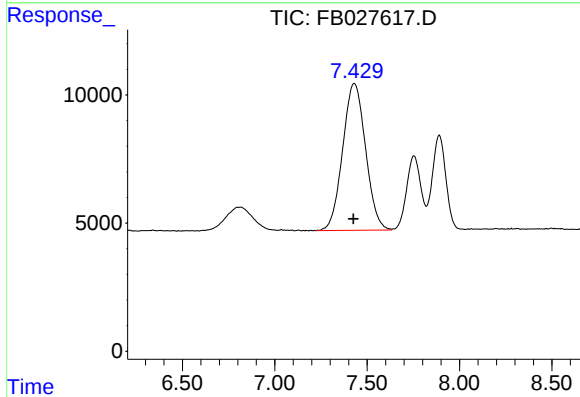


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: 0.004 min
Response: 494607
Conc: 28.17 ng/ml

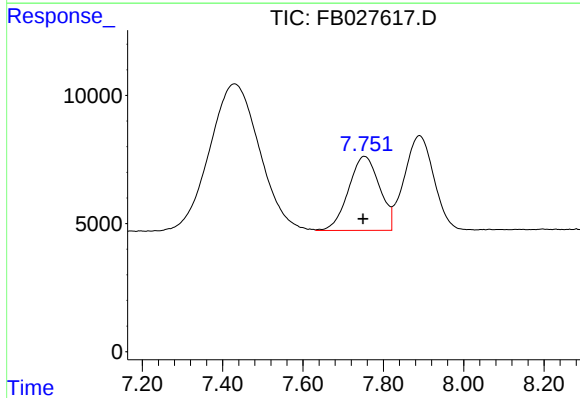


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.004 min
Response: 154933
Conc: 8.84 ng/ml

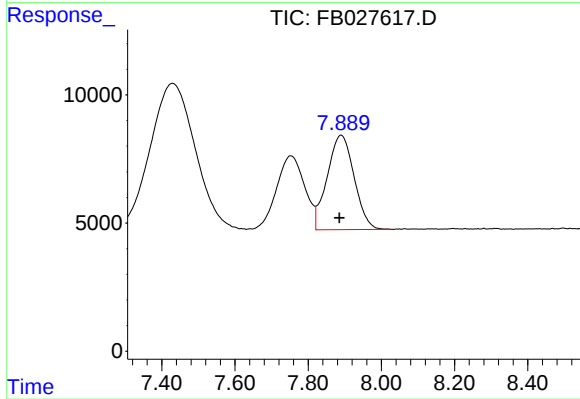

#4 Benzene


R.T.: 7.891 min
Delta R.T.: 0.005 min
Response: 188503
Conc: 9.24 ng/ml

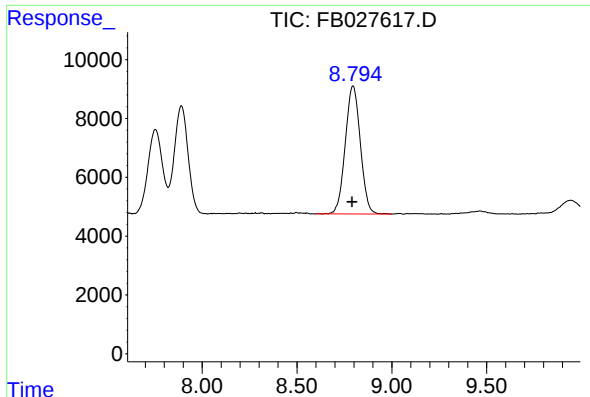

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.004 min
Response: 240455
Conc: 21.44 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S5

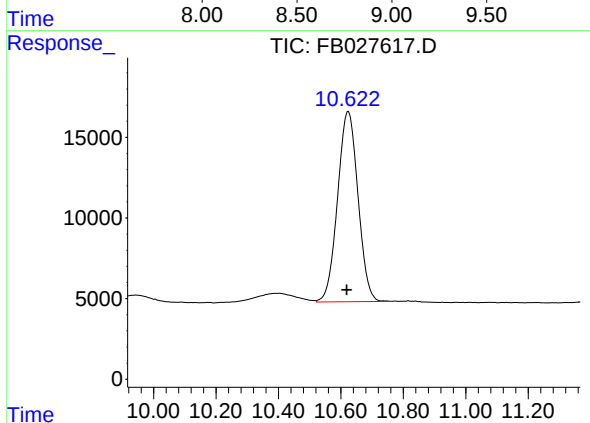


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.004 min
Response: 536099
Conc: 27.69 ng/ml

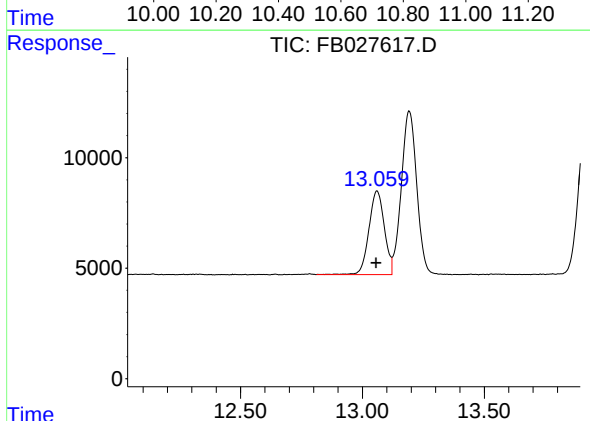


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.004 min
Response: 166750
Conc: 9.21 ng/ml

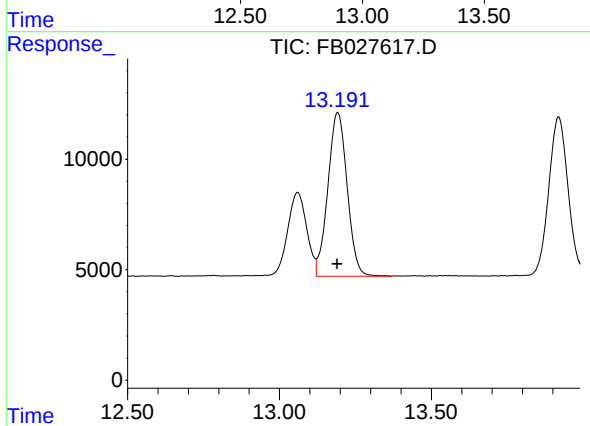

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.003 min
Response: 326115
Conc: 18.29 ng/ml

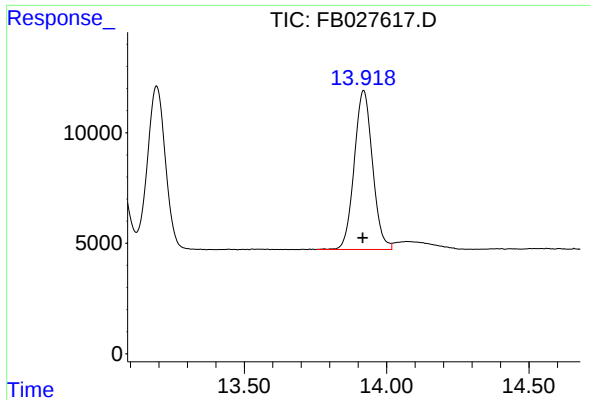

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.003 min
Response: 321131
Conc: 18.48 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0701S5

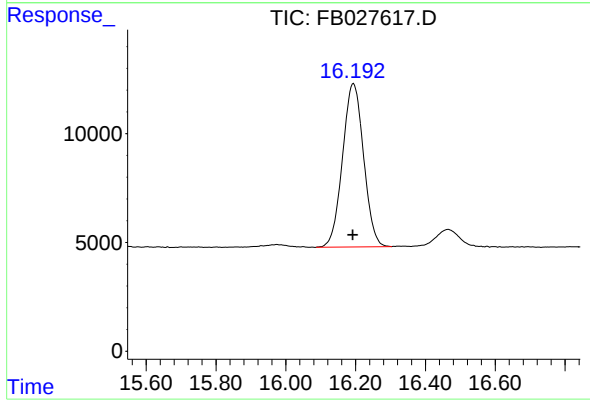

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.003 min
Response: 314645
Conc: 18.32 ng/ml