

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070125\
Data File : FB031989.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2025 12:38
Operator : YP/AJ
Sample : Q2458-07
Misc : 3.77G/5.00 ML DI WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-62

Integration File: Calibration.e
Quant Time: Jul 02 00:01:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.804	292209	18.940 ng/ml
Target Compounds			
8) t m-Xylene	13.191	4772	0.145 ng/ml
9) t O-Xylene	13.923	3945	0.127 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	10283	0.389 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB070125\
Data File : FB031989.D
Signal(s) : FID2B.CH
Acq On : 1 Jul 2025 12:38
Operator : YP/AJ
Sample : Q2458-07
Misc : 3.77G/5.00 ML DI WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-62

Integration File: Calibration.e
Quant Time: Jul 02 00:01:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB062325.M
Quant Title :
QLast Update : Mon Jun 23 13:56:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

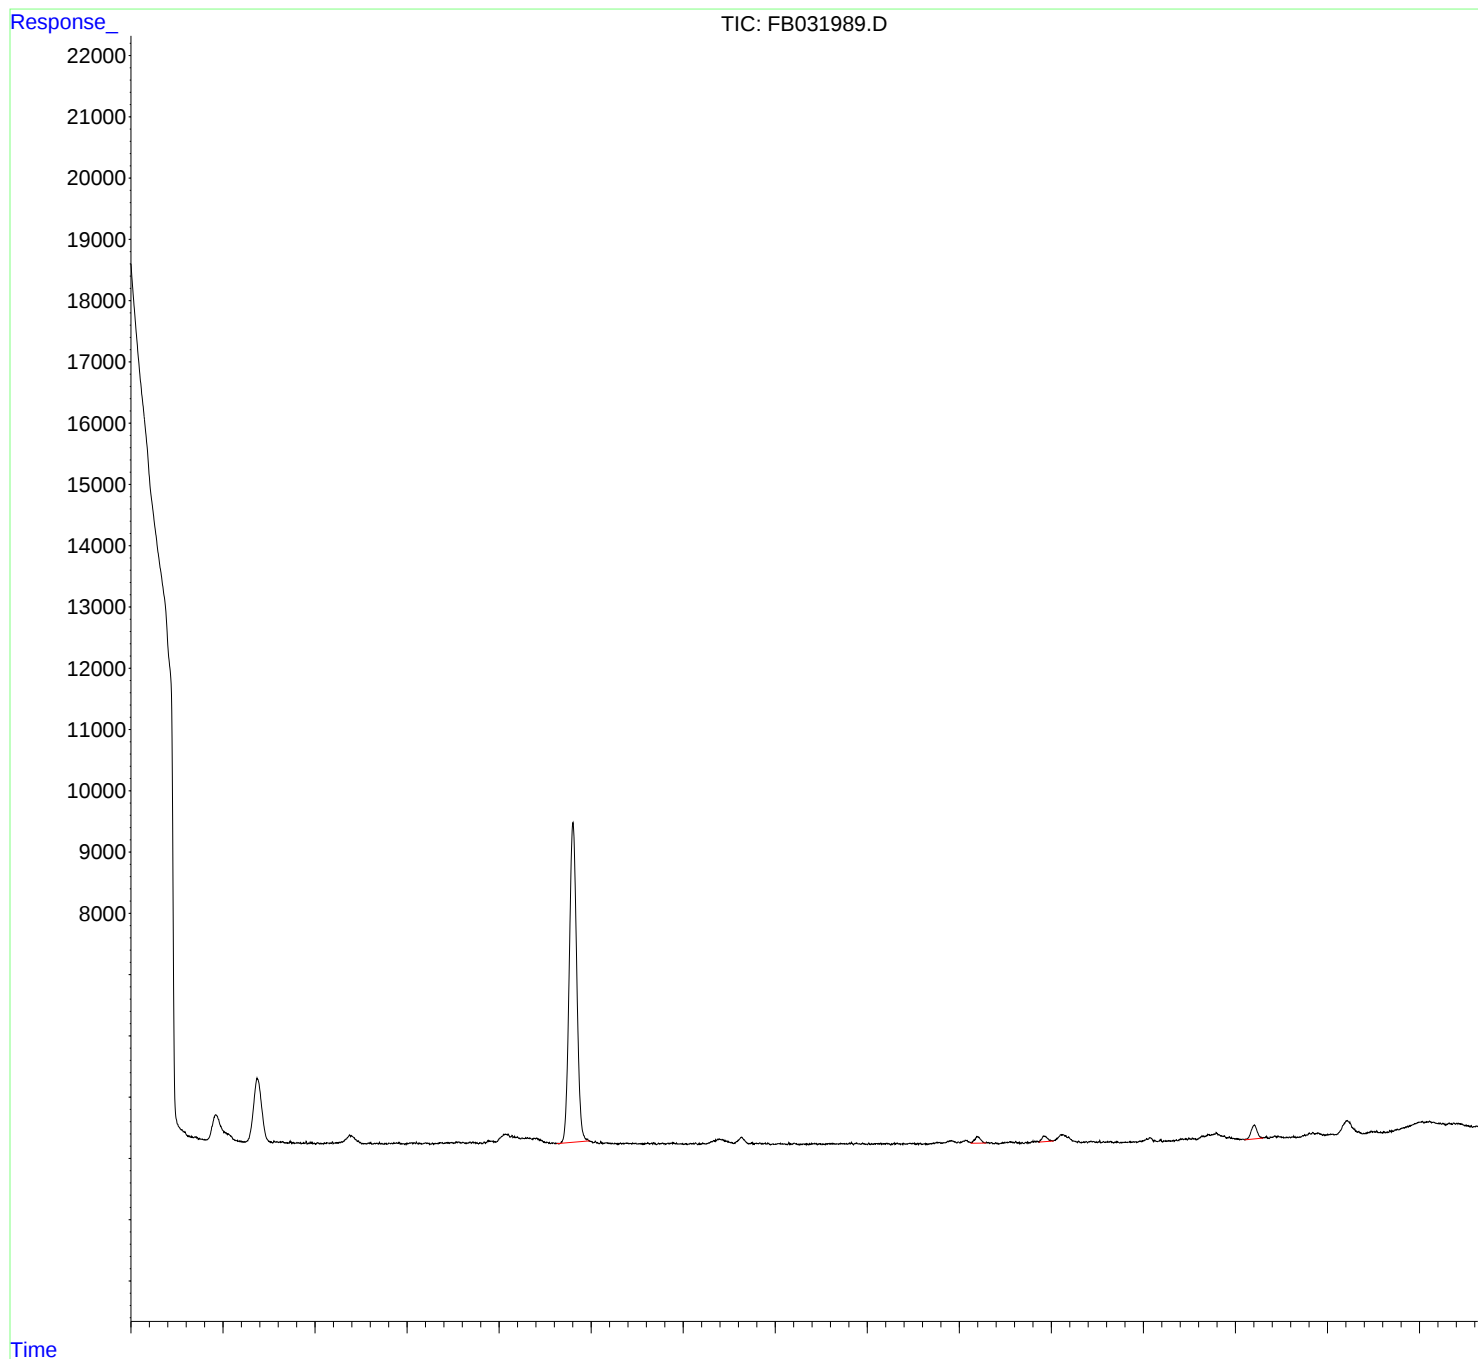


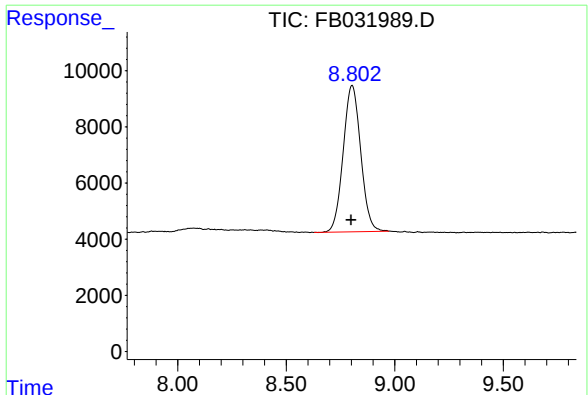

#5 AAA-TFT


R.T.: 8.804 min
Delta R.T.: 0.006 min
Response: 292209
Conc: 18.94 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-62

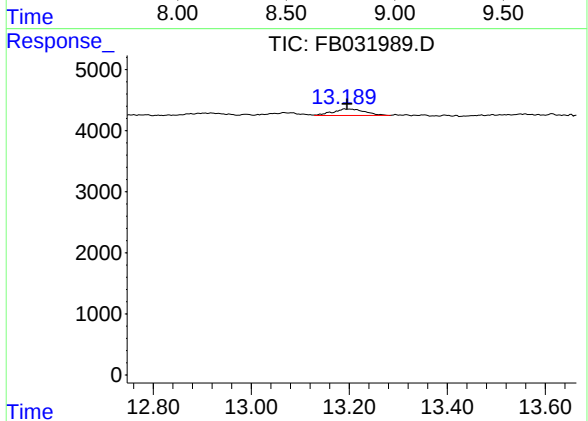


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: -0.004 min
Response: 4772
Conc: 0.15 ng/ml

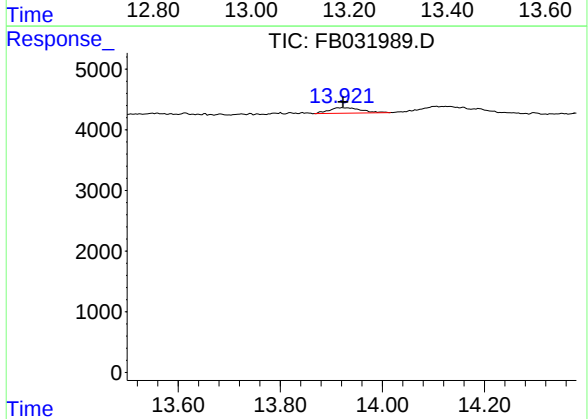

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: 0.000 min
Response: 3945
Conc: 0.13 ng/ml

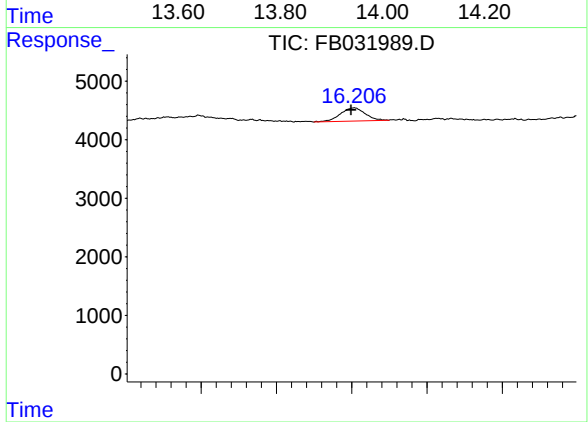

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.010 min
Response: 10283
Conc: 0.39 ng/ml